
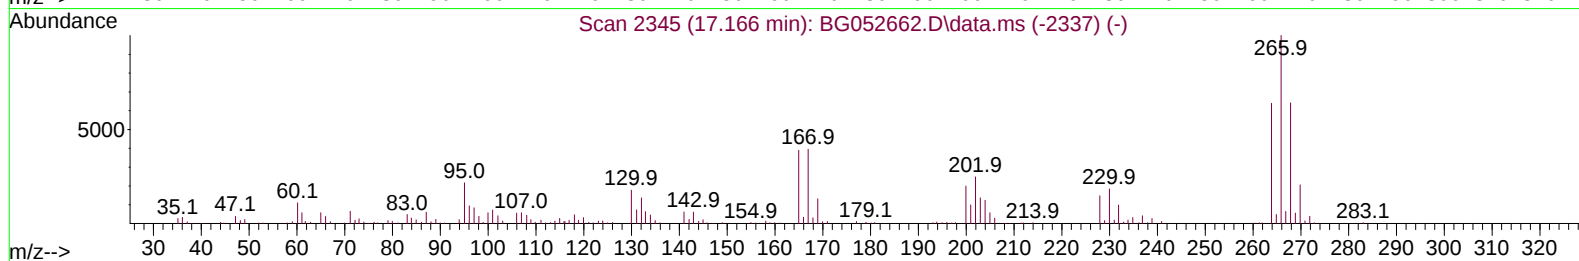
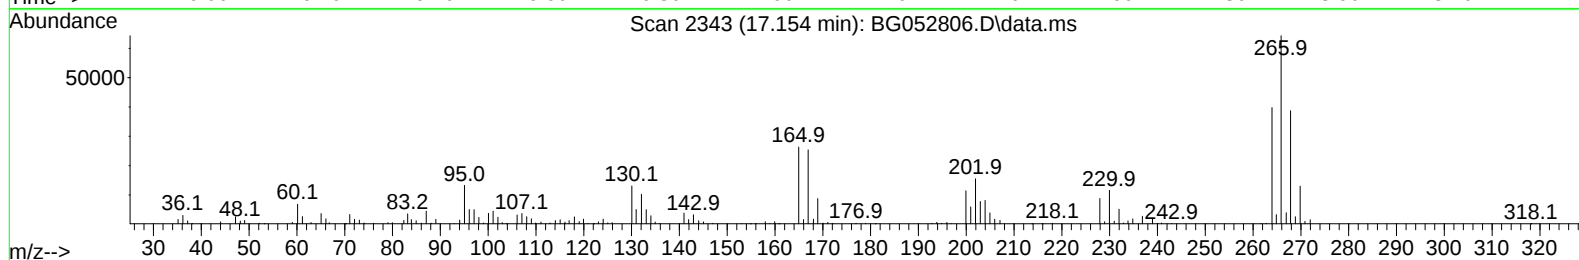


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032422\
Data File : BG052806.D
Acq On : 24 Mar 2022 12:49
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 24 16:55:46 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG031522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 24 16:48:57 2022
Response via : Initial Calibration

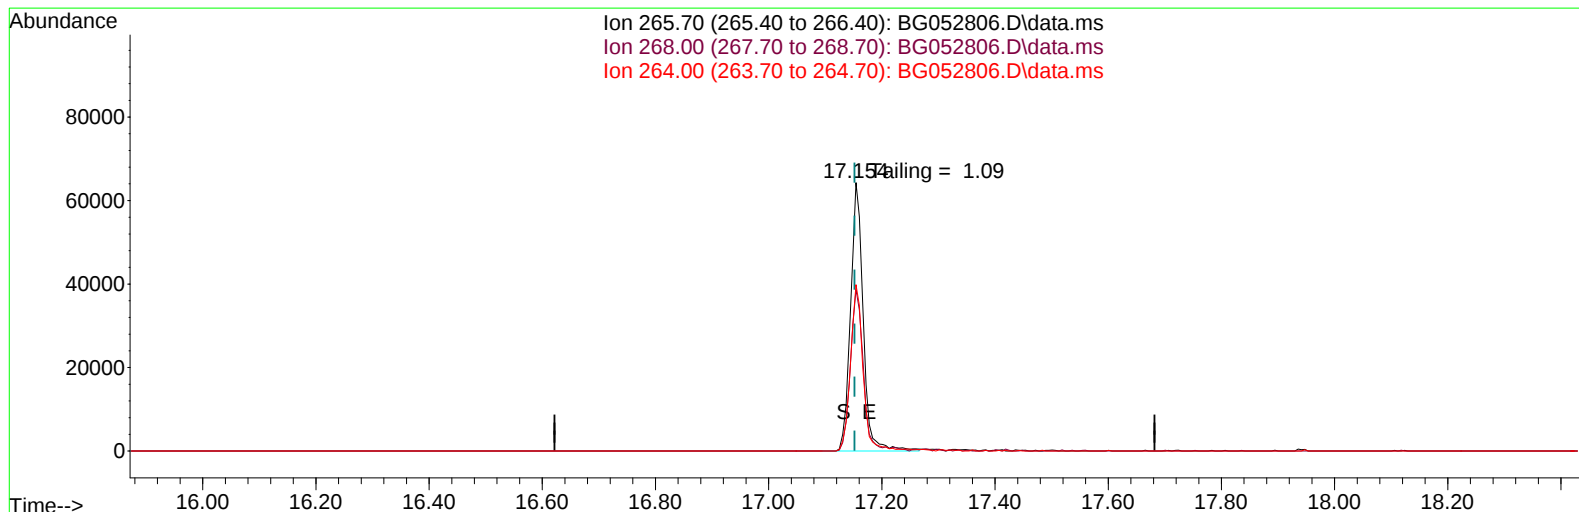

TIC: BG052806.D\data.ms

(70) Pentachlorophenol (C)




17.154min (+ 0.003) 113426.62 ng

response 100309

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	57.40	60.18
264.00	56.60	61.93
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032422\
Data File : BG052806.D
Acq On : 24 Mar 2022 12:49
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 24 16:55:46 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG031522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 24 16:48:57 2022
Response via : Initial Calibration

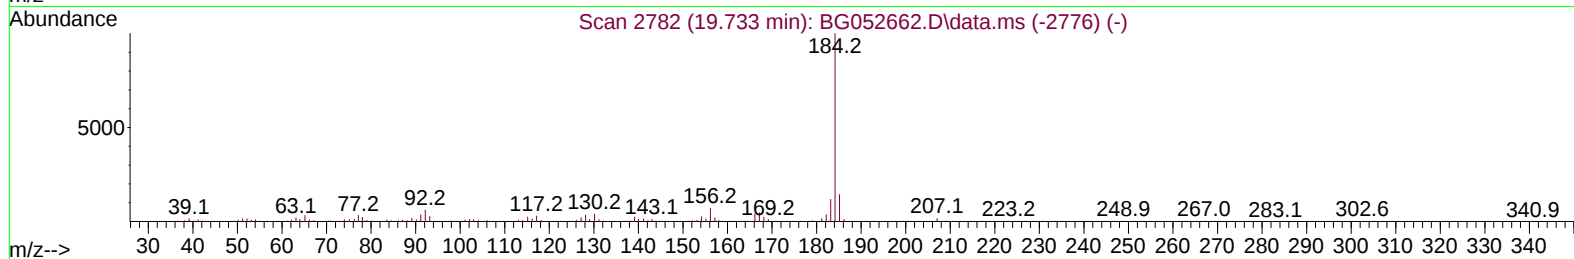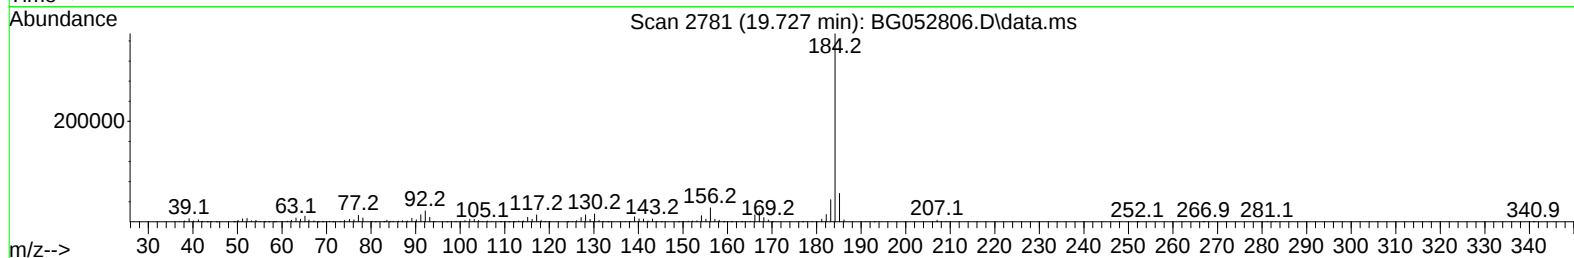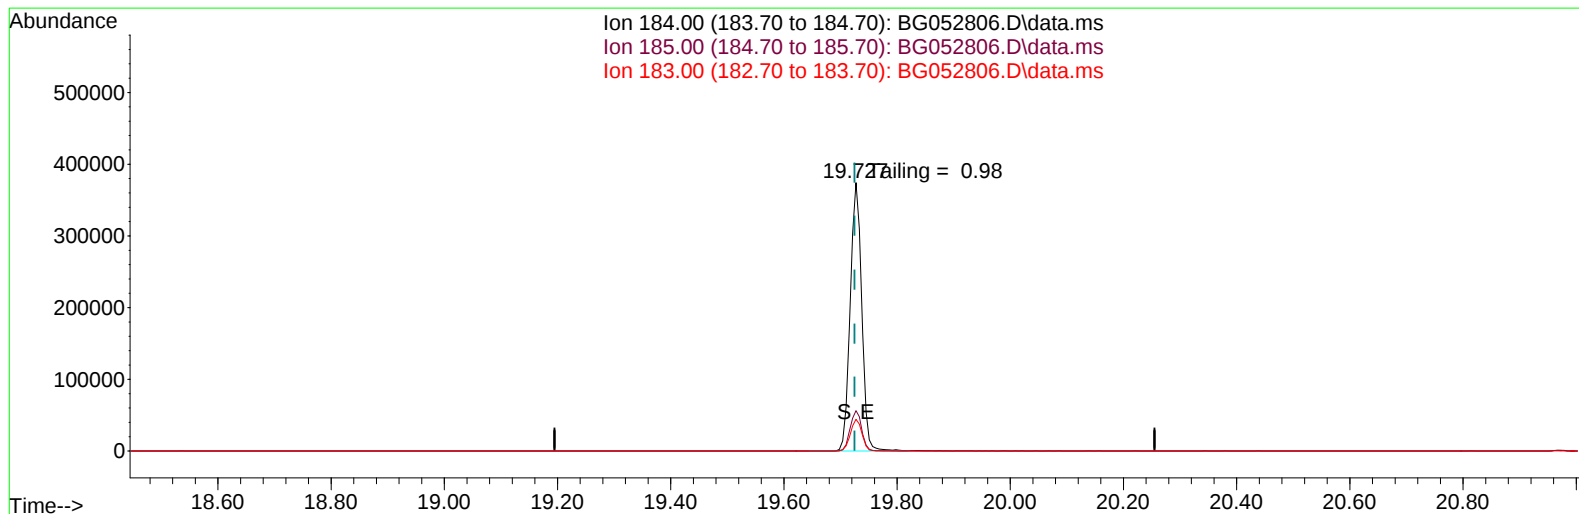

TIC: BG052806.D\data.ms

(77) Benzidine

19.727min (+ 0.003) 364654.13 ng

response 526689

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	15.06
183.00	11.80	11.81
0.00	0.00	0.00