

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032422\
 Data File : BG052808.D
 Acq On : 24 Mar 2022 14:26
 Operator : CG/JU
 Sample : PB143535BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 PB143535BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG031522.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG052808.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.699	386	393	403	rBV	718984	1151590	29.81%	8.278%
2	7.291	655	664	676	rBV	721940	1285558	33.28%	9.240%
3	8.142	802	809	816	rVB	129466	221554	5.74%	1.593%
4	9.300	997	1006	1016	rBV	452447	829371	21.47%	5.961%
5	10.956	1278	1288	1297	rBV	172183	311235	8.06%	2.237%
6	13.388	1694	1702	1709	rBV	1233455	1968285	50.95%	14.148%
7	14.763	1929	1936	1945	rBV	289351	461676	11.95%	3.318%
8	16.243	2182	2188	2199	rBV	1066470	1677521	43.42%	12.058%
9	17.506	2396	2403	2410	rBV	418276	636168	16.47%	4.573%
10	20.109	2840	2846	2852	rBV	2887979	3863170	100.00%	27.768%
11	21.789	3126	3132	3140	rVB	444108	776379	20.10%	5.581%
12	25.108	3687	3697	3709	rVB2	241681	729719	18.89%	5.245%




Sum of corrected areas: 13912226

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032422\
Data File : BG052808.D
Acq On : 24 Mar 2022 14:26
Operator : CG/JU
Sample : PB143535BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB143535BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG031522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

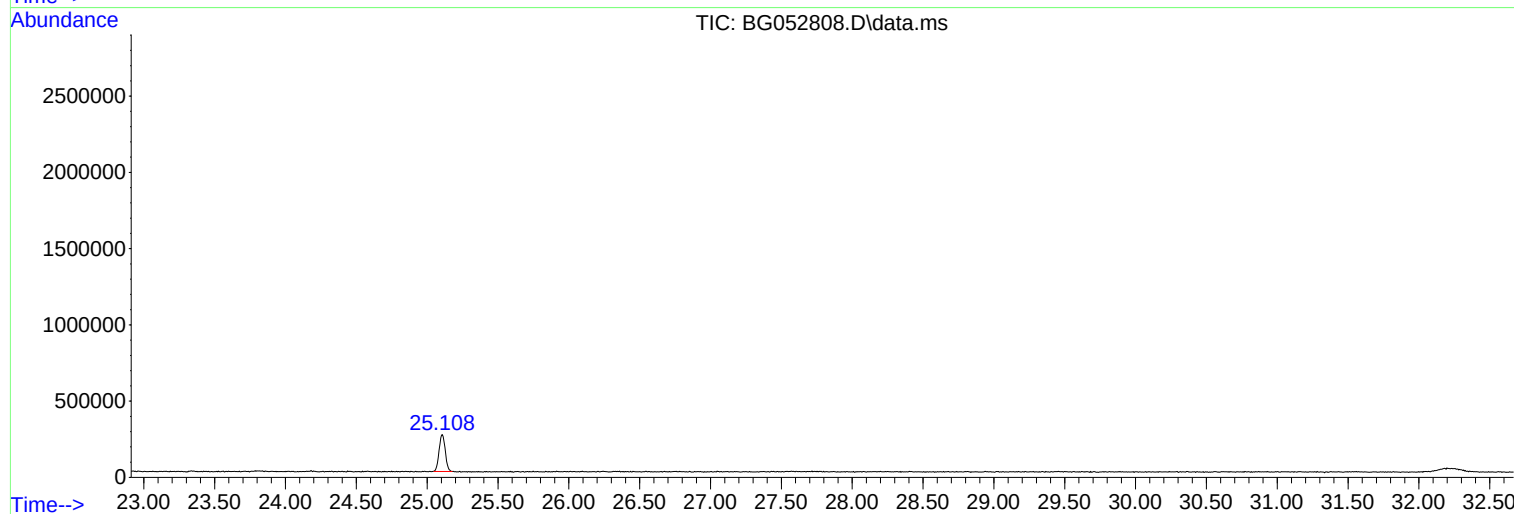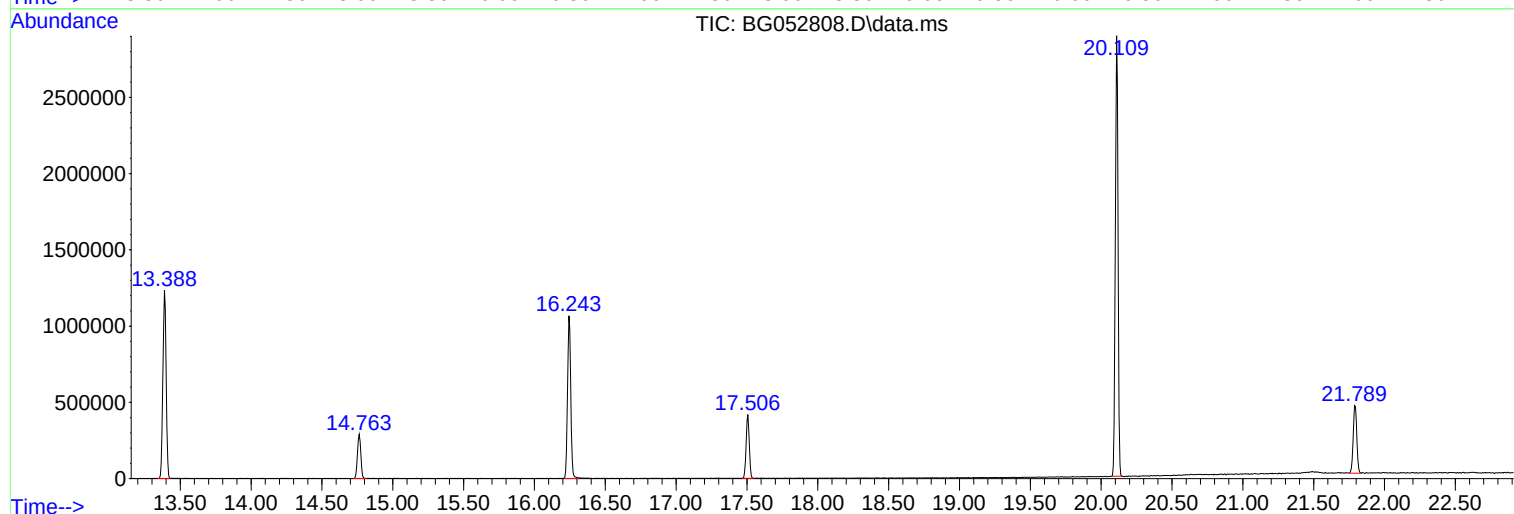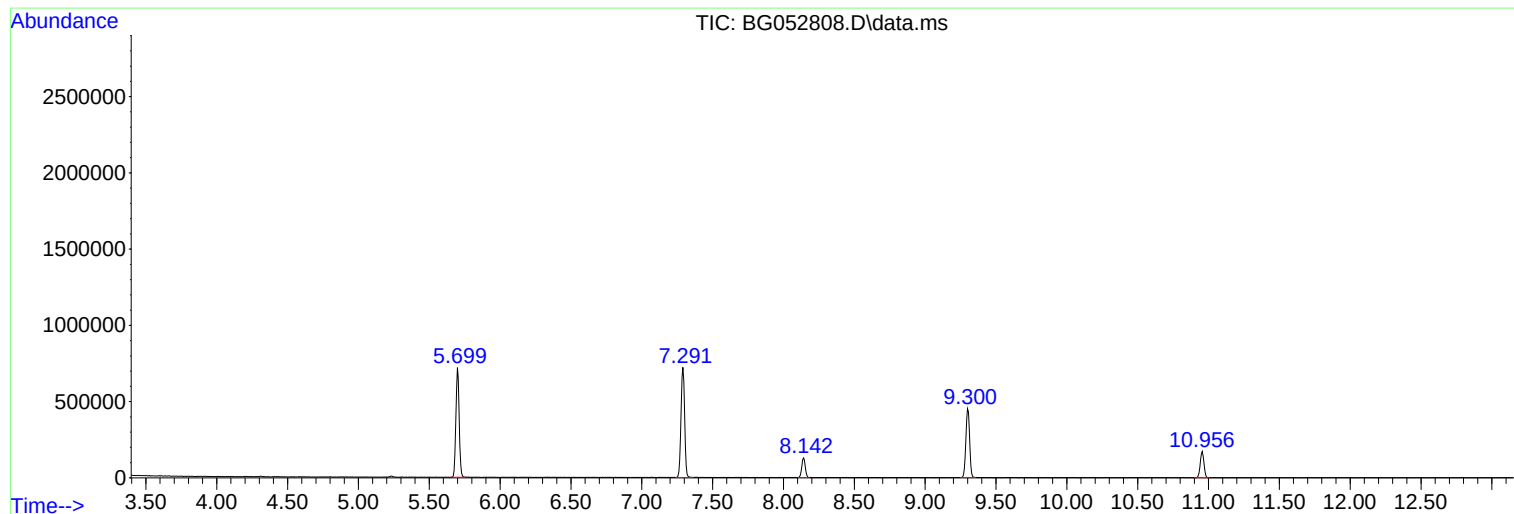

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032422\
Data File : BG052808.D
Acq On : 24 Mar 2022 14:26
Operator : CG/JU
Sample : PB143535BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB143535BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG031522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032422\
Data File : BG052808.D
Acq On : 24 Mar 2022 14:26
Operator : CG/JU
Sample : PB143535BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB143535BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG031522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------