

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032422\
 Data File : BG052815.D
 Acq On : 24 Mar 2022 19:00
 Operator : CG/JU
 Sample : N2090-06
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 MW-50D

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG031522.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG052815.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.697	383	393	402	rBV	265936	428558	12.77%	3.815%
2	7.289	656	664	671	rBV	179648	320796	9.56%	2.856%
3	8.141	803	809	815	rBV	92970	156258	4.65%	1.391%
4	9.298	998	1006	1016	rBV	406718	728606	21.70%	6.486%
5	10.955	1280	1288	1294	rBV	131406	233434	6.95%	2.078%
6	13.387	1695	1702	1713	rBV	1116540	1753837	52.24%	15.613%
7	14.550	1894	1900	1906	rBV	21669	35924	1.07%	0.320%
8	14.761	1930	1936	1943	rVB	236040	376000	11.20%	3.347%
9	15.102	1988	1994	2001	rBV2	75095	118425	3.53%	1.054%
10	16.248	2182	2189	2202	rBV	1145729	1823228	54.31%	16.231%
11	17.505	2397	2403	2409	rBV	348746	539683	16.08%	4.804%
12	18.386	2549	2553	2561	rBV9	18152	35863	1.07%	0.319%
13	20.107	2840	2846	2857	rVB	2436017	3357190	100.00%	29.886%
14	21.423	3067	3070	3077	rVB7	29865	51490	1.53%	0.458%
15	21.793	3126	3133	3141	rVB	375839	642279	19.13%	5.718%
16	25.106	3687	3697	3709	rVB2	208366	631636	18.81%	5.623%




Sum of corrected areas: 11233207

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032422\
Data File : BG052815.D
Acq On : 24 Mar 2022 19:00
Operator : CG/JU
Sample : N2090-06
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
MW-50D

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG031522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

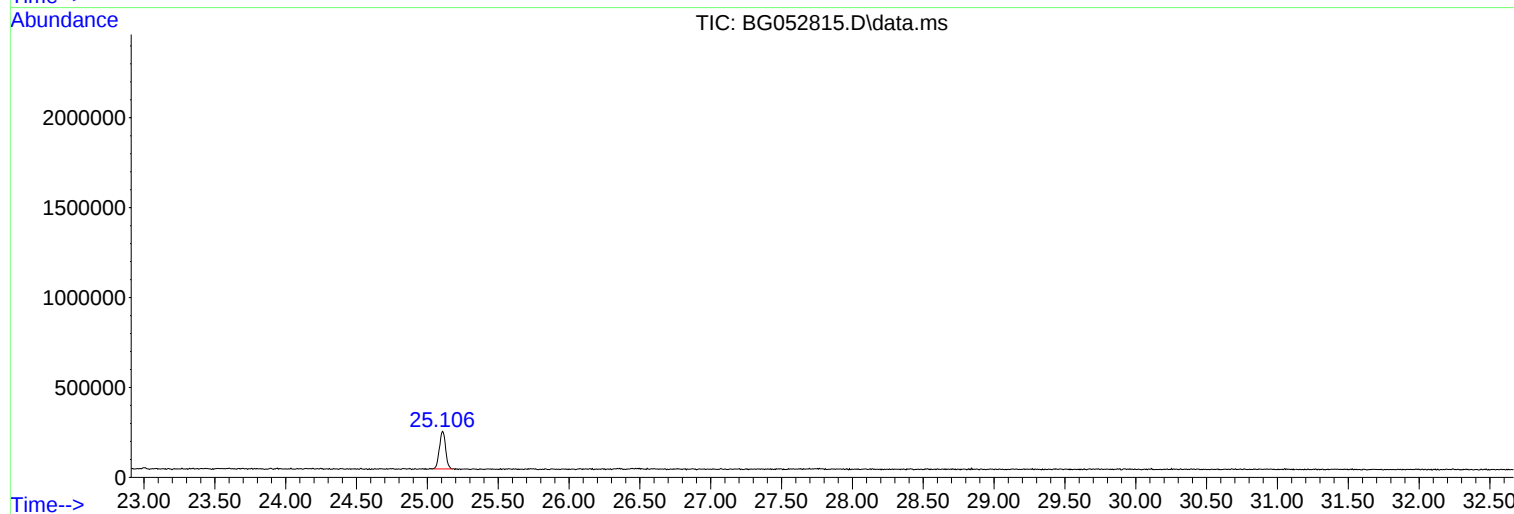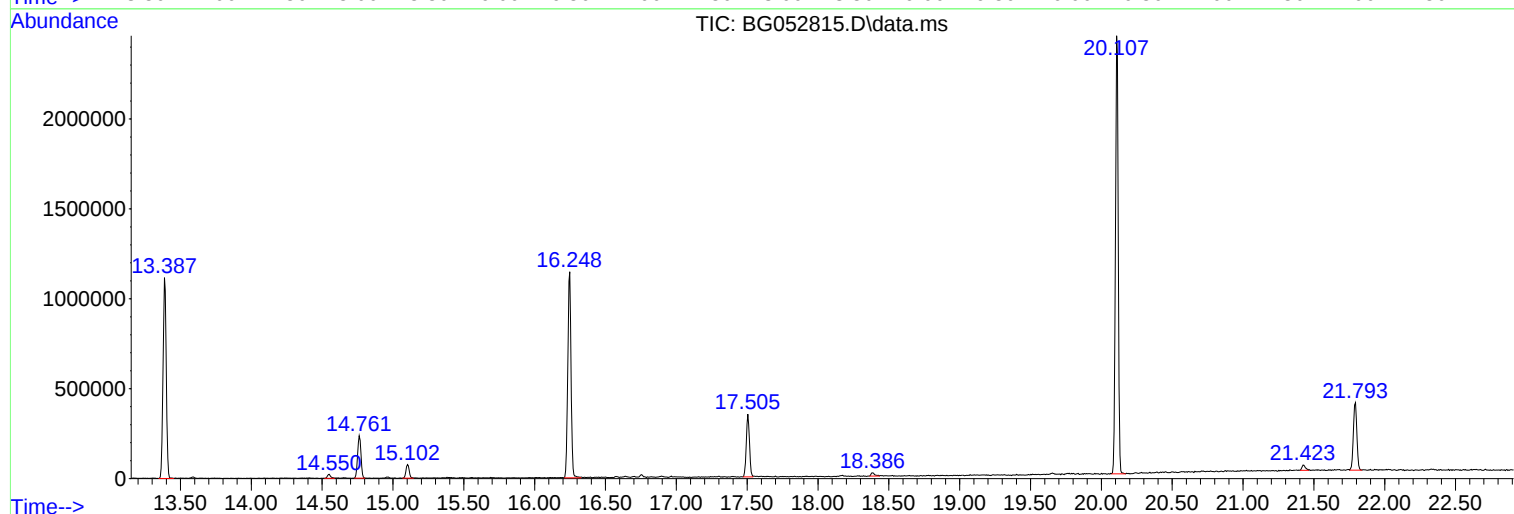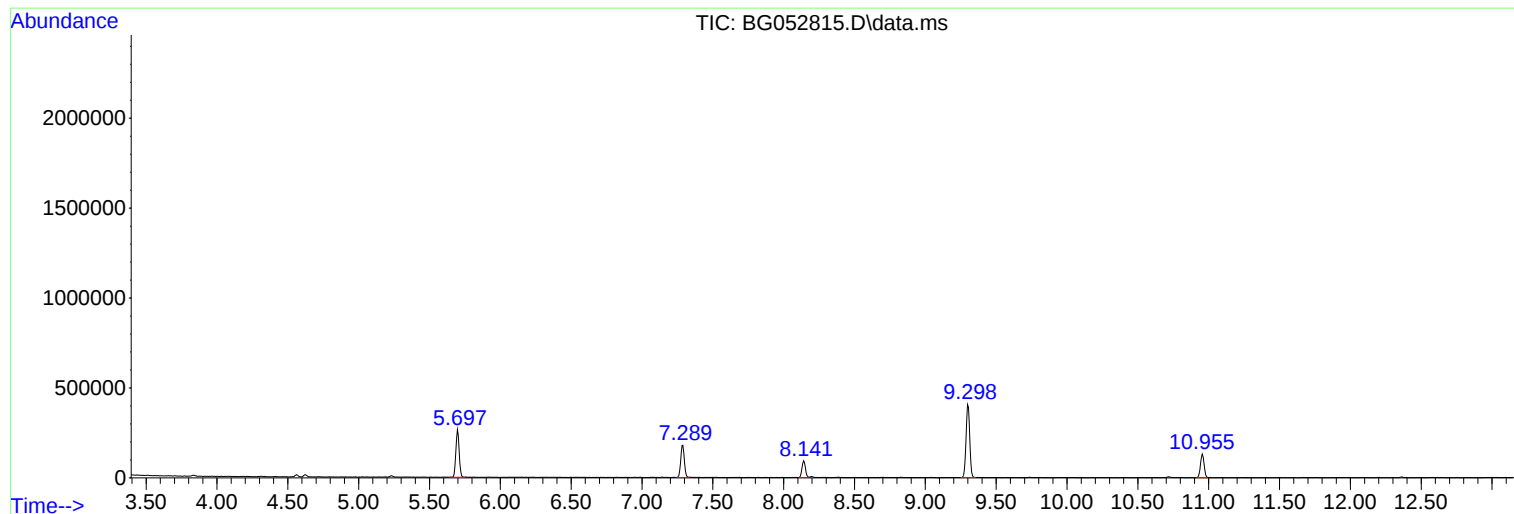

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032422\
Data File : BG052815.D
Acq On : 24 Mar 2022 19:00
Operator : CG/JU
Sample : N2090-06
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
MW-50D










Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG031522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown15.102 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
15.102	6.30 ng	118425	Acenaphthene-d10	14.761

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			1,1-Cyclopentanediacetamide	167	C9H13NO2	001075-89-4	16
2			1-Naphthaleneacetonitrile	167	C12H9N	000132-75-2	14
3			1-Pentanol, 4-amino-	103	C5H13NO	000927-55-9	14
4			2-Bornanone oxime	167	C10H17NO	013559-66-5	14
5			Benzeneethanamine, N-methyl-	135	C9H13N	000589-08-2	14

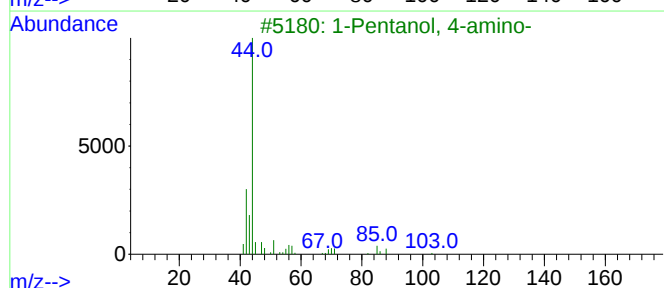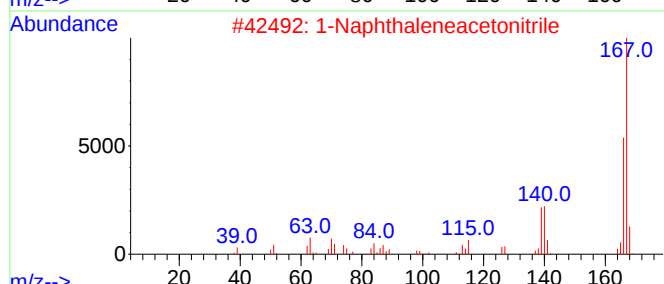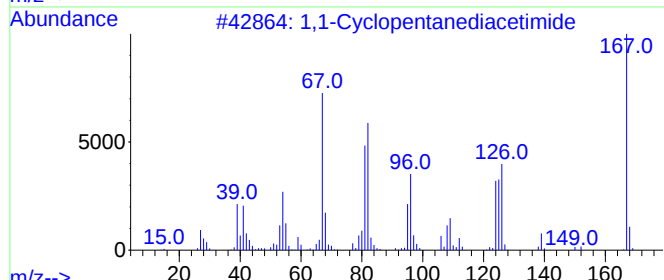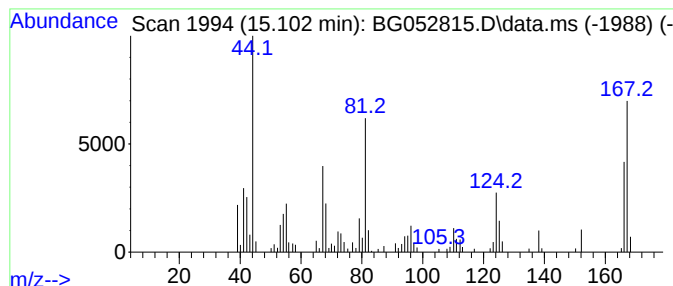

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032422\
Data File : BG052815.D
Acq On : 24 Mar 2022 19:00
Operator : CG/JU
Sample : N2090-06
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
MW-50D

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG031522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown15.102	15.102	6.3	ng	118425	3	14.761	376000	20.0