



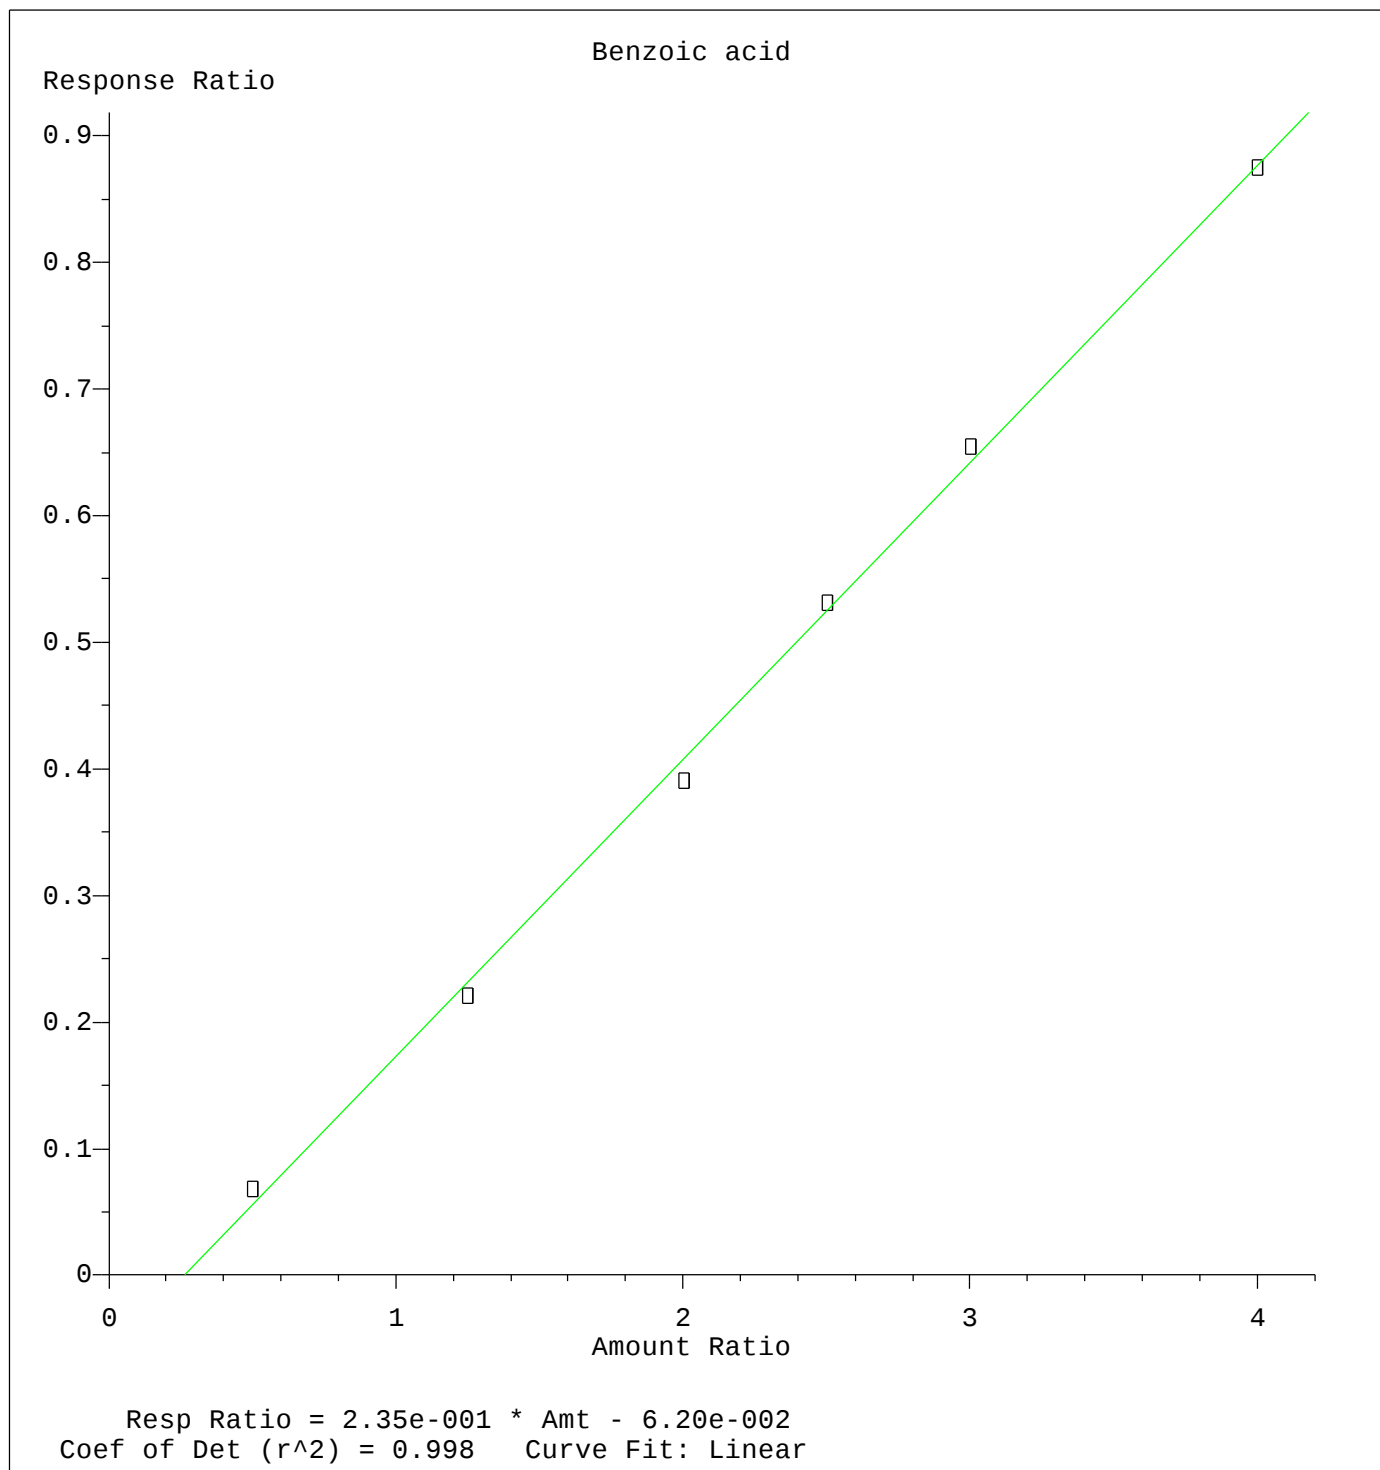

Method Name: Z:\HPCHEM1\BNA_G\METHODS\8270-BG032515.M
Calibration Table Last Updated: Thu Mar 26 15:24:59 2015

2,4-Dinitrophenol

Response Ratio

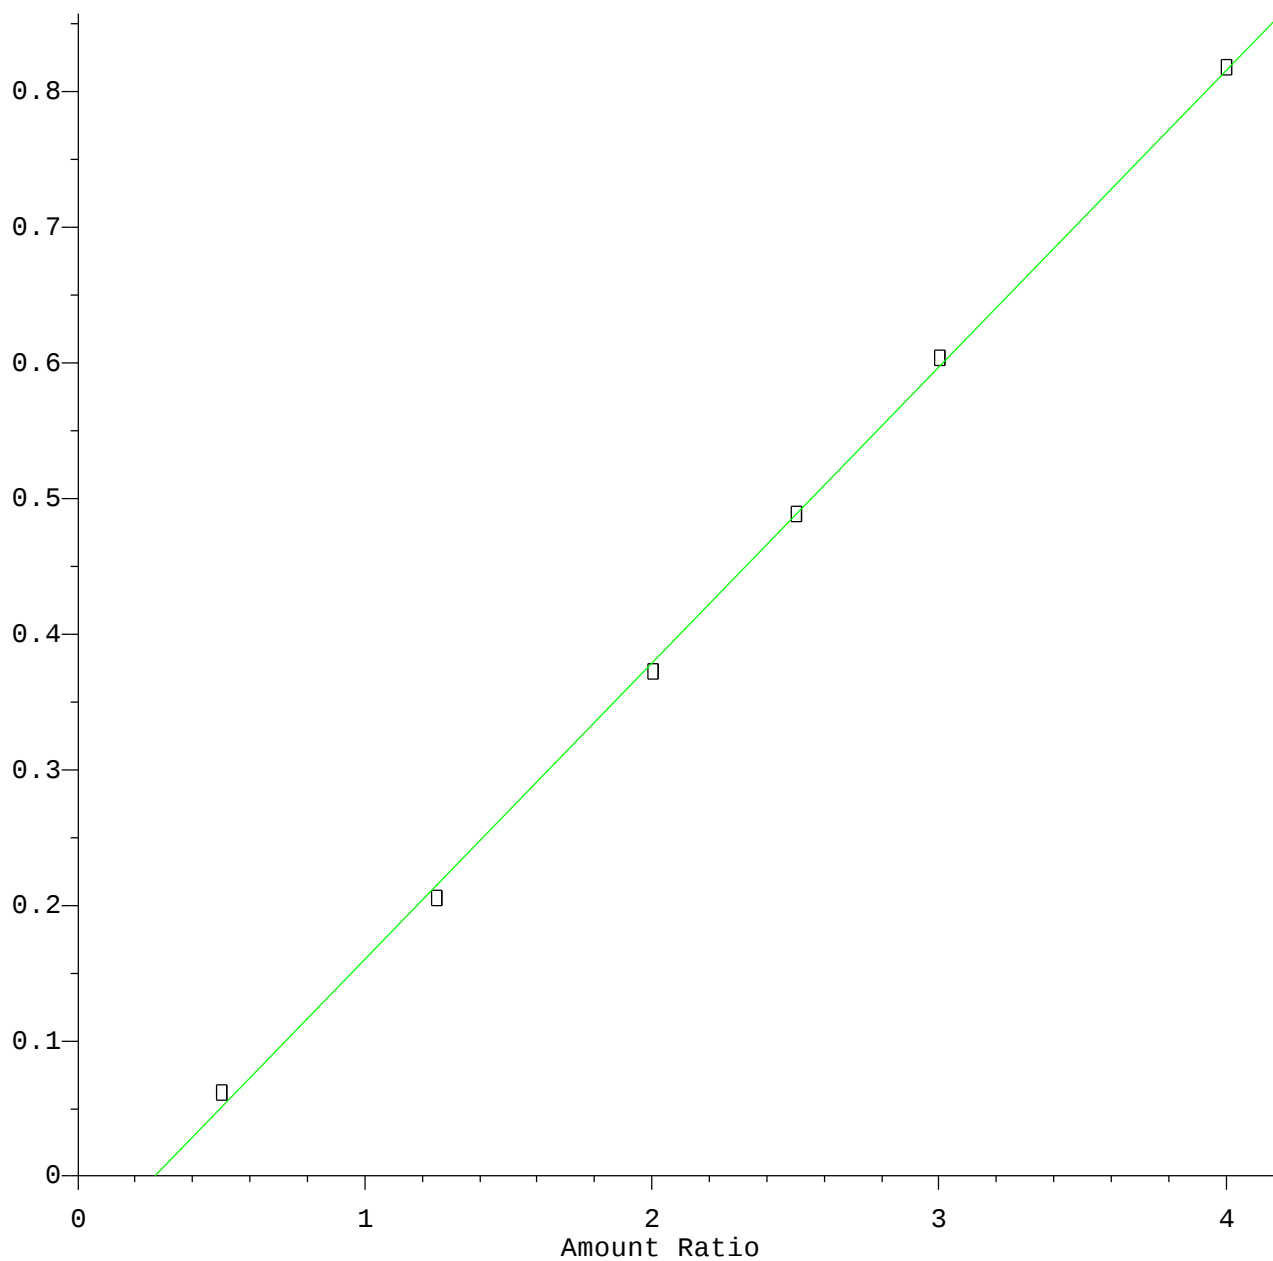

Resp Ratio = 2.19e-001 * Amt - 5.87e-002
Coef of Det (r²) = 0.999 Curve Fit: Linear

Method Name: Z:\HPCHEM1\BNA_G\METHODS\8270-BG032515.M
Calibration Table Last Updated: Thu Mar 26 15:24:59 2015