
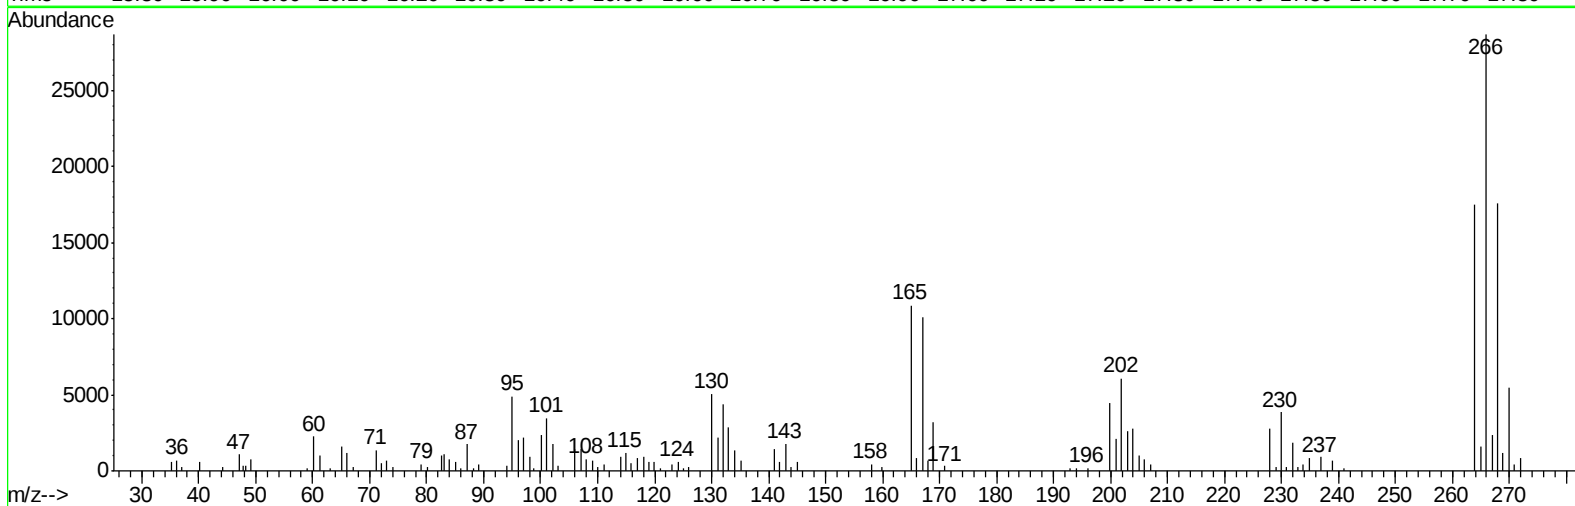


Data Path : Z:\HPCHEM1\BNA_G\Data\BG032515\
Data File : BG016116.D
Acq On : 25 Mar 2015 23:44
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 26 08:28:04 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG032515.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 26 02:10:27 2015
Response via : Initial Calibration

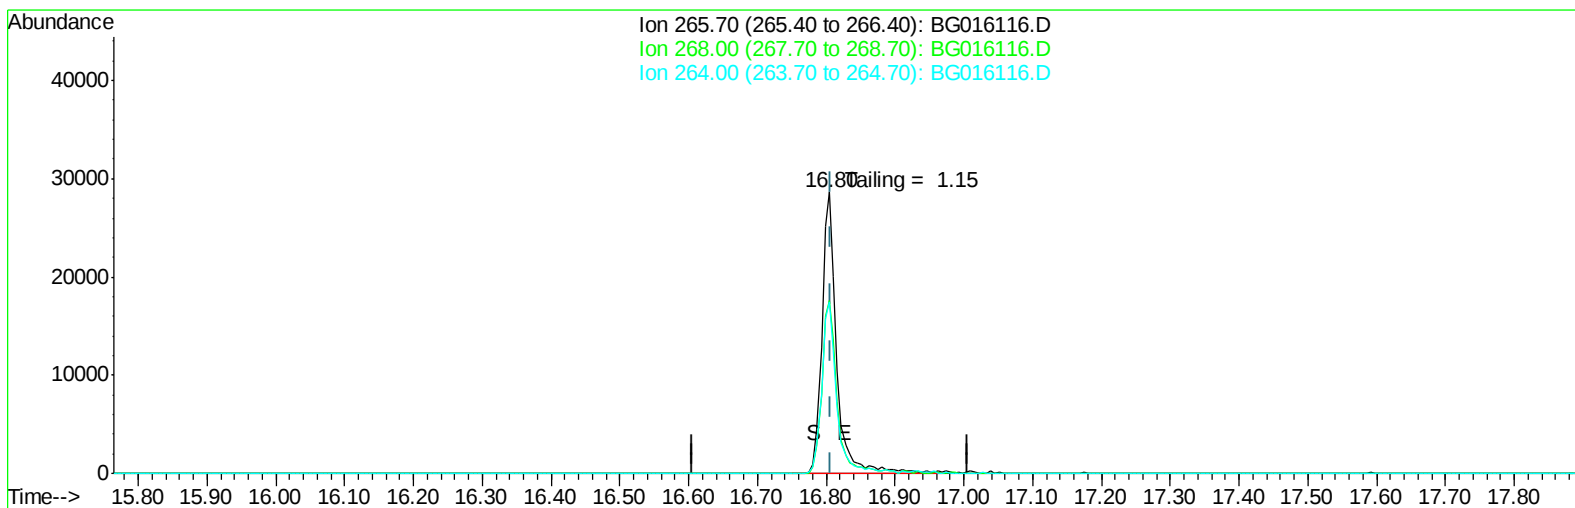

TIC: BG016116.D

(69) Pentachlorophenol (C)



16.804min (-0.002) 0.00ng

response 41972

Ion	Exp%	Act%
265.70	100	100
268.00	64.40	61.22
264.00	62.20	60.91
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_G\Data\BG032515\
Data File : BG016116.D
Acq On : 25 Mar 2015 23:44
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 26 08:28:04 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG032515.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 26 02:10:27 2015
Response via : Initial Calibration

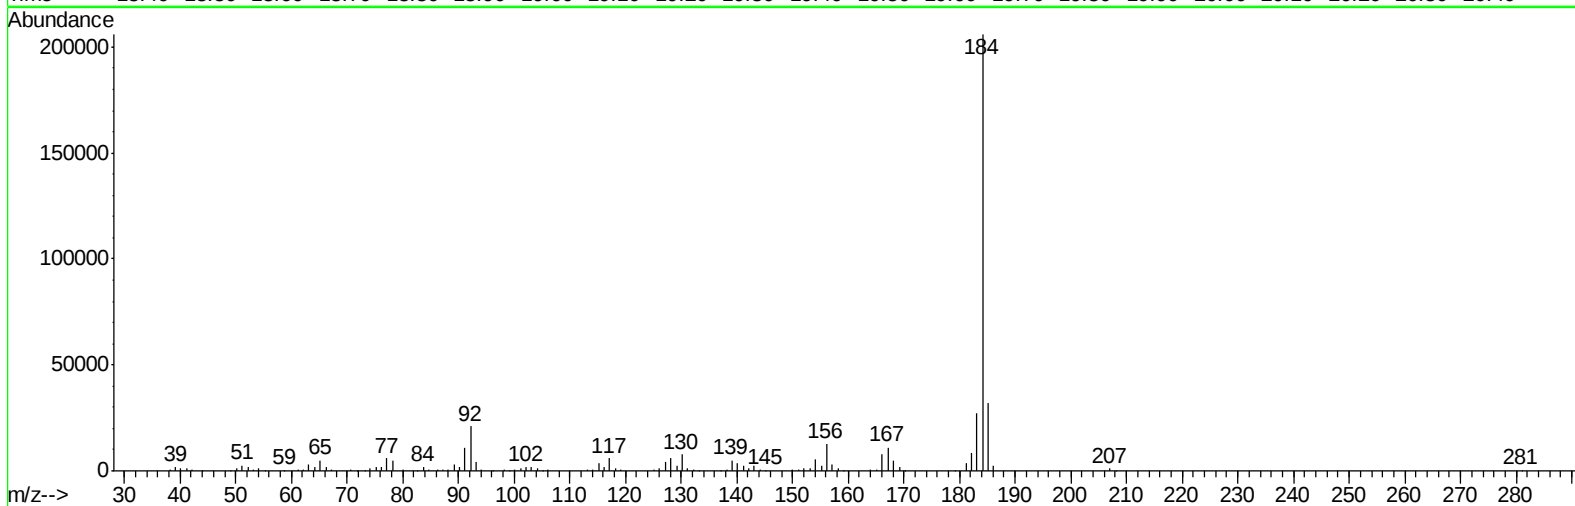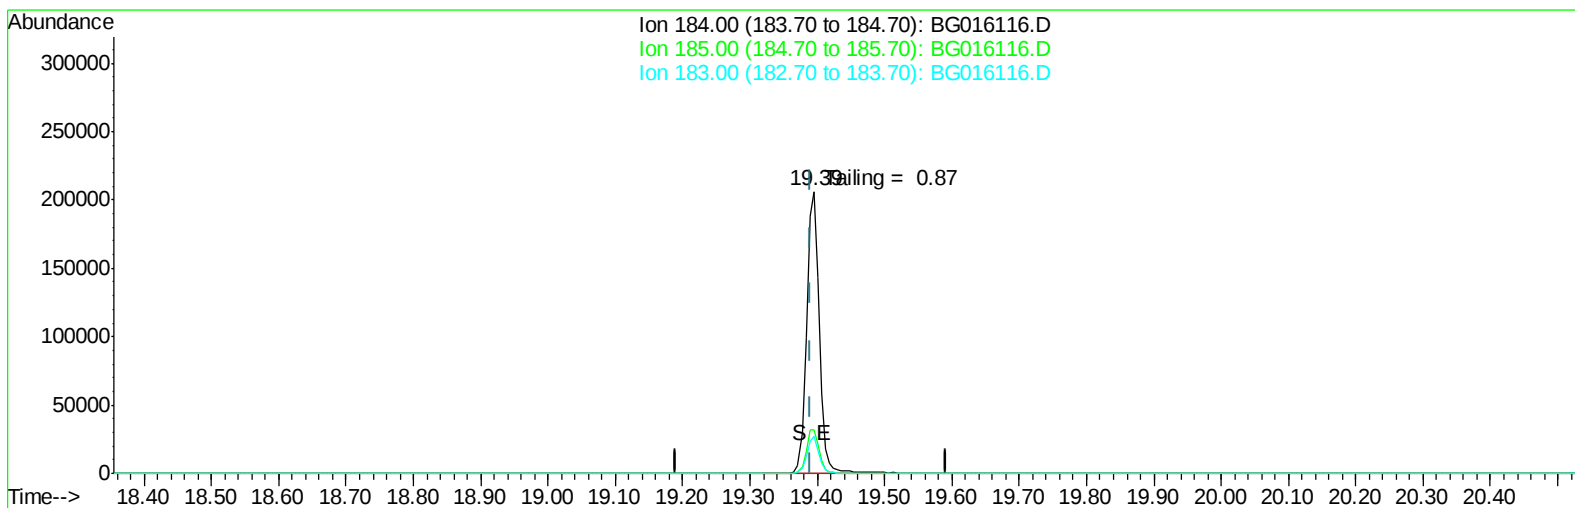

TIC: BG016116.D

(76) Benzidine

19.395min (+0.004) 84704.42ng

response 275205

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	15.67
183.00	12.80	13.08
0.00	0.00	0.00