

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG032515\
 Data File : BG016123.D
 Acq On : 26 Mar 2015 4:21
 Operator : TP/IZ
 Sample : PB82242BL
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 PB82242BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG032515.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.793	14	18	37	rVB	4770767	5864602	100.00%	24.754%
2	4.919	374	380	388	rVB	107930	150920	2.57%	0.637%
3	5.377	452	458	470	rVB	894462	1271927	21.69%	5.369%
4	6.958	719	727	736	rBV	867448	1334758	22.76%	5.634%
5	7.322	782	789	797	rBV	869726	1377459	23.49%	5.814%
6	7.792	859	869	876	rBV	199092	310653	5.30%	1.311%
7	8.109	917	923	932	rVB	649430	1043570	17.79%	4.405%
8	8.943	1058	1065	1076	rBV	491625	796897	13.59%	3.364%
9	10.576	1336	1343	1352	rBV	287404	465031	7.93%	1.963%
10	13.038	1756	1762	1769	rVB	1394316	2063621	35.19%	8.710%
11	14.412	1990	1996	2004	rBV2	444714	668598	11.40%	2.822%
12	15.899	2242	2249	2258	rBV	1120068	1552919	26.48%	6.555%
13	17.150	2456	2462	2469	rBV2	613012	881605	15.03%	3.721%
14	19.776	2903	2909	2922	rBV	2969031	3683299	62.81%	15.547%
15	21.321	3166	3172	3183	rBV	906924	1090176	18.59%	4.602%
16	23.606	3553	3561	3574	rBV	550302	1047432	17.86%	4.421%
17	25.315	3839	3852	3853	rBV	25936	88129	1.50%	0.372%


Sum of corrected areas: 23691596

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG032515\
Data File : BG016123.D
Acq On : 26 Mar 2015 4:21
Operator : TP/IZ
Sample : PB82242BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB82242BL

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG032515.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

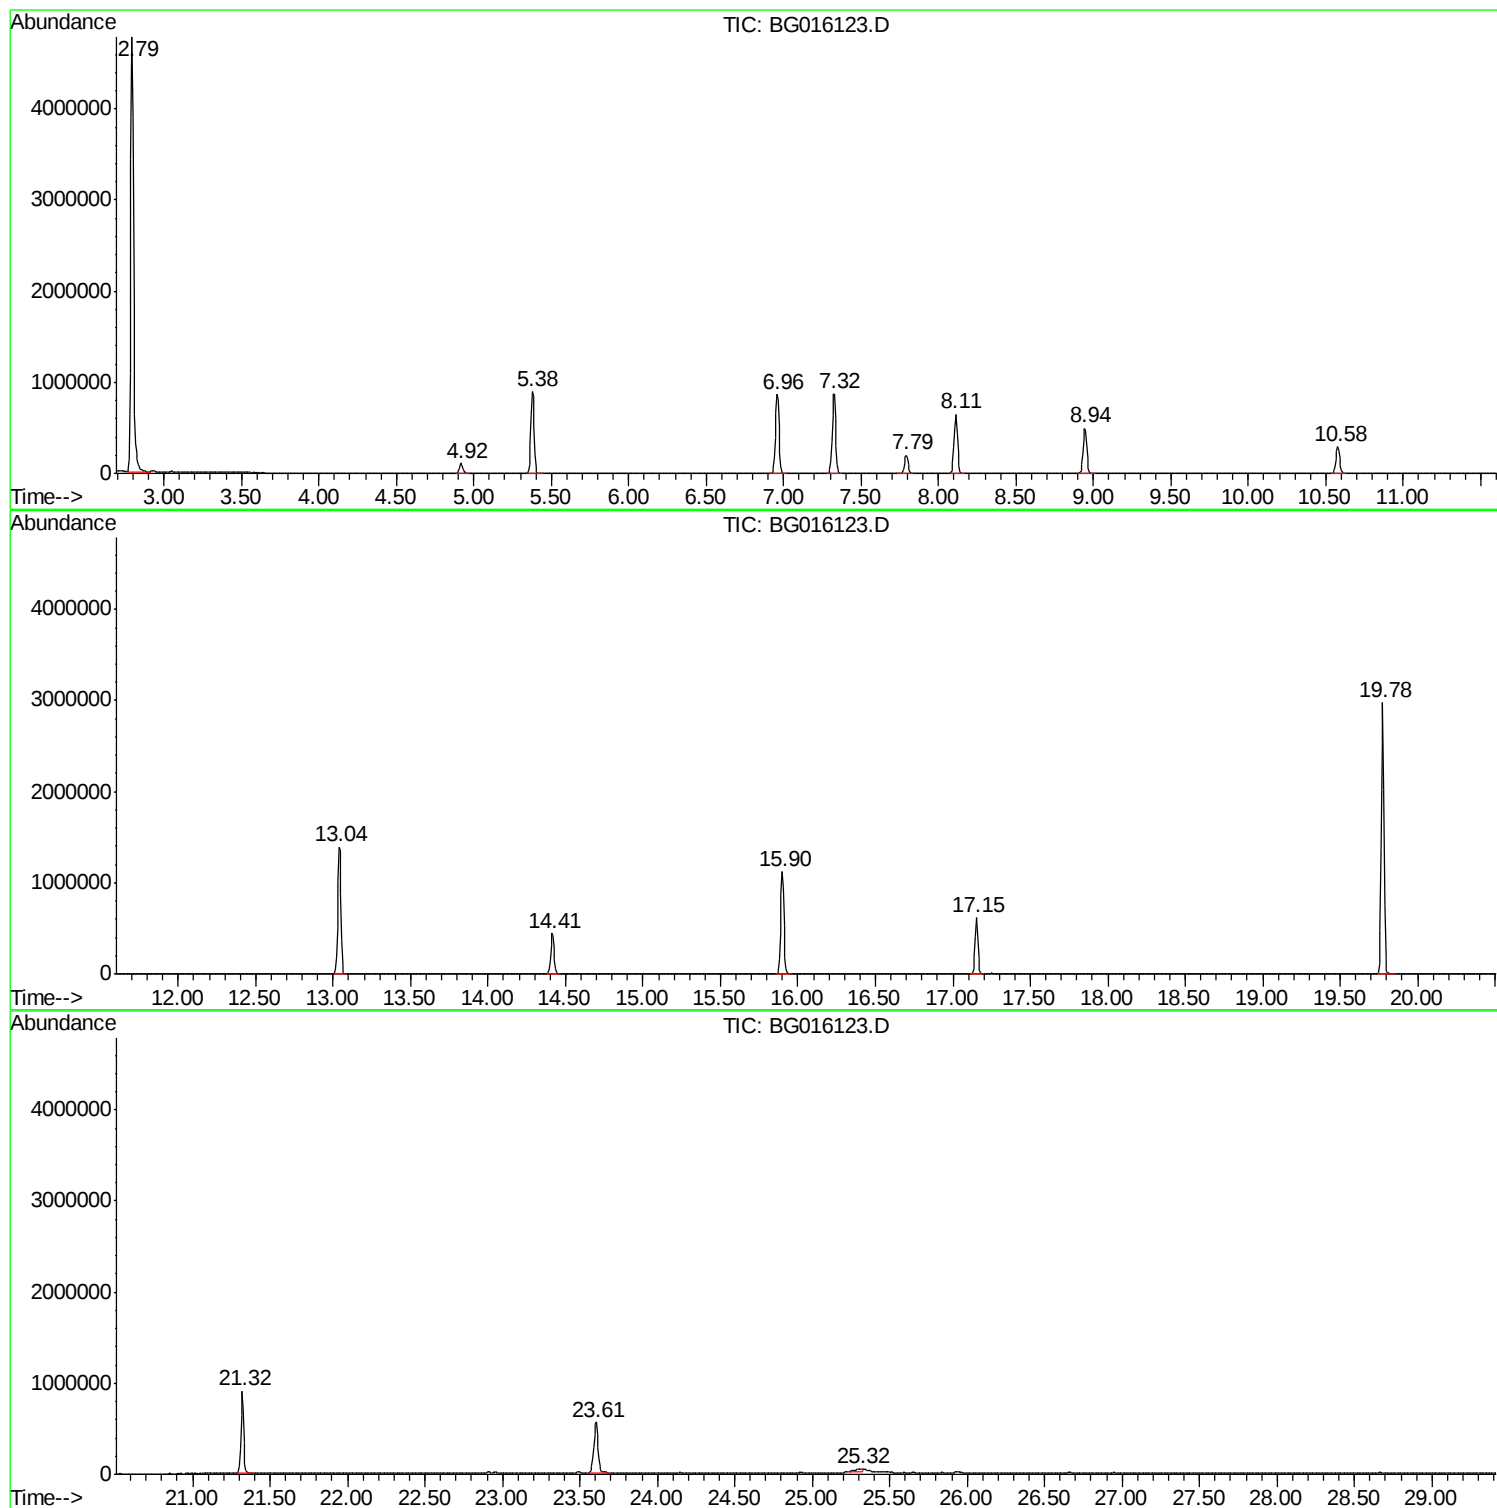

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG032515\
Data File : BG016123.D
Acq On : 26 Mar 2015 4:21
Operator : TP/IZ
Sample : PB82242BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampled :
PB82242BL










Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG032515.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 4

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.92	9.72 ng	150920	1,4-Dichlorobenzene-d4	7.79

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	53
2		(+)-4-Amino-4,5-dihydro-2(3H)-f...	101	C4H7NO2	016504-58-8	43
3		1,8-Nonanediol, 8-methyl-	174	C10H22O2	054725-73-4	23
4		Acetic acid, cyano-, 1,1-dimethy...	141	C7H11NO2	001116-98-9	12
5		Acetone	58	C3H6O	000067-64-1	9

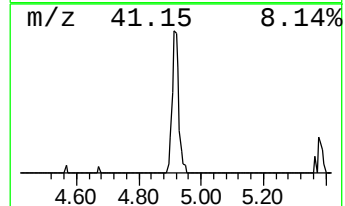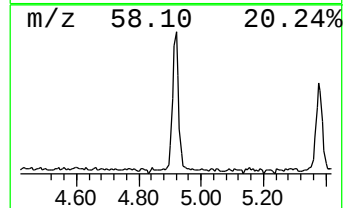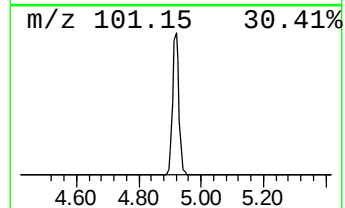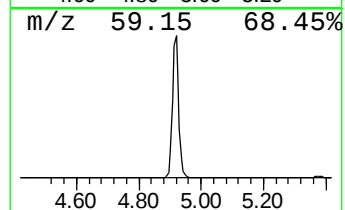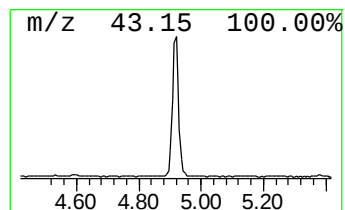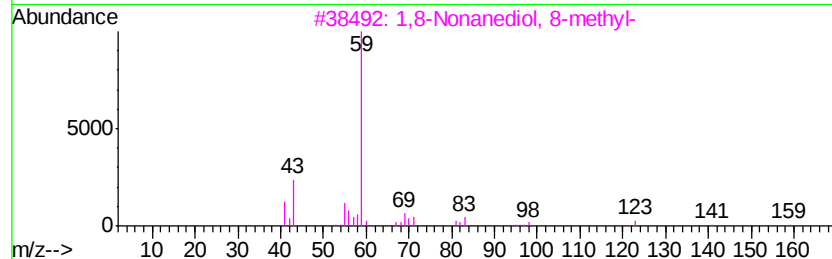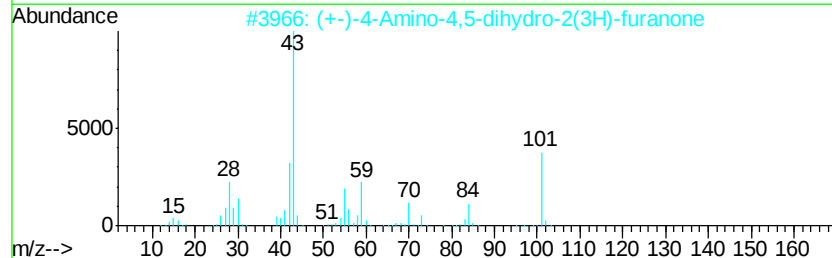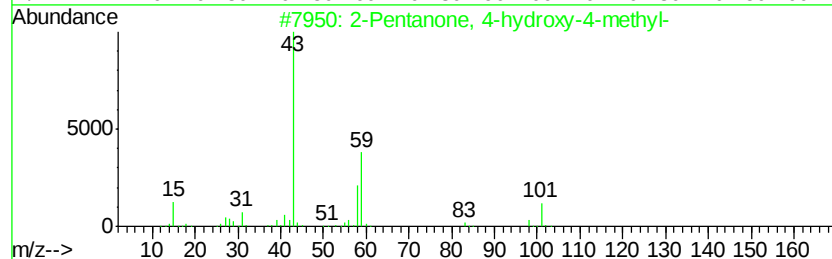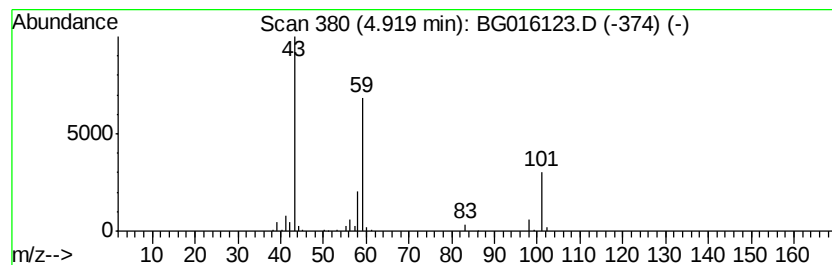

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG032515\
Data File : BG016123.D
Acq On : 26 Mar 2015 4:21
Operator : TP/IZ
Sample : PB82242BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB82242BL










Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG032515.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 3 unknown7.32 Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.32	88.68 ng	1377460	1,4-Dichlorobenzene-d4	7.79

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	38
2		(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	35
3		Tranylcypromine-propionyl	189	C12H15NO	1000123-86-3	12
4		4-Chloro-2-fluoro-pyrimidine	132	C4H2ClFN2	051422-00-5	9
5		4-Chloro-6-fluoro-pyrimidine	132	C4H2ClFN2	051422-01-6	9

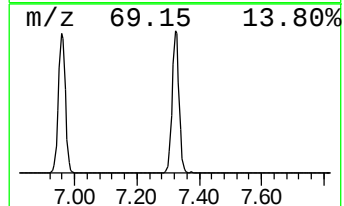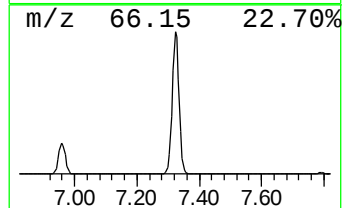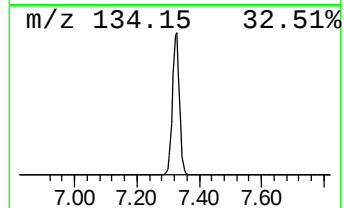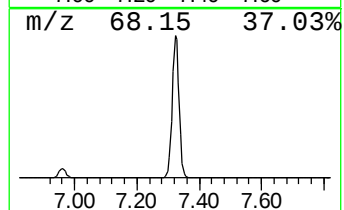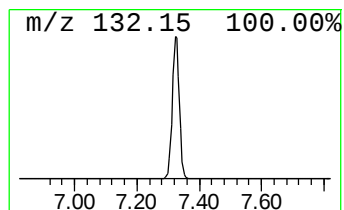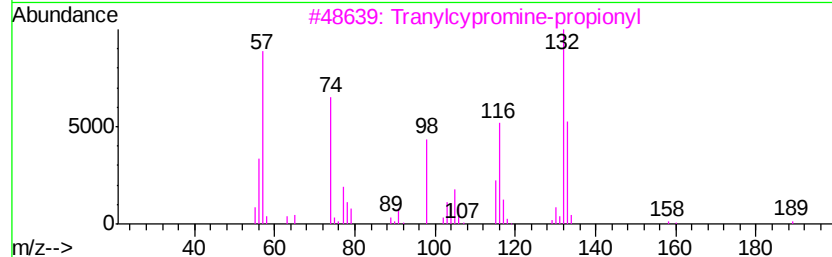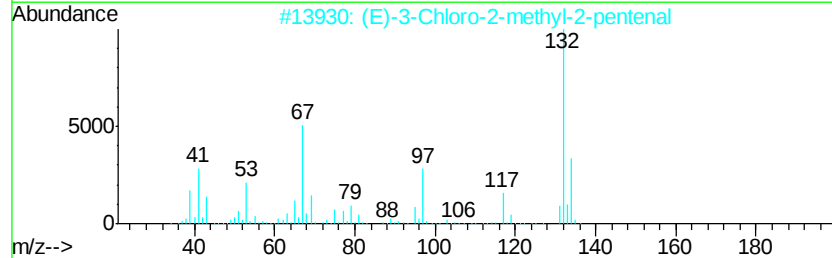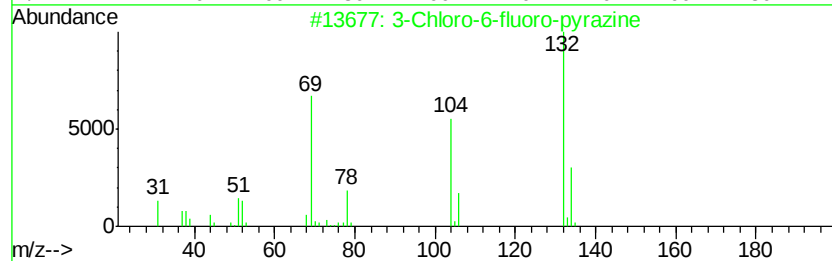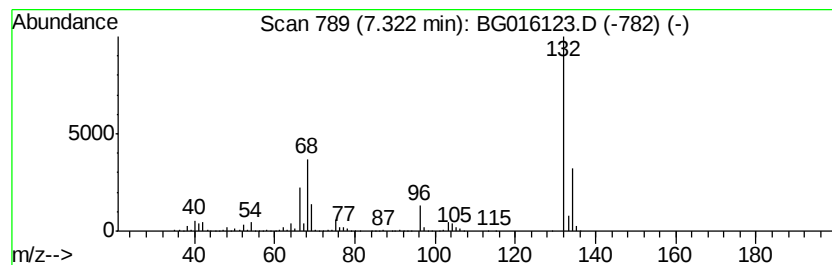

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG032515\
Data File : BG016123.D
Acq On : 26 Mar 2015 4:21
Operator : TP/IZ
Sample : PB82242BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB82242BL

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG032515.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-hy...	4.92	9.7	ng	150920	1	7.79	310653	20.0
unknown7.32	7.32	88.7	ng	1377460	1	7.79	310653	20.0