


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG032515\
 Data File : BG016116.D
 Acq On : 25 Mar 2015 23:44
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG032515.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Mar 26 15:24:59 2015

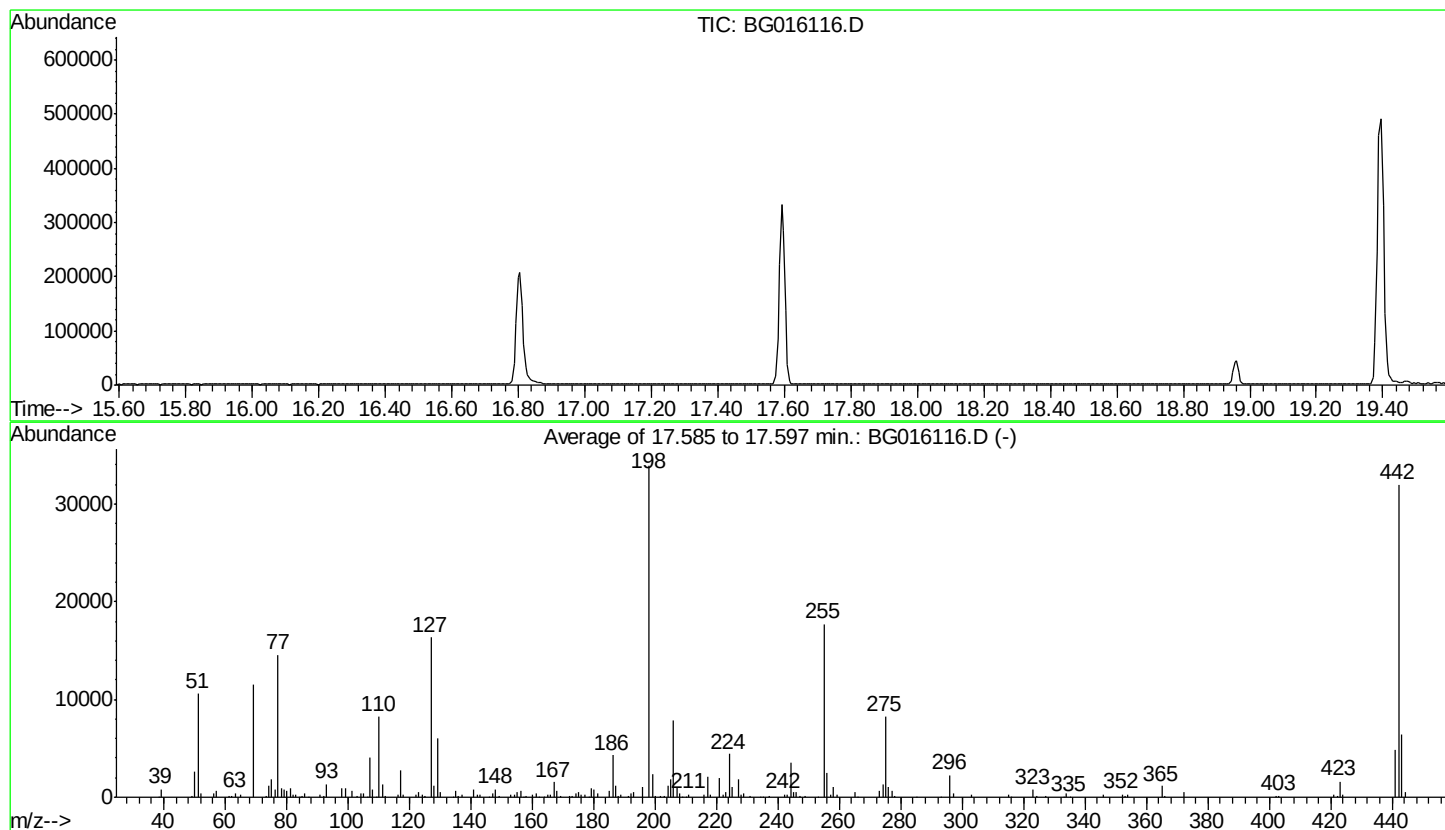

AutoFind: Scans 2536, 2537, 2538; Background Corrected with Scan 2530

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.1	10554	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	34.1	11583	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	48.2	16343	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	33933	PASS
199	198	5	9	7.1	2396	PASS
275	198	10	60	24.1	8193	PASS
365	198	1	100	3.3	1133	PASS
441	442	0.01	24	15.3	4899	PASS
442	198	50	100	94.3	32005	PASS
443	442	15	24	20.1	6419	PASS