

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG032516\
 Data File : BG021515.D
 Acq On : 25 Mar 2016 15:39
 Operator : UM/SJ
 Sample : H1909-15
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 A4T49

Quant Time: Mar 25 23:31:03 2016
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG031616.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Mar 25 23:28:37 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.06	152	17698	20.00	ng/ul	0.00
18) Naphthalene-d8	10.87	136	87744	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.68	164	56485	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.42	188	128057	20.00	ng/ul	0.00
78) Chrysene-d12	21.68	240	141347	20.00	ng/ul	0.00
86) Perylene-d12	24.90	264	139383	20.00	ng/ul	0.03

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.47	96	1205	3.05	ng/uL	0.00
5) Phenol-d5	7.34	99	28954	17.30	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.39	67	17788	17.95	ng/ul	0.00
9) 2-Chlorophenol-d4	7.64	132	22598	17.78	ng/ul	0.00
13) 4-Methylphenol-d8	8.85	113	21285	14.85	ng/ul	0.00
19) Nitrobenzene-d5	9.23	128	12264	18.63	ng/ul	0.00
22) 2-Nitrophenol-d4	9.96	143	13916	18.49	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.57	165	23328	17.34	ng/ul	0.00
29) 4-Chloroaniline-d4	11.01	131	30155	17.15	ng/ul	0.00
44) Dimethylphthalate-d6	14.08	166	80783	17.18	ng/ul	0.00
47) Acenaphthylene-d8	14.37	160	103948	17.93	ng/ul	0.00
52) 4-Nitrophenol-d4	15.10	143	8434	11.22	ng/ul	0.03
58) Fluorene-d10	15.67	176	73914	17.43	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.80	200	11509	13.60	ng/ul	0.00
71) Anthracene-d10	17.52	188	109179	17.40	ng/ul	0.00
79) Pyrene-d10	19.80	212	123757	18.78	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.68	264	129063	20.06	ng/ul	0.02


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
45) Dimethylphthalate	14.13	163	26027	5.33	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG032516\
Data File : BG021515.D
Acq On : 25 Mar 2016 15:39
Operator : UM/SJ
Sample : H1909-15
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
A4T49

Quant Time: Mar 25 23:31:03 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG031616.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Mar 25 23:28:37 2016
Response via : Initial Calibration

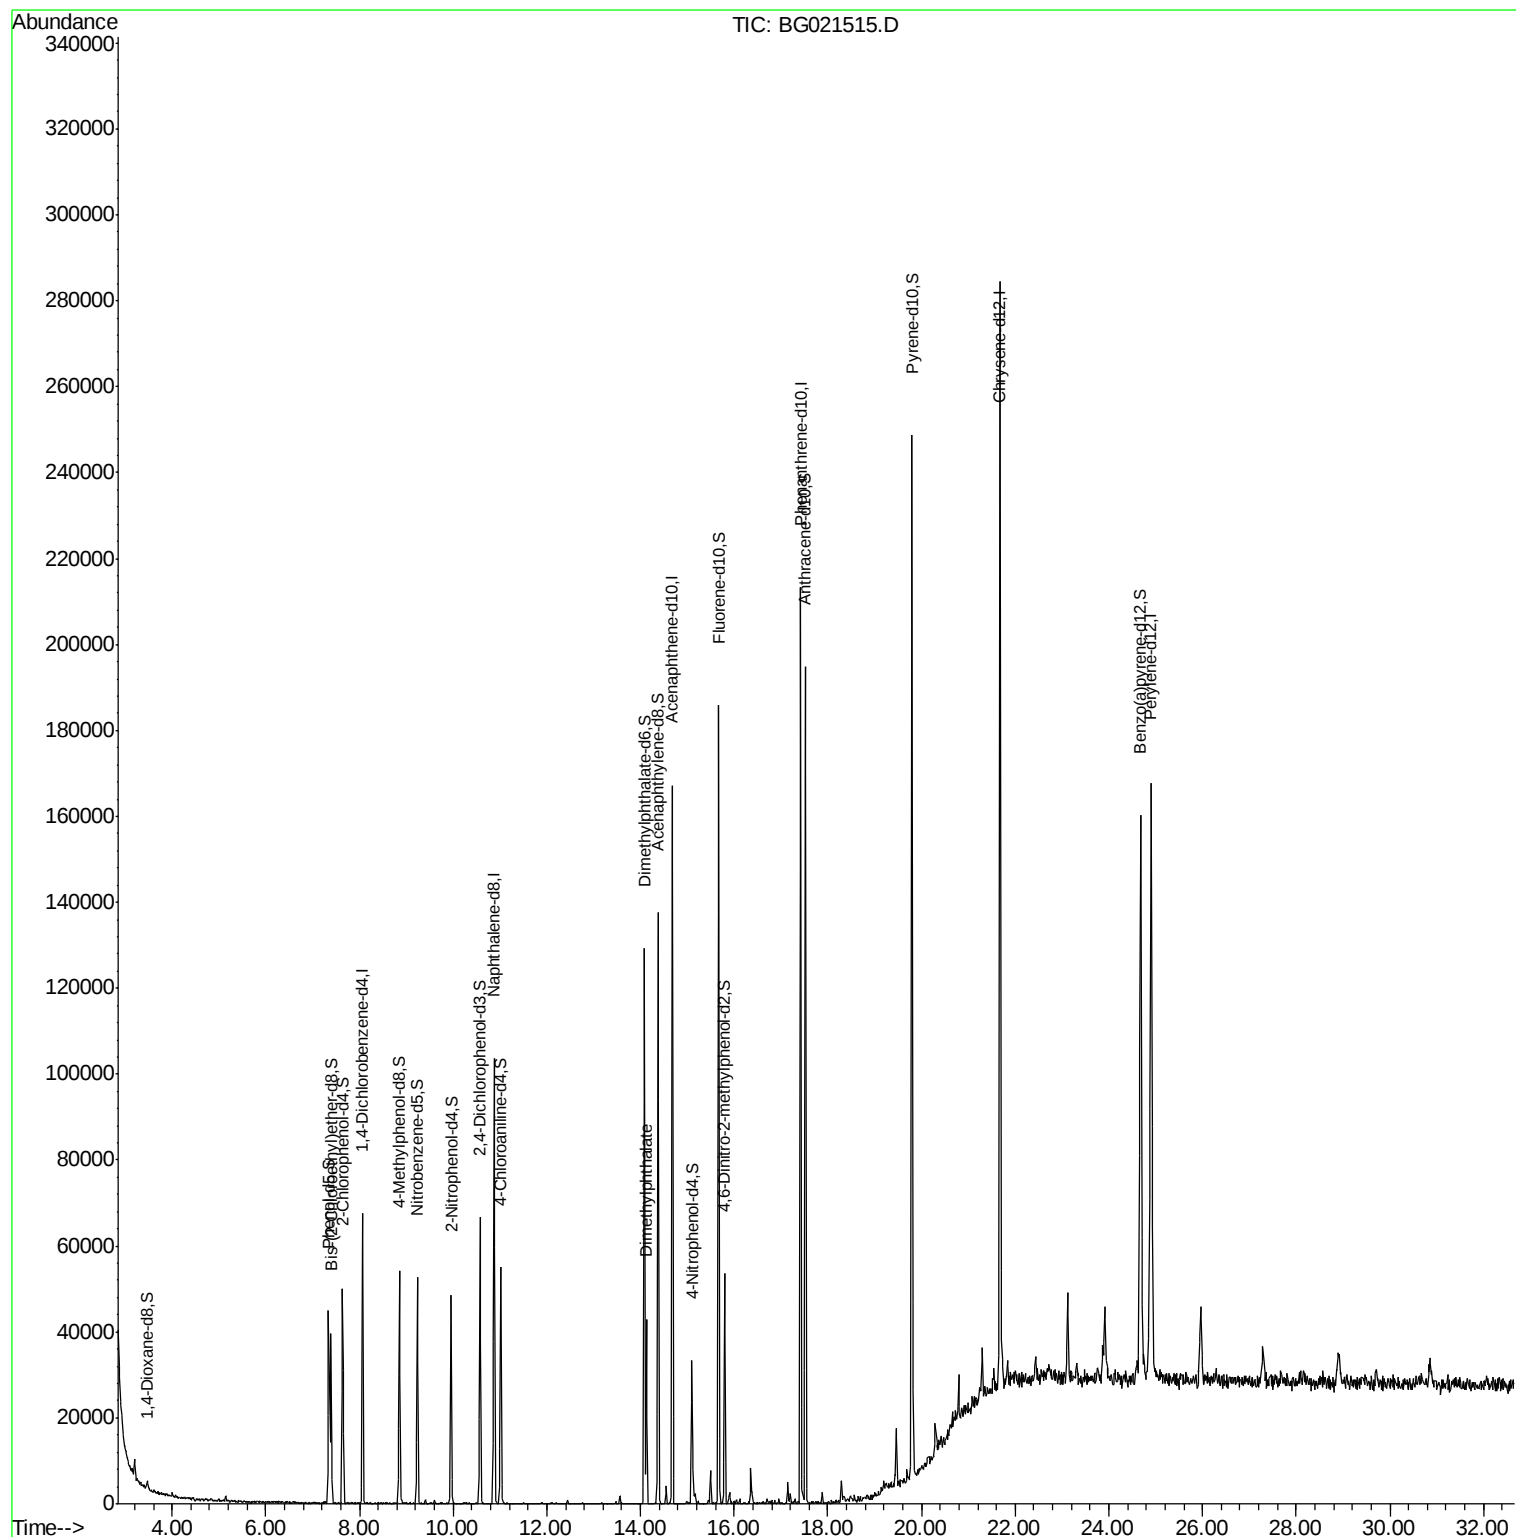

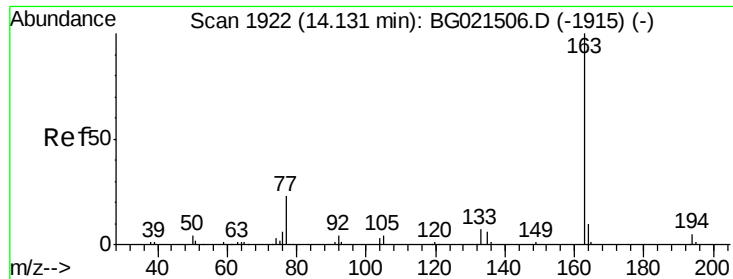

#45

Dimethylphthalate

Concen: 5.33 ng/ul

RT: 14.13 min Scan# 1921

Delta R.T. -0.00 min

Lab File: BG021515.D

Acq: 25 Mar 2016 15:39

Instrument :

BNA_G

ClientSampleId :

A4T49


Tgt Ion:163 Resp: 26027

Ion Ratio Lower Upper

163 100

194 4.3 3.9 5.9

164 10.4 8.7 13.1

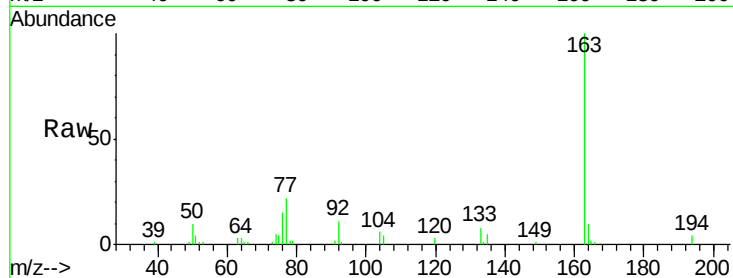

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

