

Data Path : Z:\HPCHEM1\BNA G\DATA\BG032516\
 Data File : BG021510.D
 Acq On : 25 Mar 2016 11:40
 Operator : UM/SJ
 Sample : H1909-10MS
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 A4T45MS

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG031616.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.120	43	48	50	rBV3	911	1151	0.31%	0.021%
2	3.155	50	54	57	rVV3	3095	4586	1.24%	0.083%
3	3.197	57	61	67	rVB2	3739	5579	1.51%	0.101%
4	3.244	67	69	73	rVB3	1426	1782	0.48%	0.032%
5	3.461	103	106	110	rVV2	1818	2300	0.62%	0.041%
6	3.996	193	197	202	rVB2	3318	4547	1.23%	0.082%
7	5.141	388	392	397	rBB2	878	1627	0.44%	0.029%
8	7.339	759	766	767	rBV	49395	75786	20.50%	1.367%
9	7.638	811	817	819	rBV	51735	82396	22.28%	1.486%
10	7.668	819	822	830	rVB	51631	85738	23.19%	1.547%
11	8.061	882	889	892	rBV	67101	113111	30.59%	2.040%
12	8.097	892	895	902	rVB	59543	99901	27.02%	1.802%
13	8.855	1016	1024	1032	rBV2	84445	182923	49.47%	3.300%
14	9.231	1081	1088	1096	rBB	48208	85292	23.07%	1.539%
15	9.401	1112	1117	1122	rBB2	1885	2769	0.75%	0.050%
16	9.953	1205	1211	1218	rBB2	45400	75621	20.45%	1.364%
17	10.570	1310	1316	1325	rBB	62856	111527	30.16%	2.012%
18	10.729	1337	1343	1350	rVB	79927	132495	35.83%	2.390%
19	10.870	1360	1367	1375	rBB	97664	171124	46.28%	3.087%
20	11.011	1385	1391	1403	rBV	32411	61256	16.57%	1.105%
21	12.239	1594	1600	1612	rBB	74462	129180	34.94%	2.330%
22	13.561	1821	1825	1828	rBB2	950	1165	0.32%	0.021%
23	14.078	1908	1913	1918	rBV	117600	169211	45.76%	3.052%
24	14.125	1918	1921	1927	rVB	50339	62785	16.98%	1.133%
25	14.372	1957	1963	1971	rBB	134322	203120	54.93%	3.664%
26	14.548	1989	1993	1998	rBB2	3574	4655	1.26%	0.084%
27	14.677	2009	2015	2021	rBV2	155071	238314	64.45%	4.299%
28	14.742	2021	2026	2033	rVB	159228	235199	63.61%	4.243%
29	15.041	2072	2077	2081	rBV	81121	133183	36.02%	2.402%
30	15.089	2081	2085	2101	rVB3	49664	130107	35.19%	2.347%
31	15.447	2143	2146	2150	rBV	1585	2112	0.57%	0.038%
32	15.494	2150	2154	2158	rVB	6202	8044	2.18%	0.145%
33	15.664	2177	2183	2190	rBB	180012	256745	69.43%	4.631%
34	15.788	2199	2204	2212	rBB2	53074	77034	20.83%	1.390%

Data Path : Z:\HPCHEM1\BNA G\DATA\BG032516\
 Data File : BG021510.D
 Acq On : 25 Mar 2016 11:40
 Operator : UM/SJ
 Sample : H1909-10MS
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 A4T45MS

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG031616.M
 Title : SVOA CALIBRATION

35	15.893	2215	2222	2226	rBB3	2563	4454	1.20%	0.080%
36	16.046	2244	2248	2251	rBB	1143	1007	0.27%	0.018%
37	16.111	2256	2259	2263	rBB2	938	1126	0.30%	0.020%
38	16.352	2295	2300	2303	rBV	8105	10617	2.87%	0.192%
39	16.687	2355	2357	2359	rBV2	1167	1377	0.37%	0.025%
40	16.757	2364	2369	2371	rVB2	670	1073	0.29%	0.019%
41	16.863	2384	2387	2391	rBV2	775	999	0.27%	0.018%
42	16.928	2394	2398	2400	rBV	880	989	0.27%	0.018%
43	17.092	2420	2426	2431	rBV3	29975	45708	12.36%	0.824%
44	17.145	2431	2435	2438	rVV2	5696	7353	1.99%	0.133%
45	17.192	2438	2443	2448	rVB4	2045	4063	1.10%	0.073%
46	17.304	2459	2462	2464	rBV	766	969	0.26%	0.017%
47	17.415	2475	2481	2486	rVV2	174368	267961	72.47%	4.834%
48	17.456	2486	2488	2493	rVV	8560	11582	3.13%	0.209%
49	17.515	2493	2498	2508	rVV2	187539	271241	73.35%	4.893%
50	17.615	2512	2515	2518	rVB	904	1196	0.32%	0.022%
51	17.680	2518	2526	2527	rBV	890	1491	0.40%	0.027%
52	17.768	2534	2541	2548	rBV3	1735	4069	1.10%	0.073%
53	17.879	2556	2560	2565	rVB	4259	5503	1.49%	0.099%
54	18.020	2580	2584	2588	rBV	17087	21024	5.69%	0.379%
55	18.061	2588	2591	2595	rVB	1045	1669	0.45%	0.030%
56	18.220	2613	2618	2619	rBV2	792	933	0.25%	0.017%
57	18.285	2624	2629	2634	rBV2	10418	14621	3.95%	0.264%
58	18.332	2634	2637	2645	rVV4	2904	6794	1.84%	0.123%
59	18.396	2645	2648	2650	rVV2	1114	1250	0.34%	0.023%
60	18.420	2650	2652	2656	rVB2	1298	1374	0.37%	0.025%
61	18.485	2656	2663	2665	rBV3	2179	3748	1.01%	0.068%
62	18.567	2673	2677	2680	rVV2	2498	3095	0.84%	0.056%
63	18.702	2695	2700	2701	rBV2	1111	1242	0.34%	0.022%
64	18.778	2709	2713	2716	rVB3	1703	1877	0.51%	0.034%
65	18.825	2718	2721	2724	rVV5	1801	2216	0.60%	0.040%
66	19.019	2749	2754	2755	rVV4	1164	1562	0.42%	0.028%
67	19.078	2759	2764	2766	rBV4	1807	2693	0.73%	0.049%
68	19.101	2766	2768	2769	rBV3	1182	990	0.27%	0.018%
69	19.190	2779	2783	2787	rVV4	3883	5056	1.37%	0.091%
70	19.248	2790	2793	2795	rVB3	1779	1874	0.51%	0.034%
71	19.266	2795	2796	2799	rBV3	982	1267	0.34%	0.023%

Data Path : Z:\HPCHEM1\BNA G\DATA\BG032516\
 Data File : BG021510.D
 Acq On : 25 Mar 2016 11:40
 Operator : UM/SJ
 Sample : H1909-10MS
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 A4T45MS

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG031616.M
 Title : SVOA CALIBRATION

72	19.407	2818	2820	2821	rBV2	1452	1086	0.29%	0.020%
73	19.460	2825	2829	2835	rVB2	23832	32028	8.66%	0.578%
74	19.554	2842	2845	2849	rVB5	2837	4446	1.20%	0.080%
75	19.601	2849	2853	2854	rBV3	1490	1502	0.41%	0.027%
76	19.619	2854	2856	2857	rBV2	1784	1126	0.30%	0.020%
77	19.660	2861	2863	2865	rBV2	1133	1142	0.31%	0.021%
78	19.707	2865	2871	2874	rVB5	3301	5524	1.49%	0.100%
79	19.795	2876	2886	2888	rBV	224342	348729	94.31%	6.290%
80	19.824	2888	2891	2897	rVB	265047	341946	92.48%	6.168%
81	19.871	2897	2899	2902	rBV4	1357	1971	0.53%	0.036%
82	19.936	2908	2910	2913	rVB4	1811	1713	0.46%	0.031%
83	19.965	2913	2915	2917	rBV3	2367	2298	0.62%	0.041%
84	20.065	2930	2932	2935	rVB4	2493	2204	0.60%	0.040%
85	20.100	2935	2938	2939	rBV3	1321	1633	0.44%	0.029%
86	20.136	2941	2944	2952	rVB8	3411	8364	2.26%	0.151%
87	20.206	2952	2956	2957	rBV3	1878	2105	0.57%	0.038%
88	20.294	2965	2971	2978	rVB7	10322	21635	5.85%	0.390%
89	20.347	2978	2980	2981	rBV2	1368	930	0.25%	0.017%
90	20.365	2981	2983	2984	rBV2	1652	1483	0.40%	0.027%
91	20.465	2994	3000	3002	rBV5	5105	9284	2.51%	0.167%
92	20.606	3020	3024	3029	rBV3	3906	7947	2.15%	0.143%
93	20.788	3051	3055	3058	rBV4	8780	12470	3.37%	0.225%
94	20.976	3085	3087	3091	rBV4	3783	5003	1.35%	0.090%
95	21.287	3136	3140	3146	rBV3	26557	39075	10.57%	0.705%
96	21.399	3157	3159	3166	rVB7	5392	9507	2.57%	0.171%
97	21.540	3179	3183	3186	rVB3	12630	16251	4.39%	0.293%
98	21.669	3198	3205	3211	rBV	216529	369770	100.00%	6.670%
99	24.671	3708	3716	3723	rBV2	120257	289301	78.24%	5.218%
100	24.895	3746	3754	3764	rVB2	118196	334927	90.58%	6.041%


Sum of corrected areas: 5543828

Data Path : Z:\HPCHEM1\BNA G\DATA\BG032516\
Data File : BG021510.D
Acq On : 25 Mar 2016 11:40
Operator : UM/SJ
Sample : H1909-10MS
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
A4T45MS

Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG031616.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

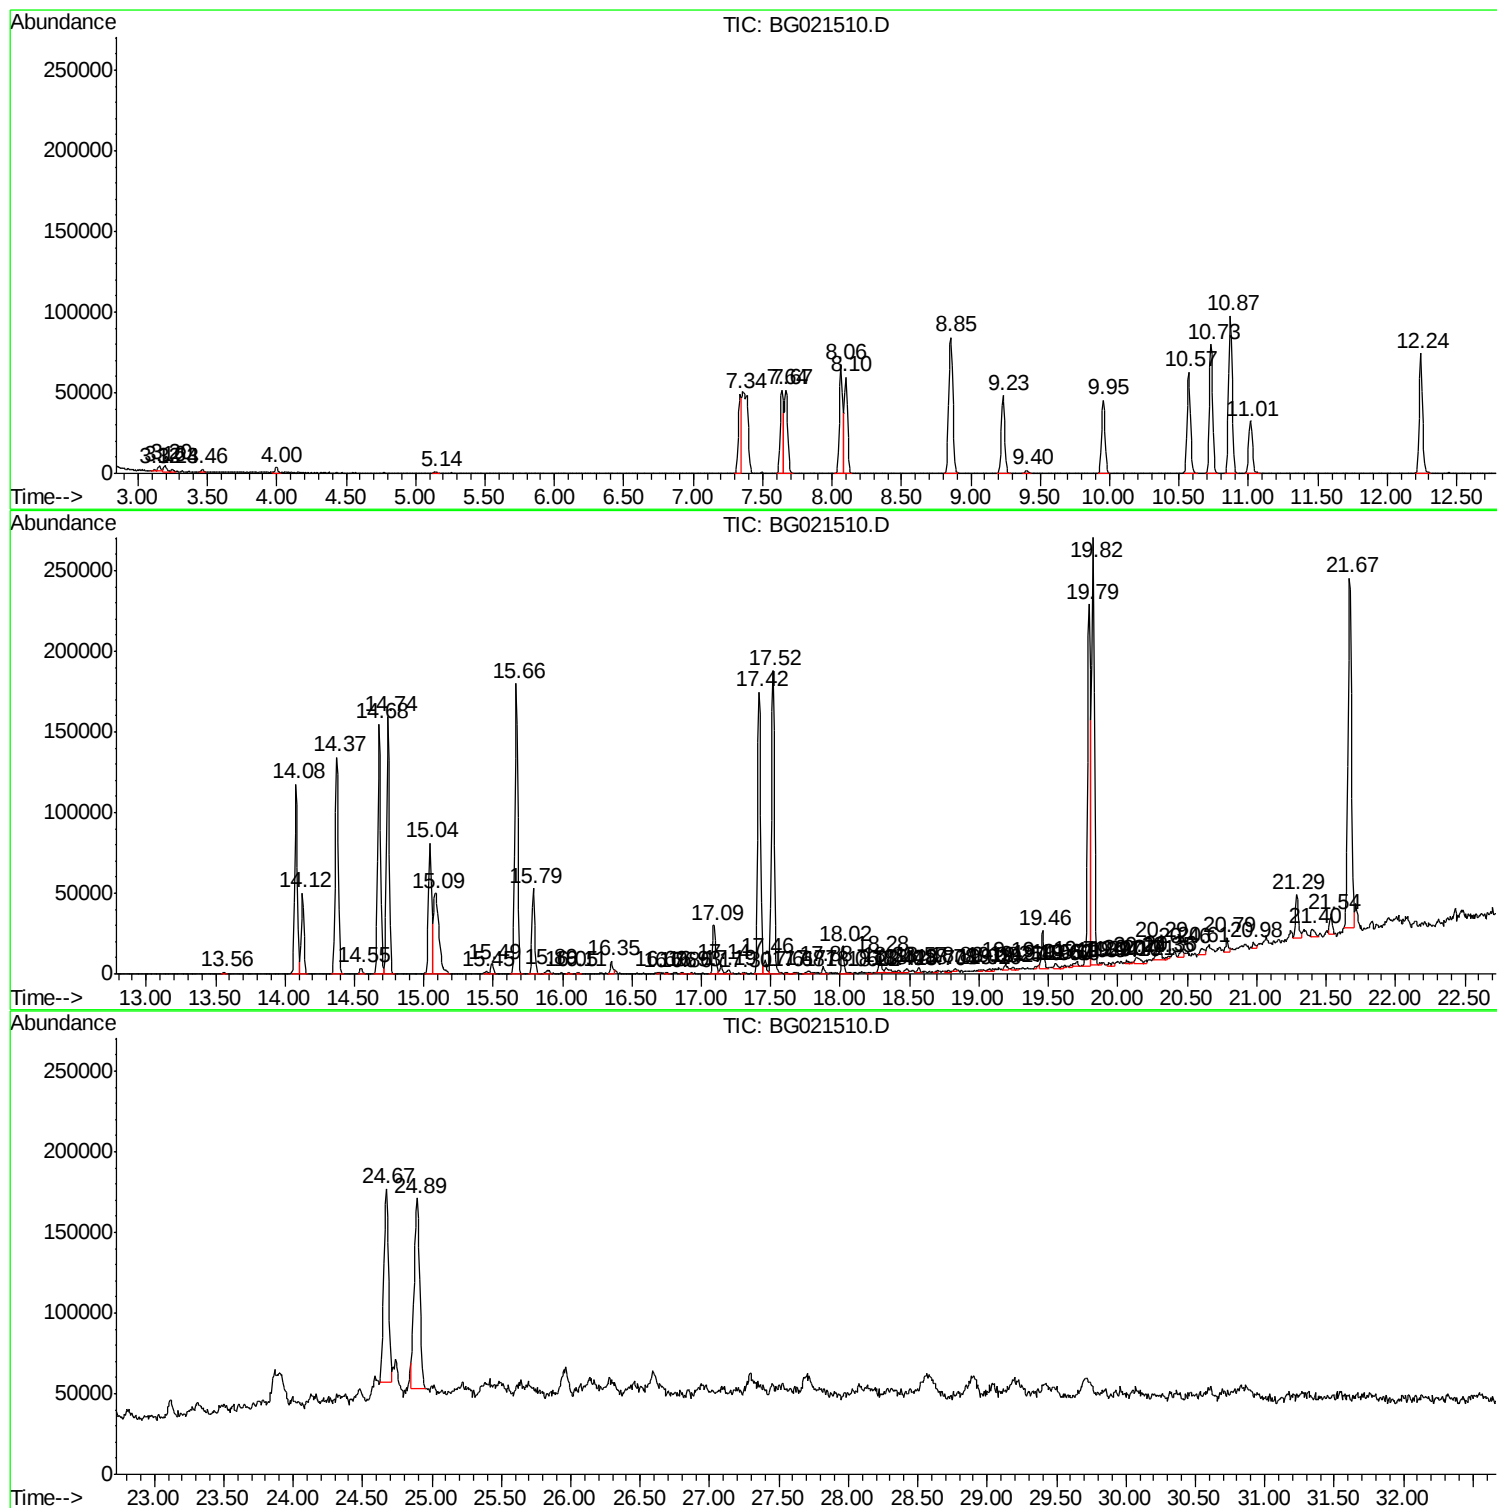

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG032516\
Data File : BG021510.D
Acq On : 25 Mar 2016 11:40
Operator : UM/SJ
Sample : H1909-10MS
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
A4T45MS

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG031616.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG032516\
Data File : BG021510.D
Acq On : 25 Mar 2016 11:40
Operator : UM/SJ
Sample : H1909-10MS
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
A4T45MS

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG031616.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc