
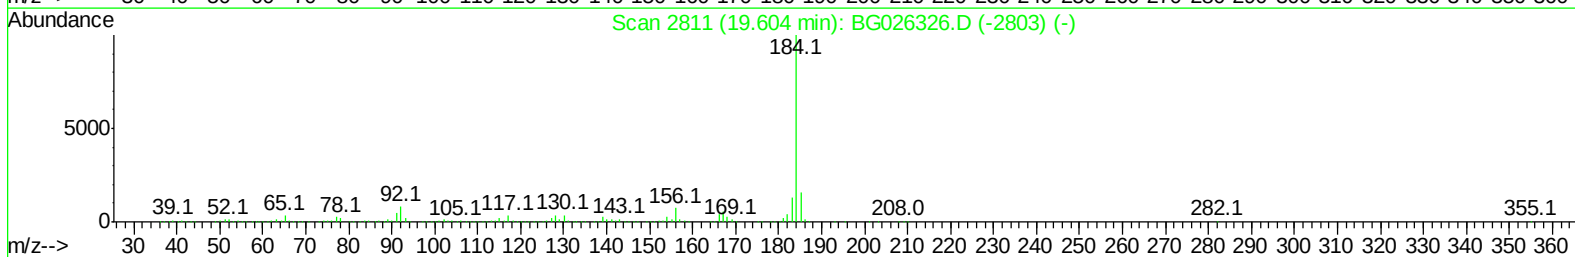
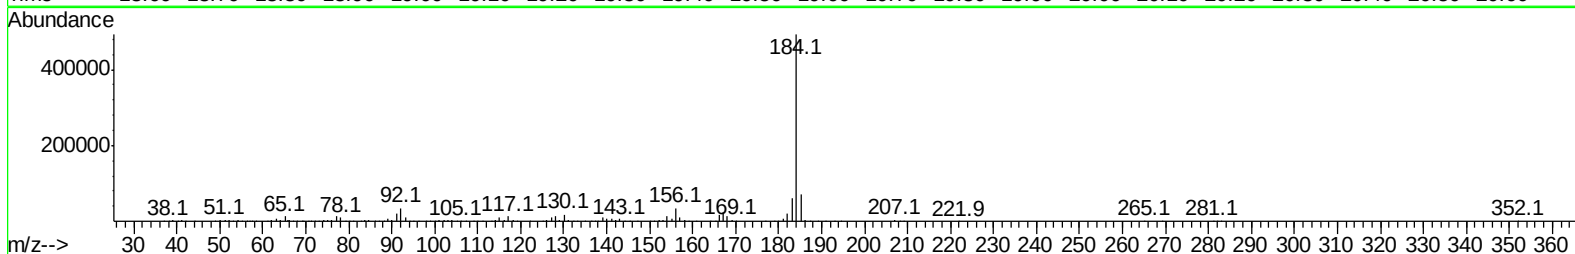


Data Path : Z:\HPCHEM1\BNA G\Data\BG032517\
 Data File : BG026414.D
 Acq On : 24 Mar 2017 14:36
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 27 01:09:51 2017
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG032017.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Mar 20 17:43:27 2017
 Response via : Initial Calibration

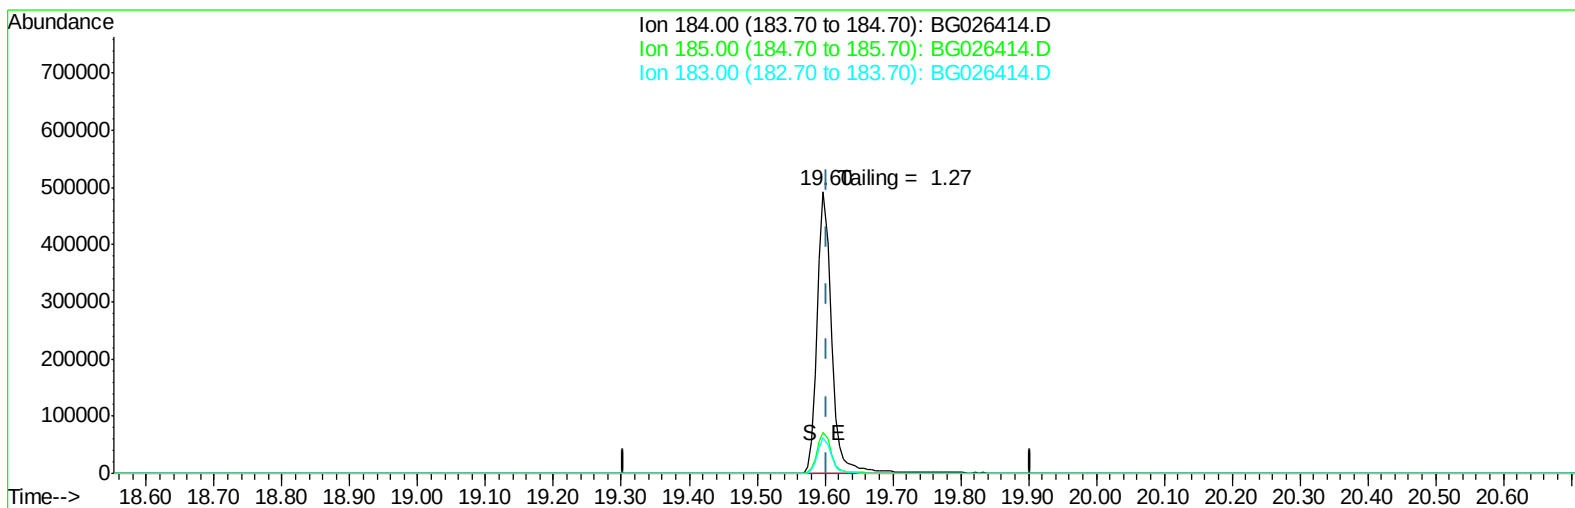

TIC: BG026414.D

(76) Benzidine




19.598min (-0.006) 54348.22ng

response 710185

Ion	Exp%	Act%
184.00	100	100
185.00	16.30	14.41
183.00	13.80	12.56
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA G\Data\BG032517\
Data File : BG026414.D
Acq On : 24 Mar 2017 14:36
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 27 01:09:51 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG032017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 20 17:43:27 2017
Response via : Initial Calibration

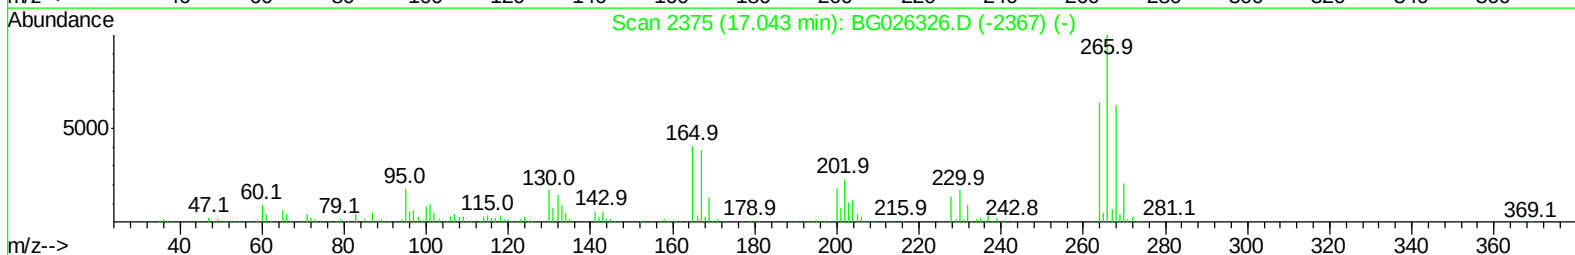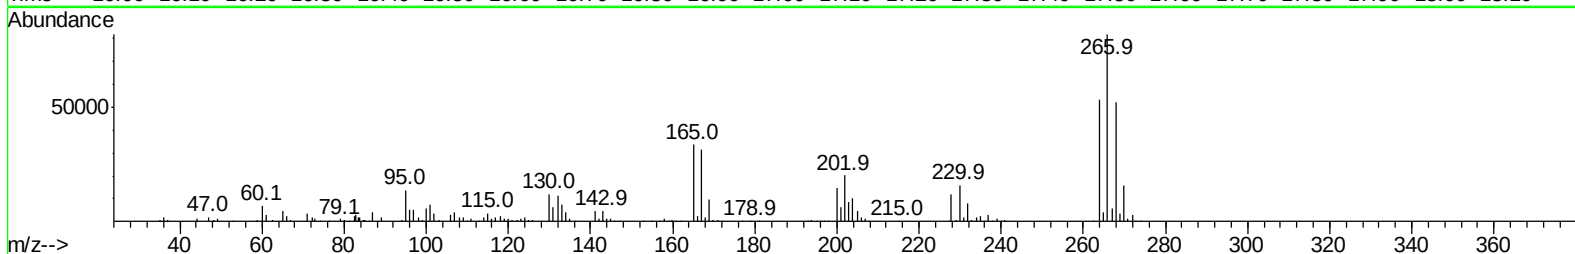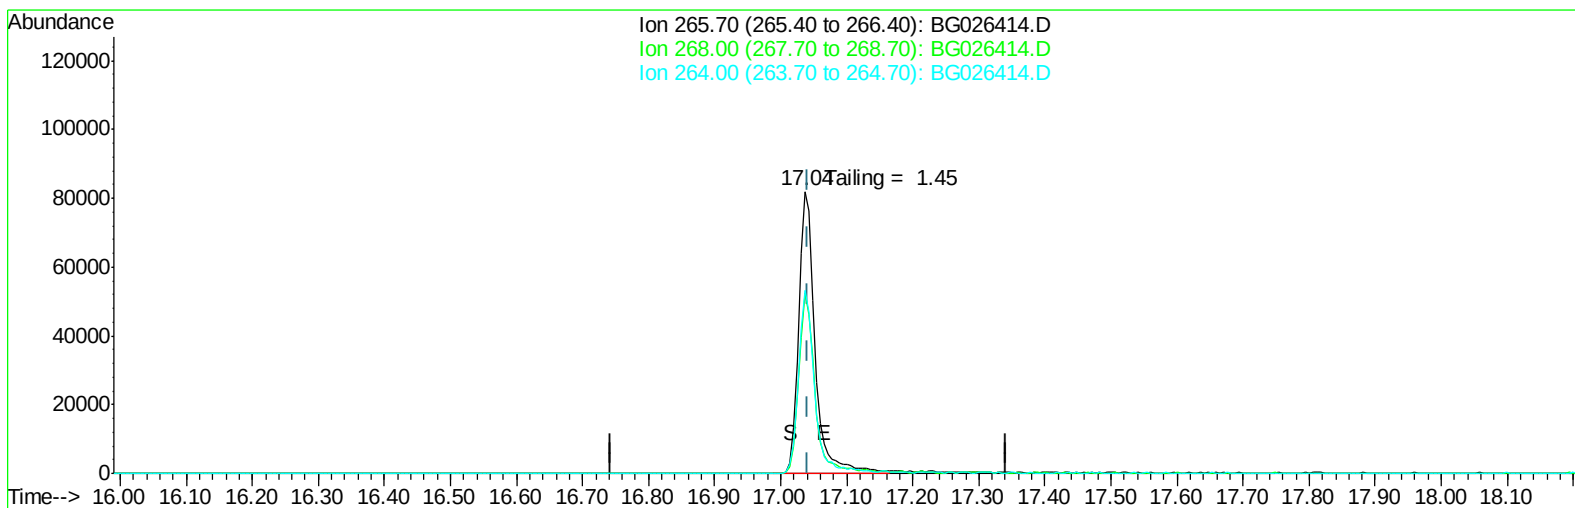

TIC: BG026414.D

(69) Pentachlorophenol (C)

17.036min (-0.006) 0.00ng

response 144957

Ion	Exp%	Act%
265.70	100	100
268.00	60.70	63.91
264.00	62.60	64.97
0.00	0.00	0.00