

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG032519\
 Data File : BG040121.D
 Acq On : 25 Mar 2019 17:32
 Operator : JU/SJ
 Sample : PB118239BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 PB118239BL

Quant Time: Mar 26 03:49:42 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG030419.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Mar 04 14:38:15 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.14	152	33764	20.00	ng	-0.03
21) Naphthalene-d8	10.96	136	145157	20.00	ng	-0.03
39) Acenaphthene-d10	14.77	164	105543	20.00	ng	-0.02
64) Phenanthrene-d10	17.51	188	279665	20.00	ng	-0.02
76) Chrysene-d12	21.80	240	297175	20.00	ng	-0.03
87) Perylene-d12	25.15	264	290402	20.00	ng	-0.05
System Monitoring Compounds						
5) 2-Fluorophenol	5.69	112	221380	111.86	ng	-0.02
7) Phenol-d6	7.29	99	319630	108.31	ng	-0.02
23) Nitrobenzene-d5	9.32	82	185878	69.26	ng	-0.03
42) 2,4,6-Tribromophenol	16.25	330	141699	115.19	ng	-0.02
45) 2-Fluorobiphenyl	13.39	172	501215	67.62	ng	-0.03
79) Terphenyl-d14	20.10	244	940200	69.66	ng	-0.02


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG032519\
Data File : BG040121.D
Acq On : 25 Mar 2019 17:32
Operator : JU/SJ
Sample : PB118239BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB118239BL

Quant Time: Mar 26 03:49:42 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG030419.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 04 14:38:15 2019
Response via : Initial Calibration

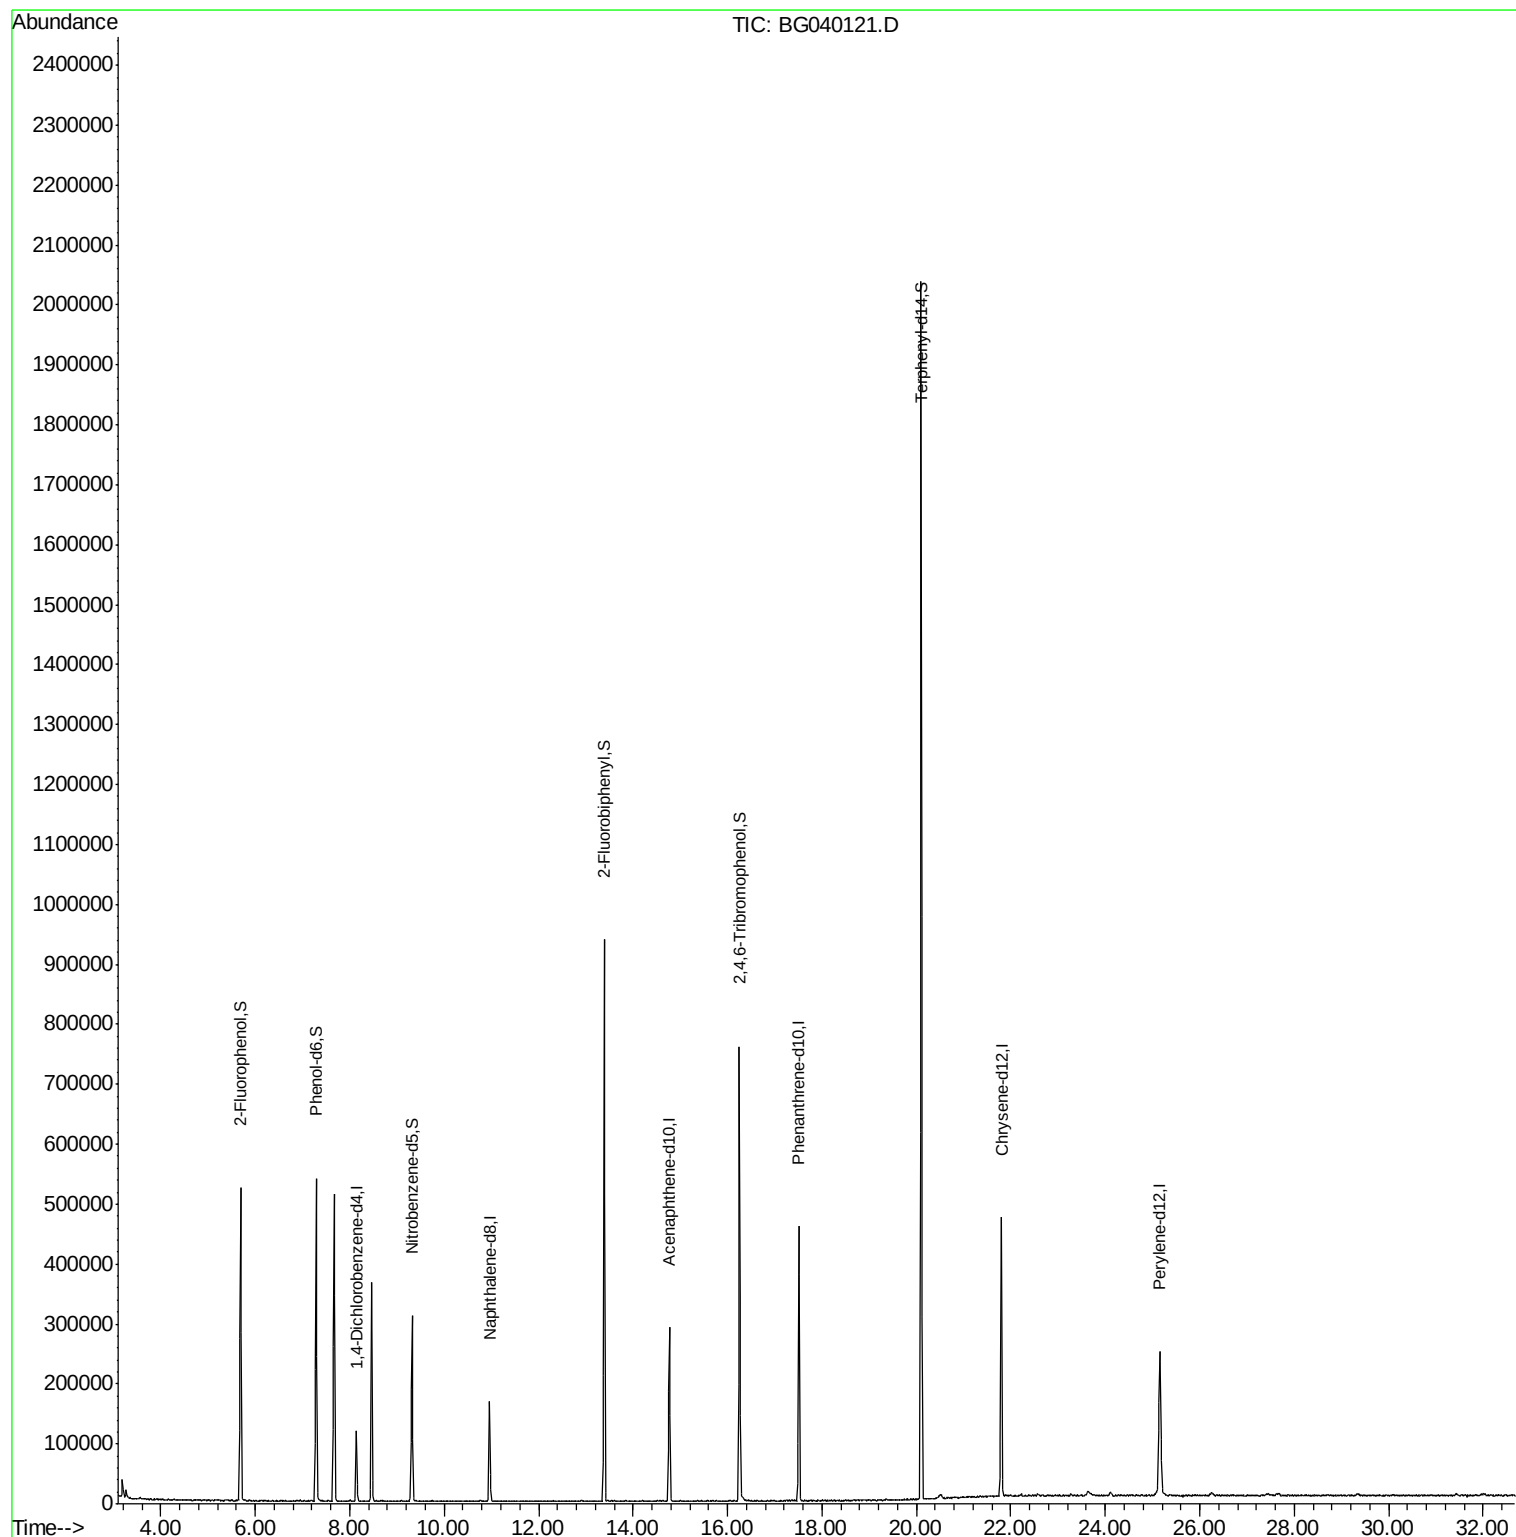

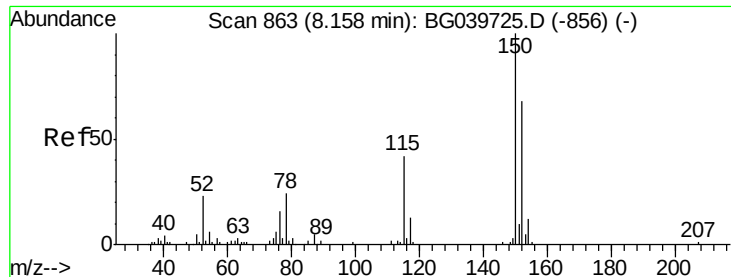


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.14 min Scan# 860
Delta R.T. -0.03 min
Lab File: BG040121.D
Acq: 25 Mar 2019 17:32

Instrument :
BNA_G
ClientSampleId :
PB118239BL

Tgt Ion:152 Resp: 33764
Ion Ratio Lower Upper
152 100
150 157.8 123.7 185.5
115 62.9 45.9 68.9

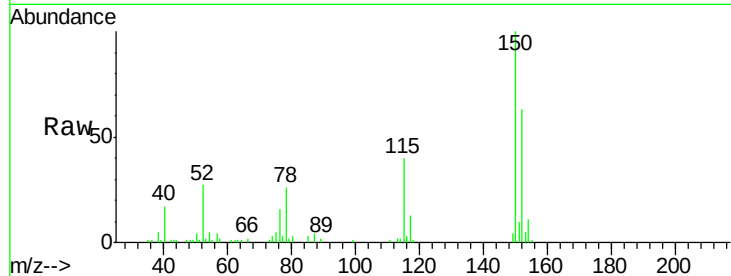


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

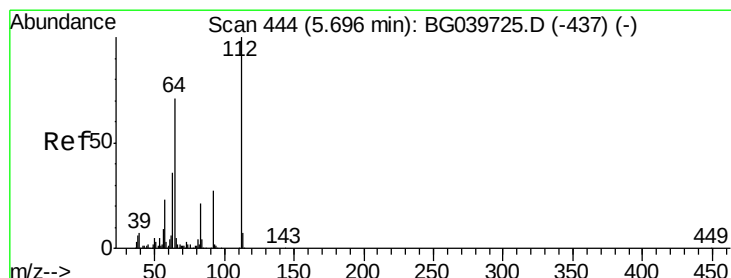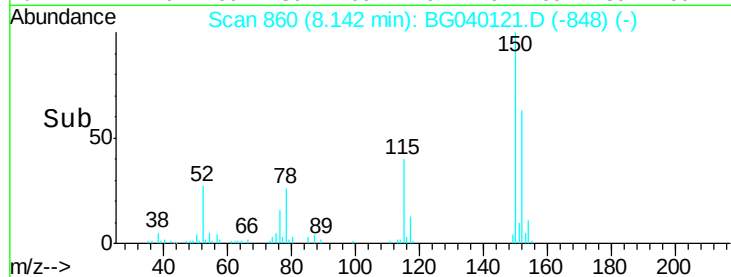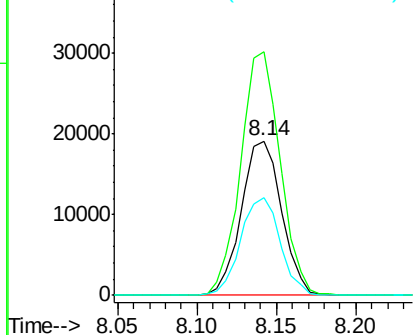



#5


2-Fluorophenol
Concen: 111.858 ng
RT: 5.69 min Scan# 442
Delta R.T. -0.02 min
Lab File: BG040121.D
Acq: 25 Mar 2019 17:32

Tgt Ion:112 Resp: 221380
Ion Ratio Lower Upper
112 100
64 68.6 57.8 86.8
63 35.4 29.8 44.6

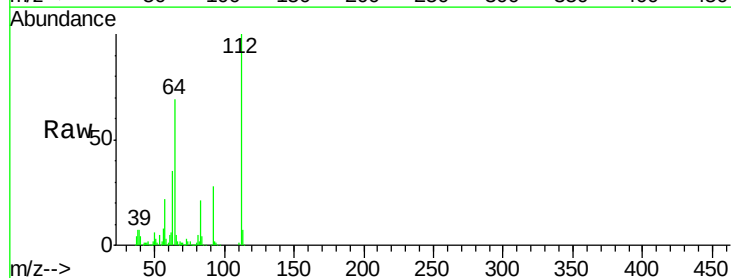

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BGC
Ion 63.00 (62.70 to 63.70): BGC

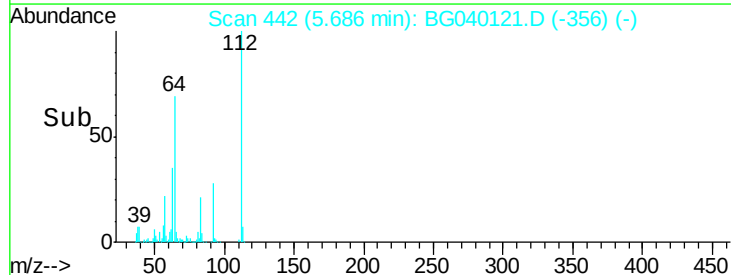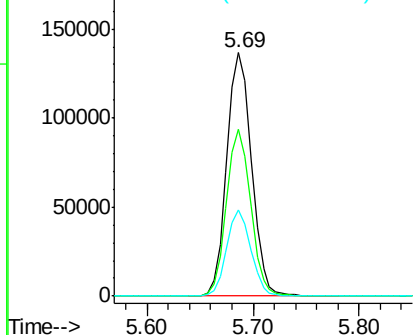

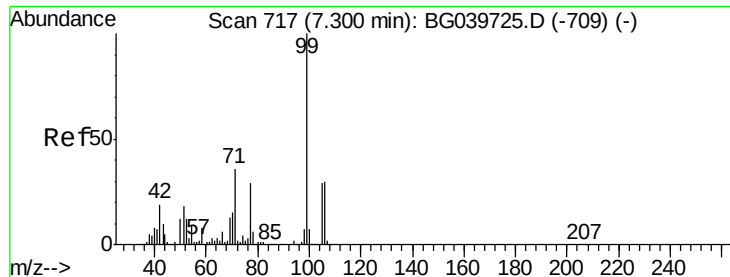

#7

Phenol-d6

Concen: 108.313 ng

RT: 7.29 min Scan# 715

Delta R.T. -0.02 min

Lab File: BG040121.D

Acq: 25 Mar 2019 17:32

Instrument :

BNA_G

ClientSampleId :

PB118239BL


Tgt Ion: 99 Resp: 319630

Ion Ratio Lower Upper




99 100

42 18.3 18.2 27.2

71 35.7 28.0 42.0

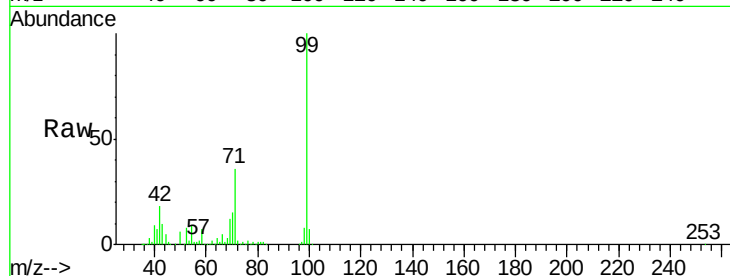

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

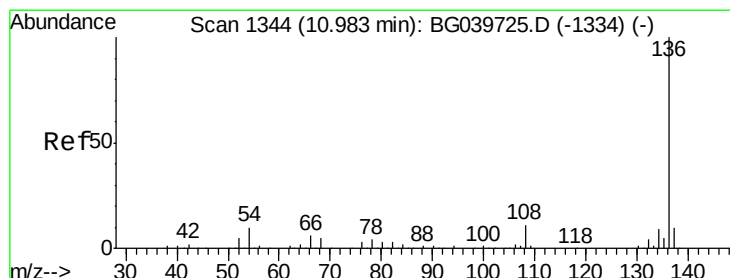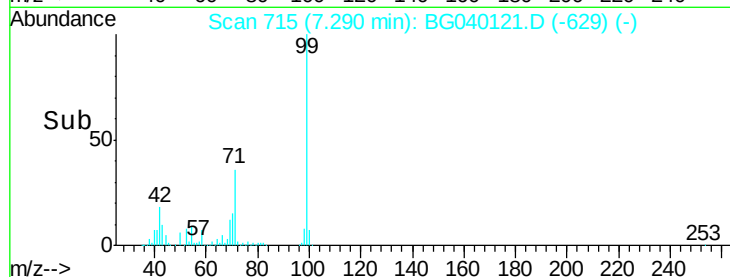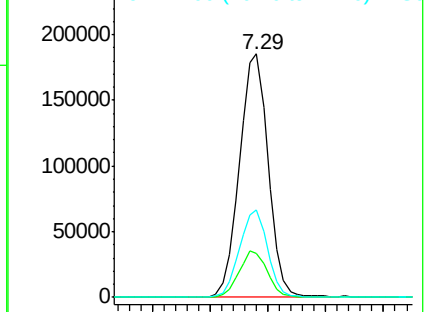

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.96 min Scan# 1340

Delta R.T. -0.03 min

Lab File: BG040121.D

Acq: 25 Mar 2019 17:32

Tgt Ion: 136 Resp: 145157


Ion Ratio Lower Upper

136 100



137 9.7 9.1 13.7


54 9.9 9.4 14.2

68 5.0 4.2 6.4

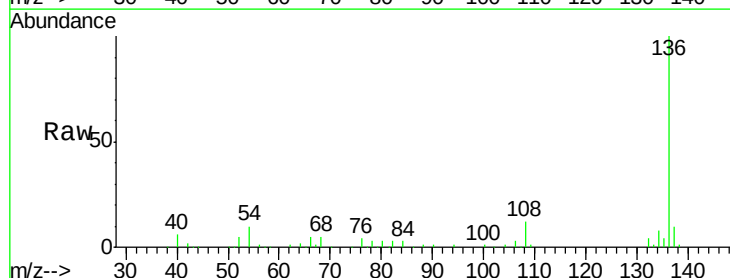

Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC

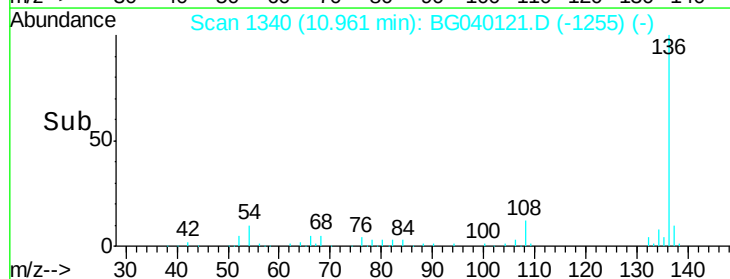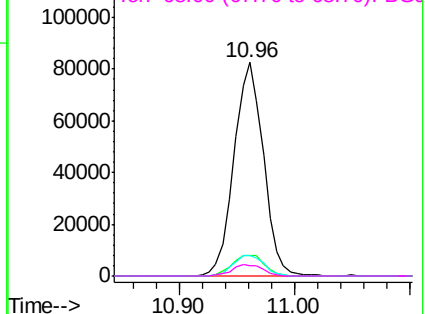


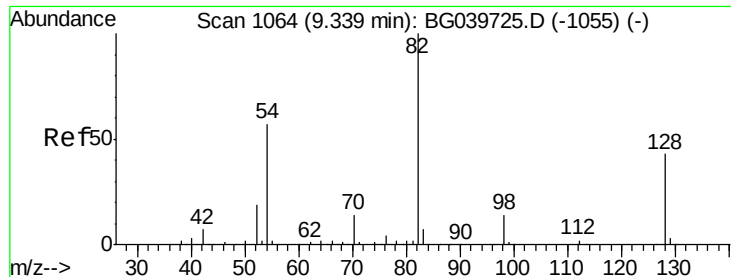




#23
Nitrobenzene-d5
Concen: 69.256 ng
RT: 9.32 min Scan# 1060
Delta R.T. -0.03 min
Lab File: BG040121.D
Acq: 25 Mar 2019 17:32

Instrument :
BNA_G
ClientSampleId :
PB118239BL

Tgt Ion: 82 Resp: 185878
Ion Ratio Lower Upper
82 100
128 42.9 31.3 46.9
54 56.3 50.9 76.3

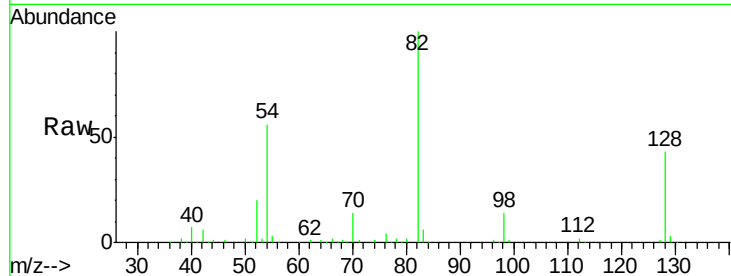


Abundance Ion 82.00 (81.70 to 82.70): BGC
Ion 128.00 (127.70 to 128.70): BGC
Ion 54.00 (53.70 to 54.70): BGC

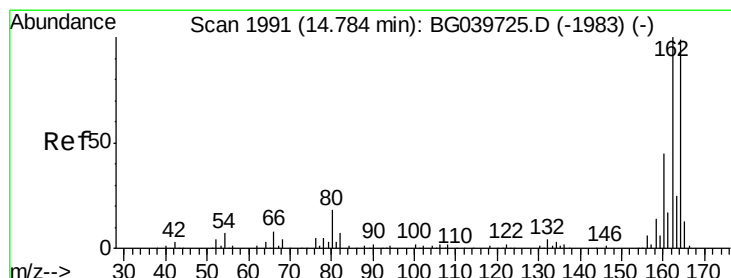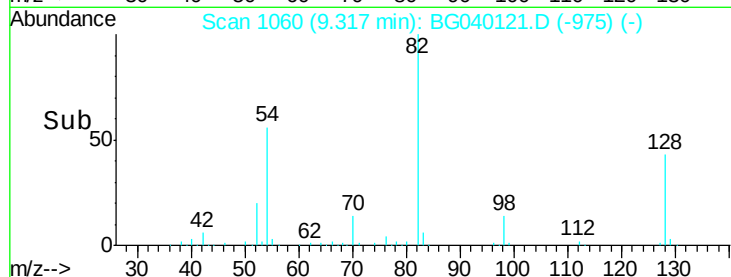
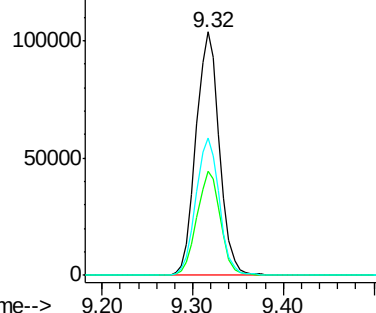



#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.77 min Scan# 1988
Delta R.T. -0.02 min
Lab File: BG040121.D
Acq: 25 Mar 2019 17:32

Tgt Ion: 164 Resp: 105543
Ion Ratio Lower Upper
164 100
162 102.6 81.6 122.4
160 45.3 34.2 51.2

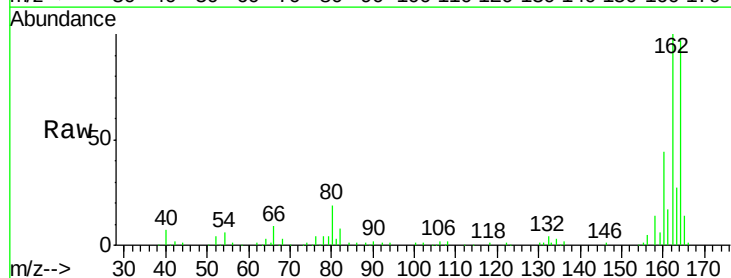

Abundance Ion 164.00 (163.70 to 164.70): BGC
Ion 162.00 (161.70 to 162.70): BGC
Ion 160.00 (159.70 to 160.70): BGC

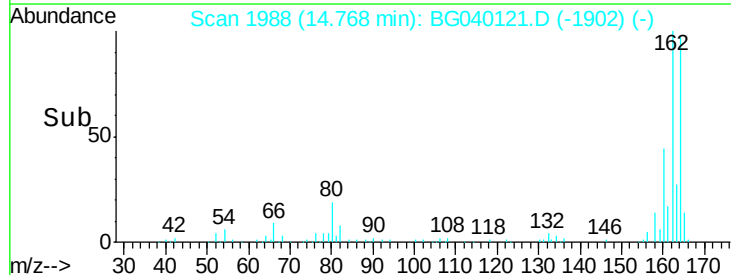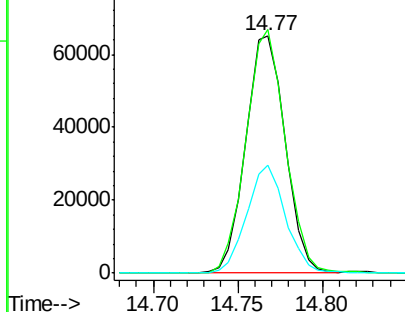

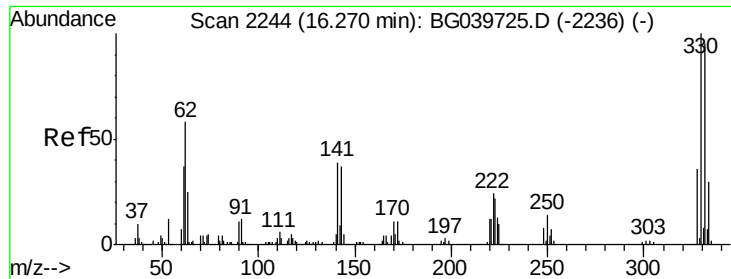

#42

2,4,6-Tribromophenol

Concen: 115.185 ng

RT: 16.25 min Scan# 2241

Delta R.T. -0.02 min

Lab File: BG040121.D

Acq: 25 Mar 2019 17:32

Instrument :

BNA_G

ClientSampleId :

PB118239BL


Tgt Ion:330 Resp: 141699

Ion Ratio Lower Upper

330 100

332 95.7 75.7 113.5




141 39.5 35.6 53.4

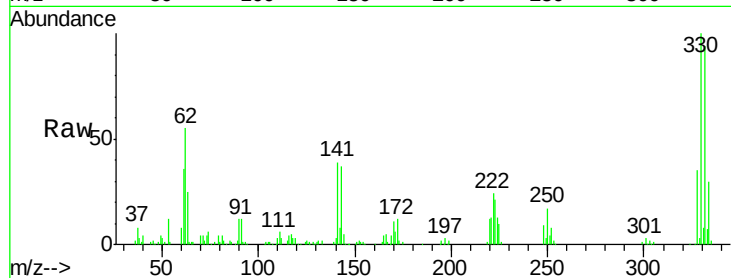

Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

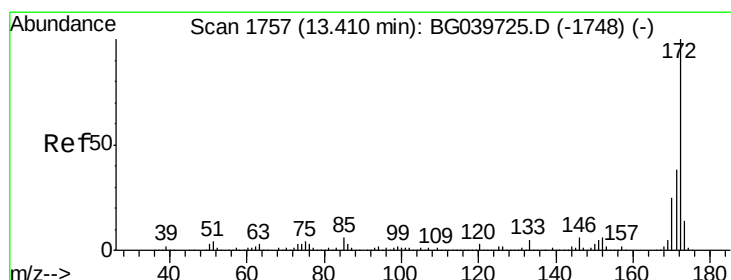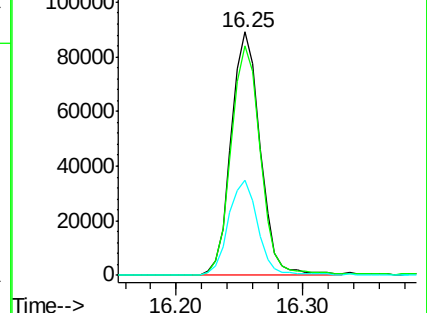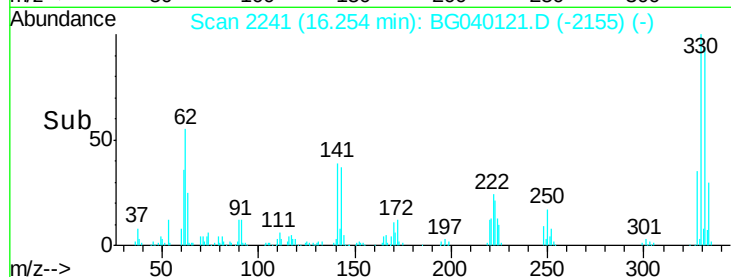

#45

2-Fluorobiphenyl

Concen: 67.616 ng

RT: 13.39 min Scan# 1753

Delta R.T. -0.03 min

Lab File: BG040121.D

Acq: 25 Mar 2019 17:32


Tgt Ion:172 Resp: 501215

Ion Ratio Lower Upper

172 100

171 37.8 30.8 46.2



170 24.7 20.2 30.4

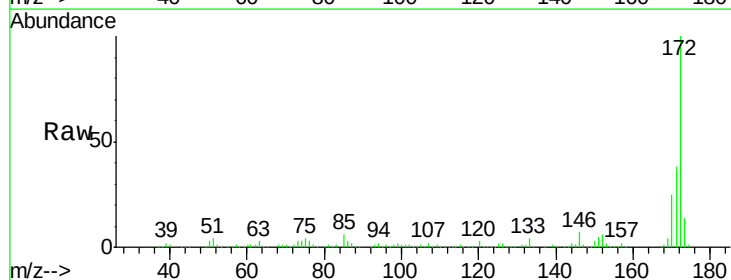


Abundance Ion 172.00 (171.70 to 172.70): E

Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E



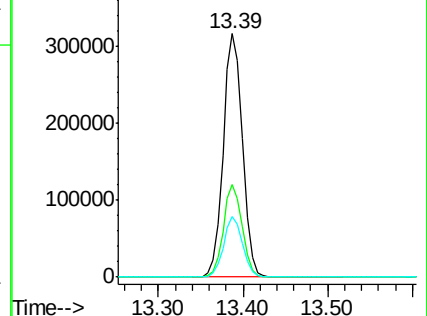
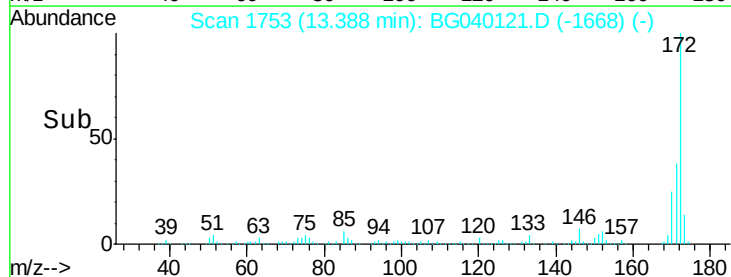


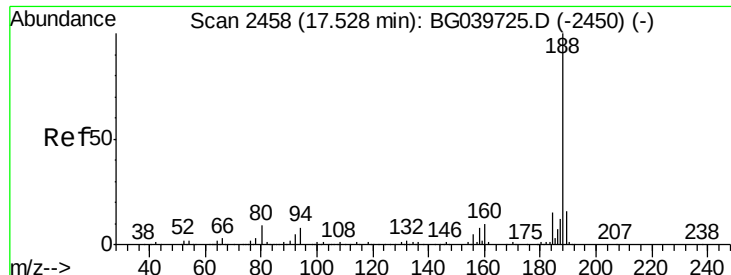

#64
 Phenanthrene-d10
 Concen: 20.000 ng
 RT: 17.51 min Scan# 2455
 Delta R.T. -0.02 min
 Lab File: BG040121.D
 Acq: 25 Mar 2019 17:32




Instrument :
 BNA_G
 ClientSampleId :
 PB118239BL


Tgt Ion:188 Resp: 279665
 Ion Ratio Lower Upper
 188 100
 94 8.4 6.9 10.3
 80 9.0 8.1 12.1

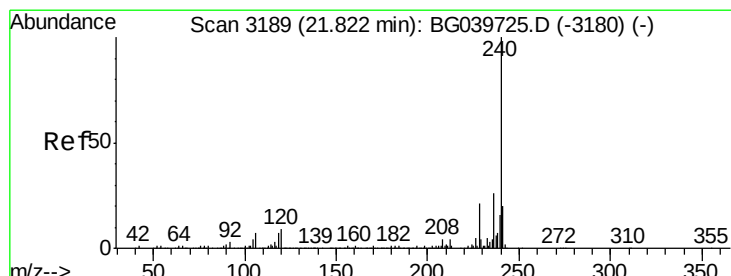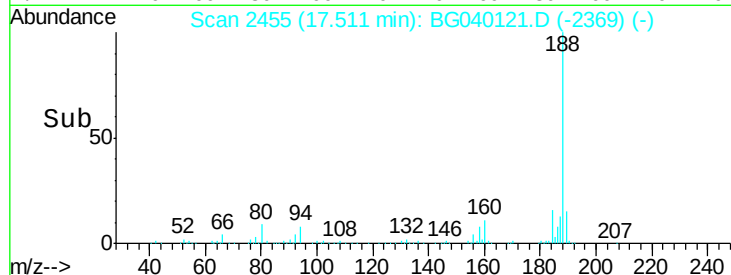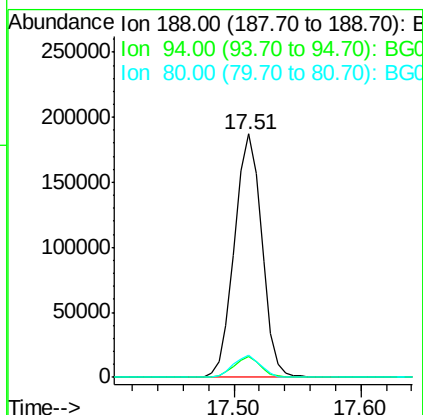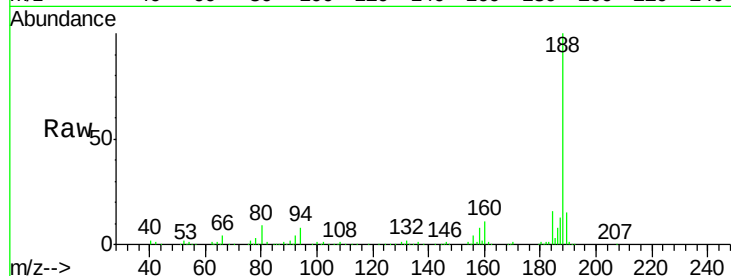

#76
 Chrysene-d12
 Concen: 20.000 ng
 RT: 21.80 min Scan# 3185
 Delta R.T. -0.03 min
 Lab File: BG040121.D
 Acq: 25 Mar 2019 17:32

Tgt Ion:240 Resp: 297175
 Ion Ratio Lower Upper
 240 100
 120 8.2 7.0 10.6
 236 25.2 21.0 31.4

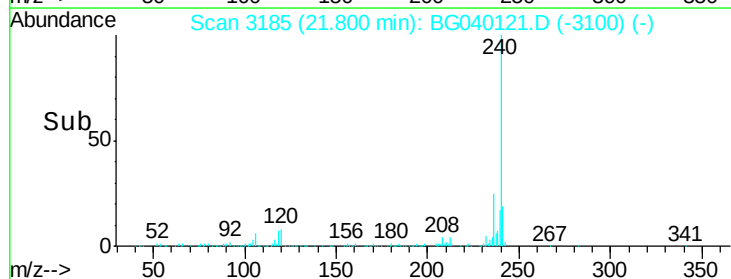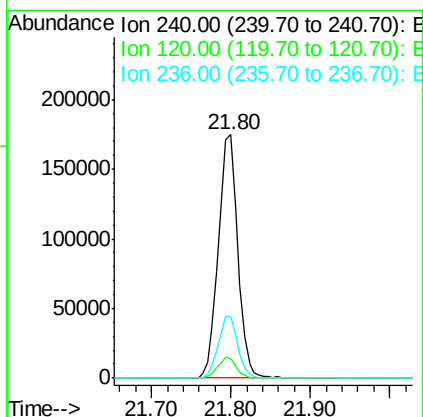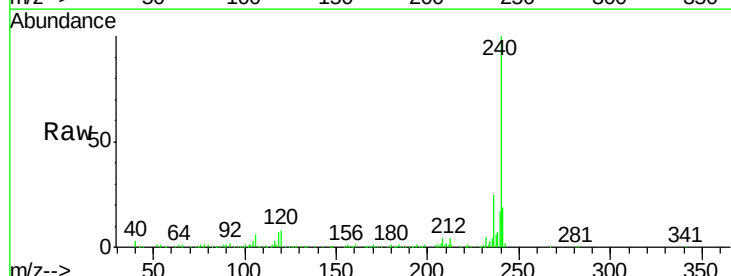

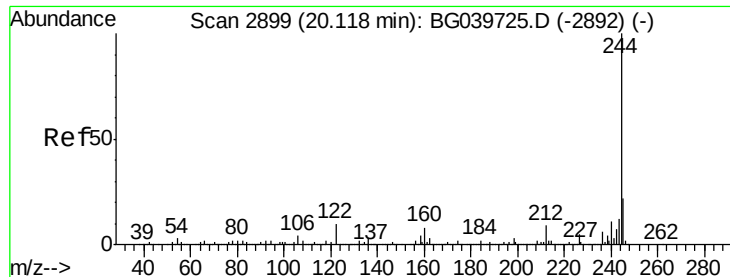

#79

Terphenyl-d14

Concen: 69.661 ng

RT: 20.10 min Scan# 2896

Delta R.T. -0.02 min

Lab File: BG040121.D

Acq: 25 Mar 2019 17:32

Instrument :

BNA_G

ClientSampleId :

PB118239BL


Tgt Ion:244 Resp: 940200

Ion Ratio Lower Upper

244 100

212 8.5 7.3 10.9


122 9.5 8.4 12.6

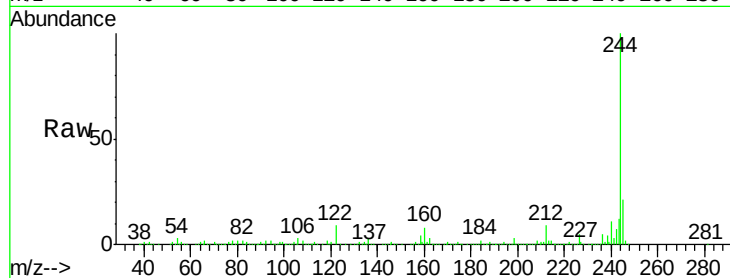



Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

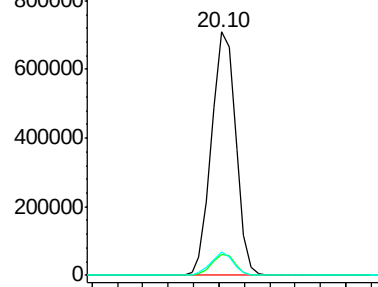

Time--> 20.00 20.10 20.20

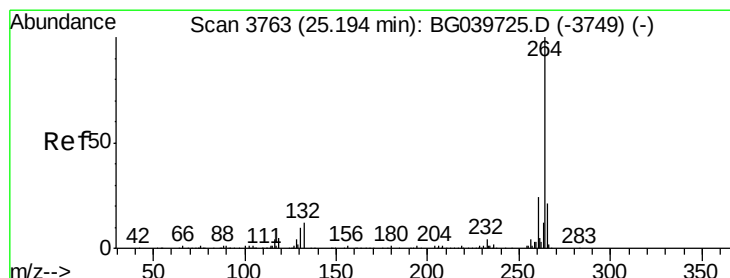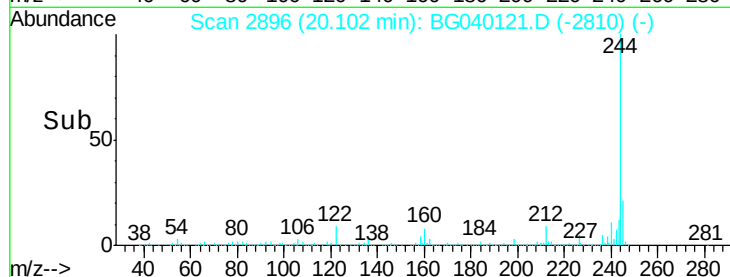

#87

Perylene-d12

Concen: 20.000 ng

RT: 25.15 min Scan# 3756

Delta R.T. -0.05 min

Lab File: BG040121.D

Acq: 25 Mar 2019 17:32


Tgt Ion:264 Resp: 290402

Ion Ratio Lower Upper

264 100

260 23.5 18.2 27.4


265 21.5 18.5 27.7

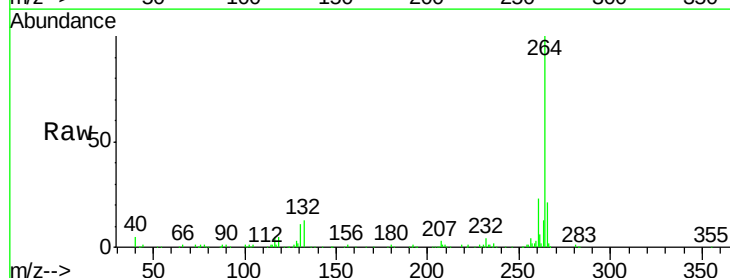

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

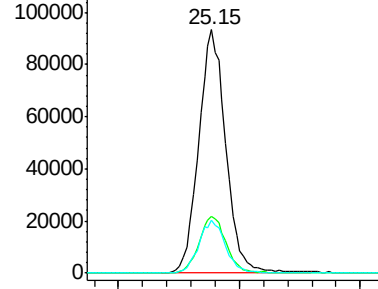

Time--> 25.00 25.20

