

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG032519\
 Data File : BG040138.D
 Acq On : 26 Mar 2019 6:12
 Operator : JU/SJ
 Sample : K2050-08
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 CS-4

Quant Time: Mar 26 09:01:47 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG030419.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Mar 04 14:38:15 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.14	152	38997	20.00	ng	-0.03
21) Naphthalene-d8	10.96	136	173516	20.00	ng	-0.03
39) Acenaphthene-d10	14.77	164	123148	20.00	ng	-0.02
64) Phenanthrene-d10	17.51	188	317191	20.00	ng	-0.02
76) Chrysene-d12	21.80	240	330593	20.00	ng	-0.03
87) Perylene-d12	25.15	264	306556	20.00	ng	-0.05
System Monitoring Compounds						
5) 2-Fluorophenol	5.68	112	277222	121.28	ng	-0.02
7) Phenol-d6	7.29	99	364521	106.95	ng	-0.02
23) Nitrobenzene-d5	9.31	82	267194	83.28	ng	-0.03
42) 2,4,6-Tribromophenol	16.25	330	164028	114.27	ng	-0.02
45) 2-Fluorobiphenyl	13.39	172	670790	77.56	ng	-0.03
79) Terphenyl-d14	20.11	244	1193501	79.49	ng	-0.02


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG032519\
Data File : BG040138.D
Acq On : 26 Mar 2019 6:12
Operator : JU/SJ
Sample : K2050-08
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
CS-4

Quant Time: Mar 26 09:01:47 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG030419.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 04 14:38:15 2019
Response via : Initial Calibration

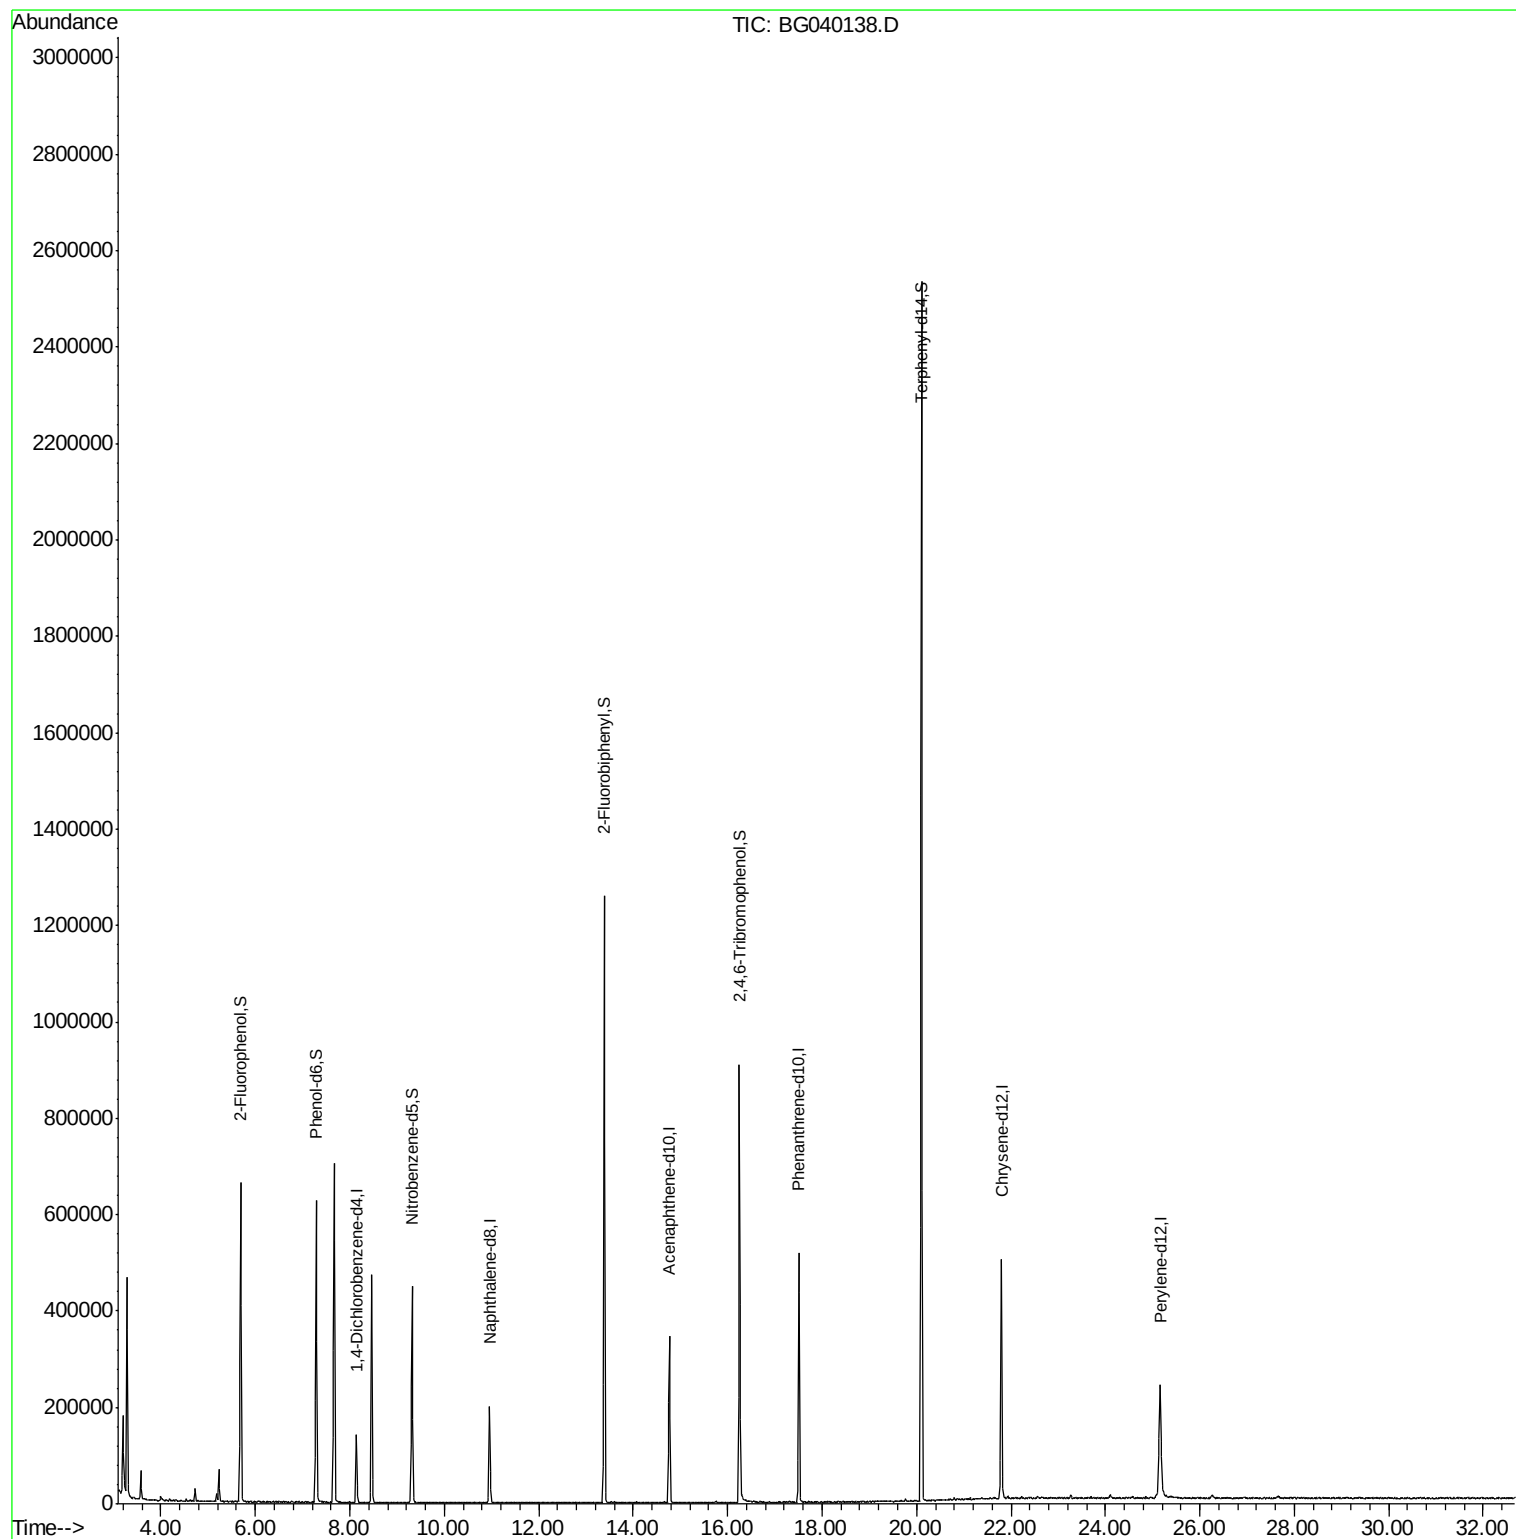




#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.14 min Scan# 860
Delta R.T. -0.03 min
Lab File: BG040138.D
Acq: 26 Mar 2019 6:12

Instrument :
BNA_G
ClientSampled :
CS-4

Tgt Ion:152 Resp: 38997
Ion Ratio Lower Upper
152 100
150 169.3 123.7 185.5
115 64.9 45.9 68.9

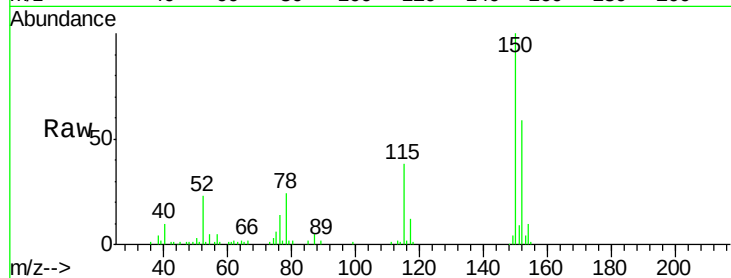


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

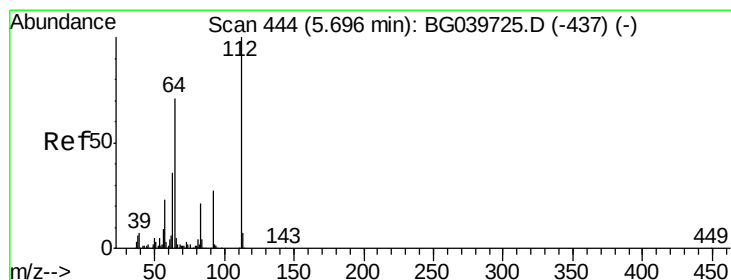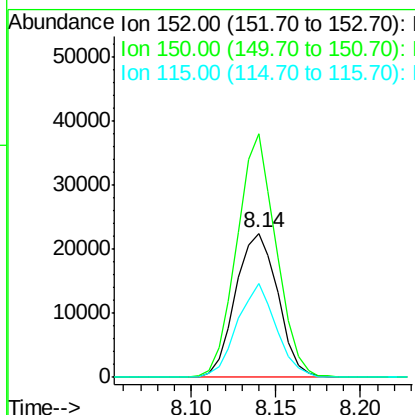



#5


2-Fluorophenol
Concen: 121.277 ng
RT: 5.68 min Scan# 442
Delta R.T. -0.02 min
Lab File: BG040138.D
Acq: 26 Mar 2019 6:12

Tgt Ion:112 Resp: 277222
Ion Ratio Lower Upper
112 100
64 68.5 57.8 86.8
63 35.2 29.8 44.6

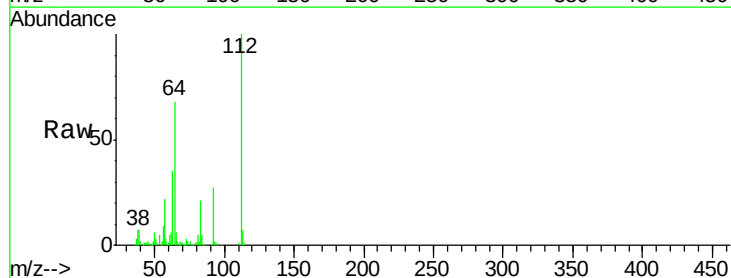

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BGC
Ion 63.00 (62.70 to 63.70): BGC

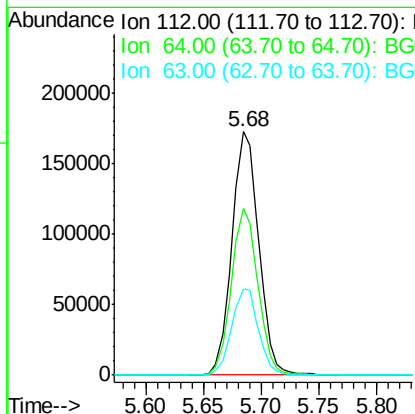



#7

Phenol-d6

Concen: 106.949 ng

RT: 7.29 min Scan# 715

Delta R.T. -0.02 min

Lab File: BG040138.D

Acq: 26 Mar 2019 6:12

Instrument :

BNA_G

ClientSampleId :

CS-4


Tgt Ion: 99 Resp: 364521

Ion Ratio Lower Upper




99 100

42 19.0 18.2 27.2

71 35.2 28.0 42.0

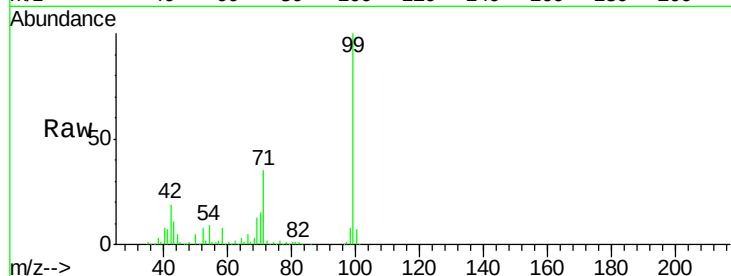

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

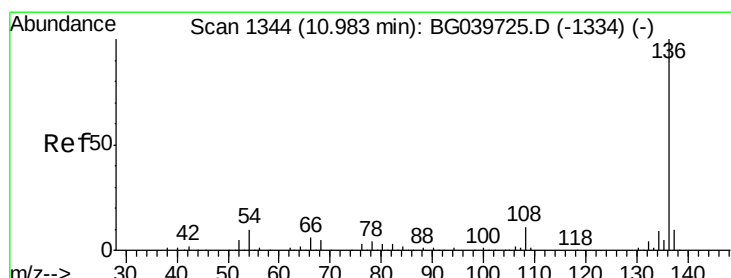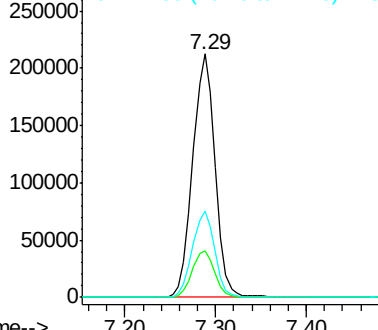

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.96 min Scan# 1340

Delta R.T. -0.03 min

Lab File: BG040138.D

Acq: 26 Mar 2019 6:12

Tgt Ion: 136 Resp: 173516


Ion Ratio Lower Upper

136 100



137 10.7 9.1 13.7


54 10.1 9.4 14.2

68 5.7 4.2 6.4

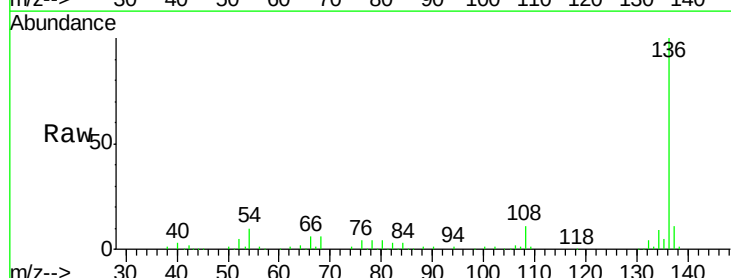

Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC

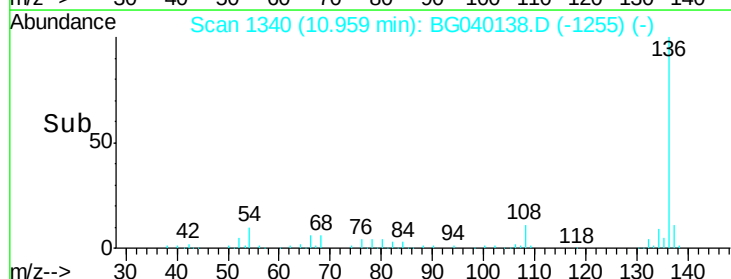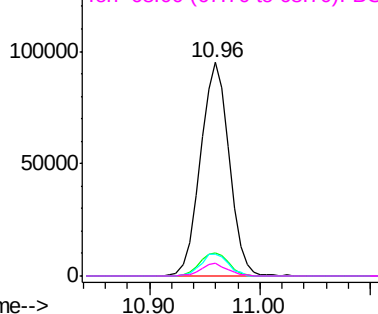







#23
Nitrobenzene-d5
Concen: 83.283 ng
RT: 9.31 min Scan# 1060
Delta R.T. -0.03 min
Lab File: BG040138.D
Acq: 26 Mar 2019 6:12

Instrument :
BNA_G
ClientSampleId :
CS-4

Tgt Ion: 82 Resp: 267194
Ion Ratio Lower Upper
82 100
128 42.3 31.3 46.9
54 56.1 50.9 76.3

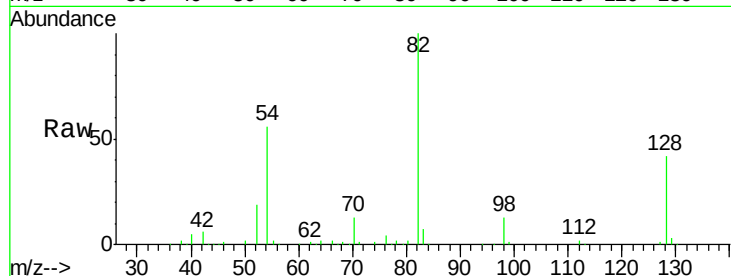


Abundance Ion 82.00 (81.70 to 82.70): BGC
Ion 128.00 (127.70 to 128.70): BGC
Ion 54.00 (53.70 to 54.70): BGC

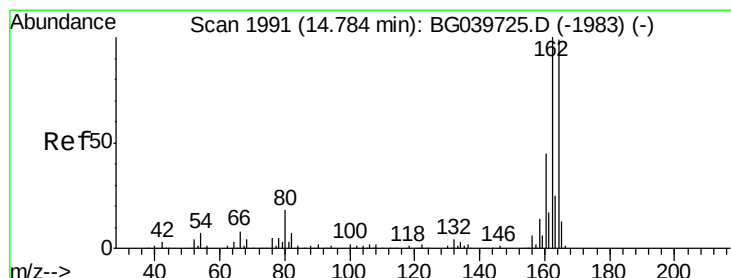
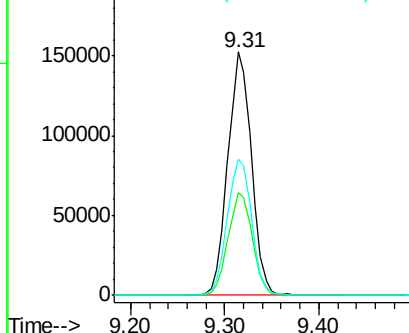



#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.77 min Scan# 1988
Delta R.T. -0.02 min
Lab File: BG040138.D
Acq: 26 Mar 2019 6:12

Tgt Ion: 164 Resp: 123148
Ion Ratio Lower Upper
164 100
162 102.9 81.6 122.4
160 45.2 34.2 51.2

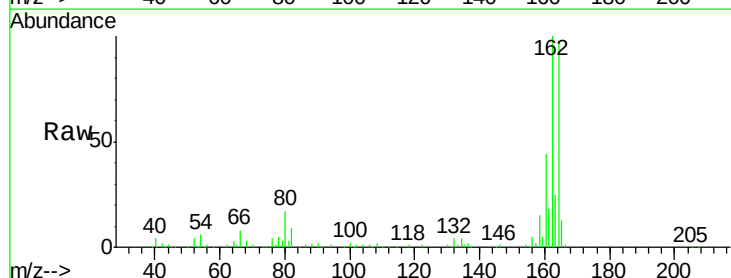

Abundance Ion 164.00 (163.70 to 164.70): BGC
Ion 162.00 (161.70 to 162.70): BGC
Ion 160.00 (159.70 to 160.70): BGC

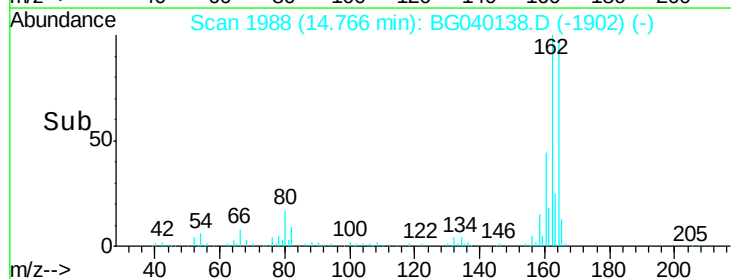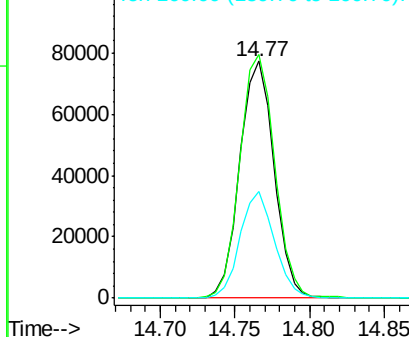


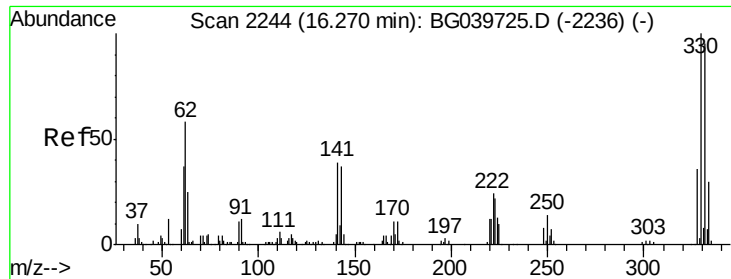




#42
 2,4,6-Tribromophenol
 Concen: 114.275 ng
 RT: 16.25 min Scan# 2241
 Delta R.T. -0.02 min
 Lab File: BG040138.D
 Acq: 26 Mar 2019 6:12

Instrument :
 BNA_G
 ClientSampleId :
 CS-4

Tgt Ion:330 Resp: 164028
 Ion Ratio Lower Upper
 330 100
 332 96.3 75.7 113.5
 141 40.8 35.6 53.4

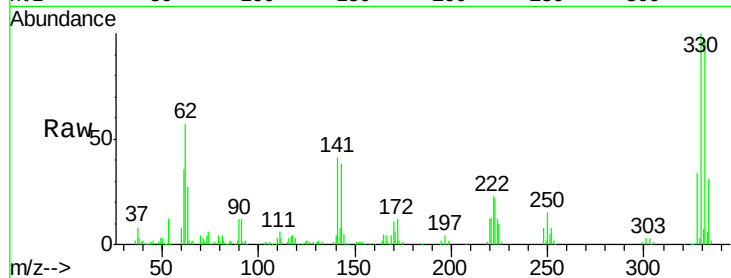


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

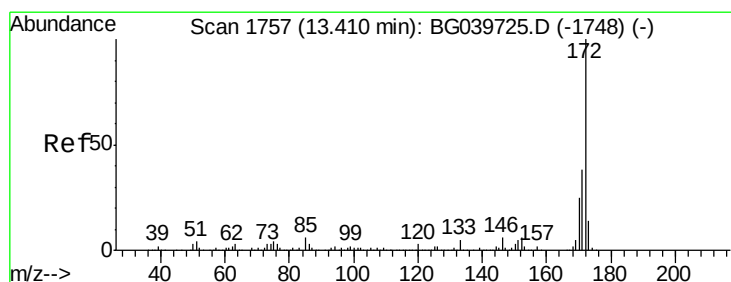
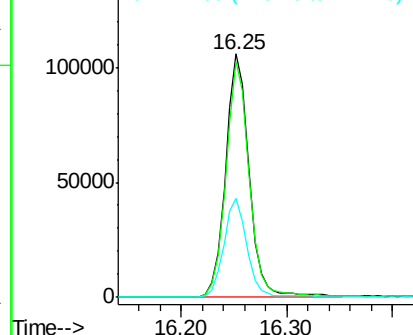



#45
 2-Fluorobiphenyl
 Concen: 77.556 ng
 RT: 13.39 min Scan# 1753
 Delta R.T. -0.03 min
 Lab File: BG040138.D
 Acq: 26 Mar 2019 6:12

Tgt Ion:172 Resp: 670790
 Ion Ratio Lower Upper
 172 100
 171 37.0 30.8 46.2
 170 24.9 20.2 30.4

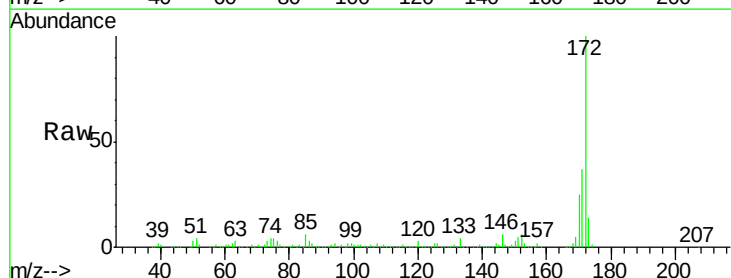

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

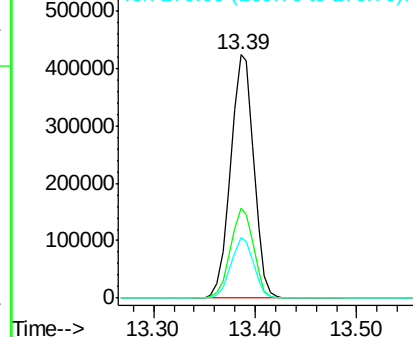







#64
 Phenanthrene-d10
 Concen: 20.000 ng
 RT: 17.51 min Scan# 2455
 Delta R.T. -0.02 min
 Lab File: BG040138.D
 Acq: 26 Mar 2019 6:12

Instrument :
 BNA_G
 ClientSampleId :
 CS-4

Tgt Ion:188 Resp: 317191
 Ion Ratio Lower Upper
 188 100
 94 7.5 6.9 10.3
 80 8.5 8.1 12.1

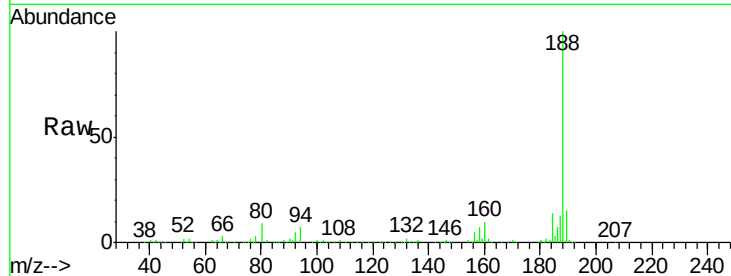


Abundance Ion 188.00 (187.70 to 188.70): E
 Ion 94.00 (93.70 to 94.70): BGC
 Ion 80.00 (79.70 to 80.70): BGC

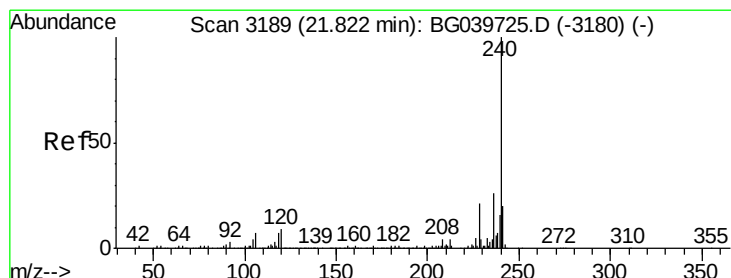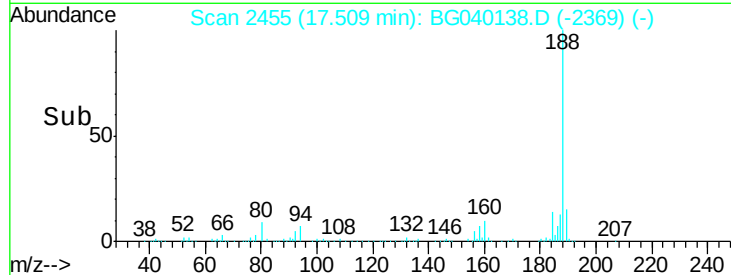
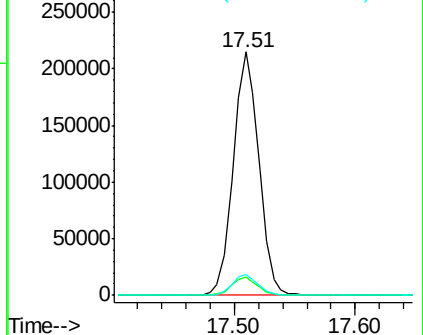



#76
 Chrysene-d12
 Concen: 20.000 ng
 RT: 21.80 min Scan# 3185
 Delta R.T. -0.03 min
 Lab File: BG040138.D
 Acq: 26 Mar 2019 6:12

Tgt Ion:240 Resp: 330593
 Ion Ratio Lower Upper
 240 100
 120 7.4 7.0 10.6
 236 26.3 21.0 31.4

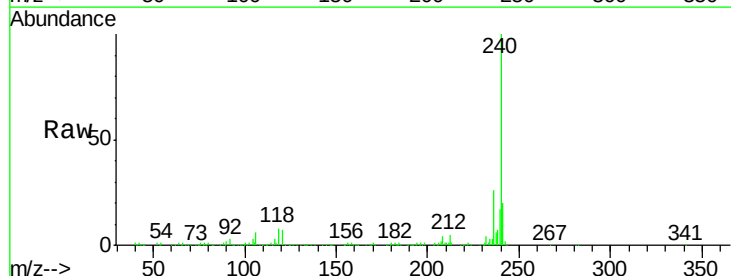

Abundance Ion 240.00 (239.70 to 240.70): E
 Ion 120.00 (119.70 to 120.70): E
 Ion 236.00 (235.70 to 236.70): E

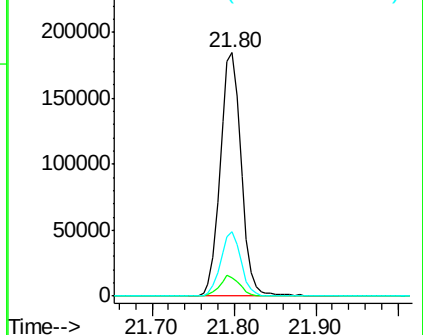

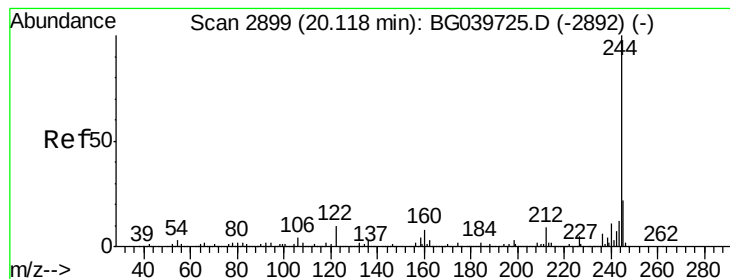

#79

Terphenyl-d14

Concen: 79.489 ng

RT: 20.11 min Scan# 2897

Delta R.T. -0.02 min

Lab File: BG040138.D

Acq: 26 Mar 2019 6:12

Instrument :

BNA_G

ClientSampled :

CS-4


Tgt Ion:244 Resp: 1193501

Ion Ratio Lower Upper

244 100

212 8.9 7.3 10.9




122 9.4 8.4 12.6

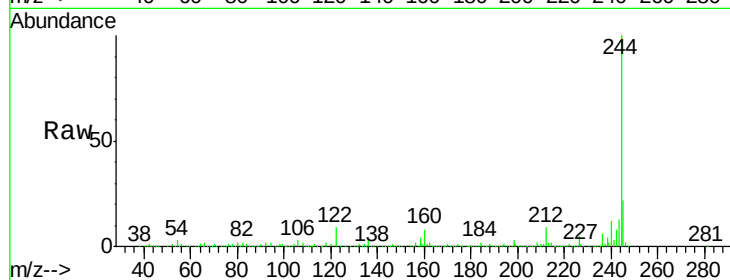

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

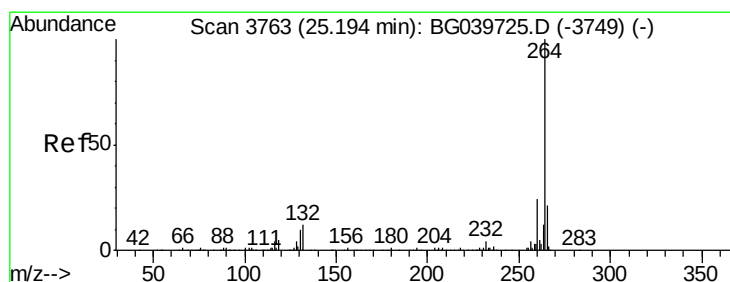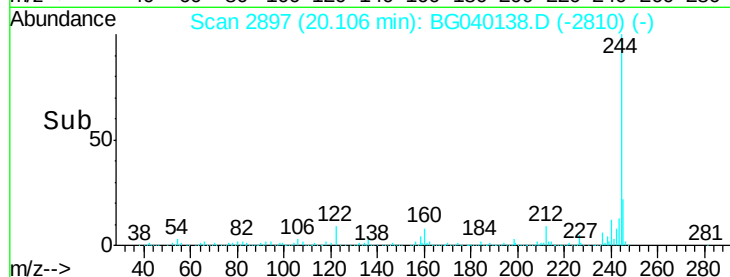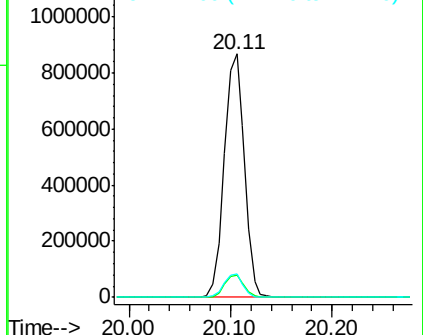

#87

Perylene-d12

Concen: 20.000 ng

RT: 25.15 min Scan# 3756

Delta R.T. -0.05 min

Lab File: BG040138.D

Acq: 26 Mar 2019 6:12


Tgt Ion:264 Resp: 306556

Ion Ratio Lower Upper

264 100

260 23.9 18.2 27.4

265 20.2 18.5 27.7

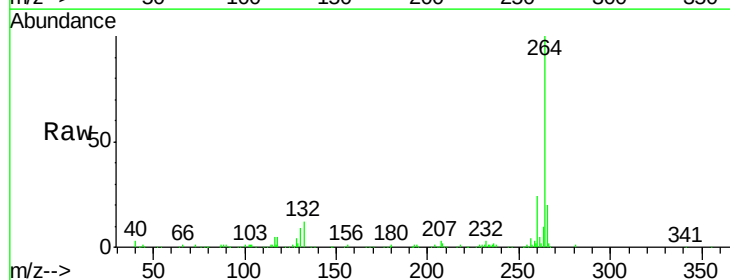

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

