


Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG032519\
 Data File : BG040115.D
 Acq On : 25 Mar 2019 13:32
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG030419.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Mar 04 14:38:15 2019

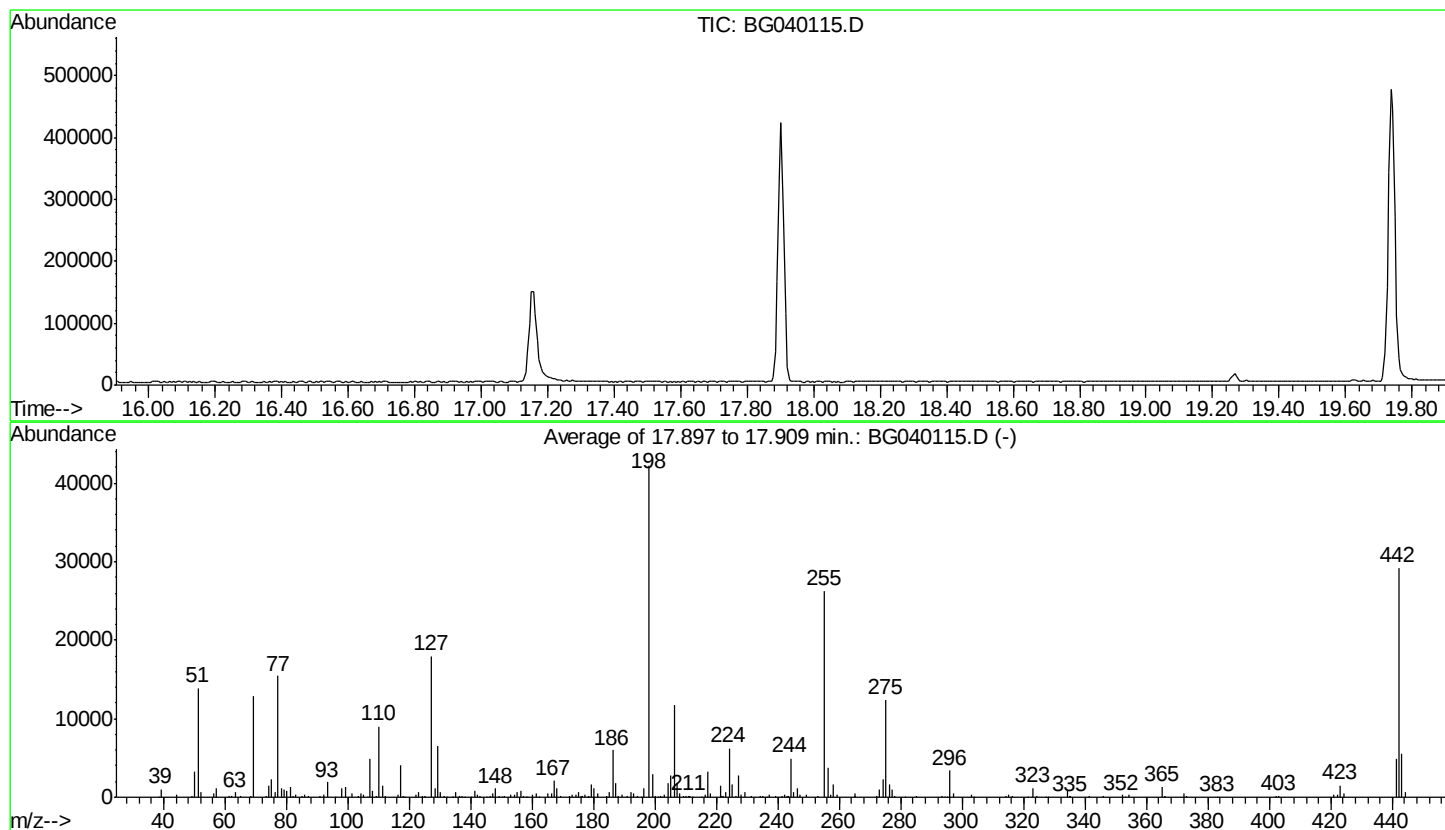

AutoFind: Scans 2521, 2522, 2523; Background Corrected with Scan 2515

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.0	13940	PASS
68	69	0.00	2	0.7	88	PASS
69	198	0.00	100	30.6	12920	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	42.5	17938	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	42232	PASS
199	198	5	9	6.9	2902	PASS
275	198	10	60	29.5	12474	PASS
365	198	1	100	3.3	1390	PASS
441	198	0.01	100	11.4	4818	PASS
442	198	50	100	69.3	29256	PASS
443	442	15	24	18.8	5513	PASS