
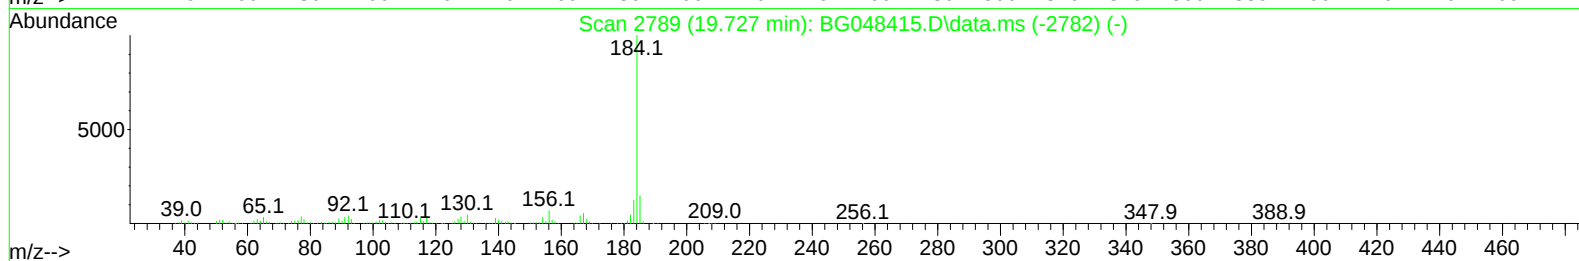
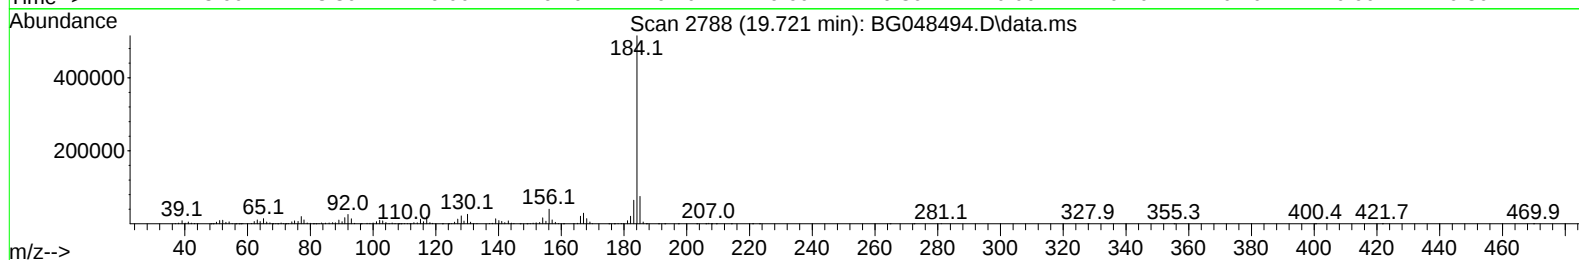


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032521\
Data File : BG048494.D
Acq On : 25 Mar 2021 9:23
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 25 11:54:08 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG031821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 25 02:47:17 2021
Response via : Initial Calibration

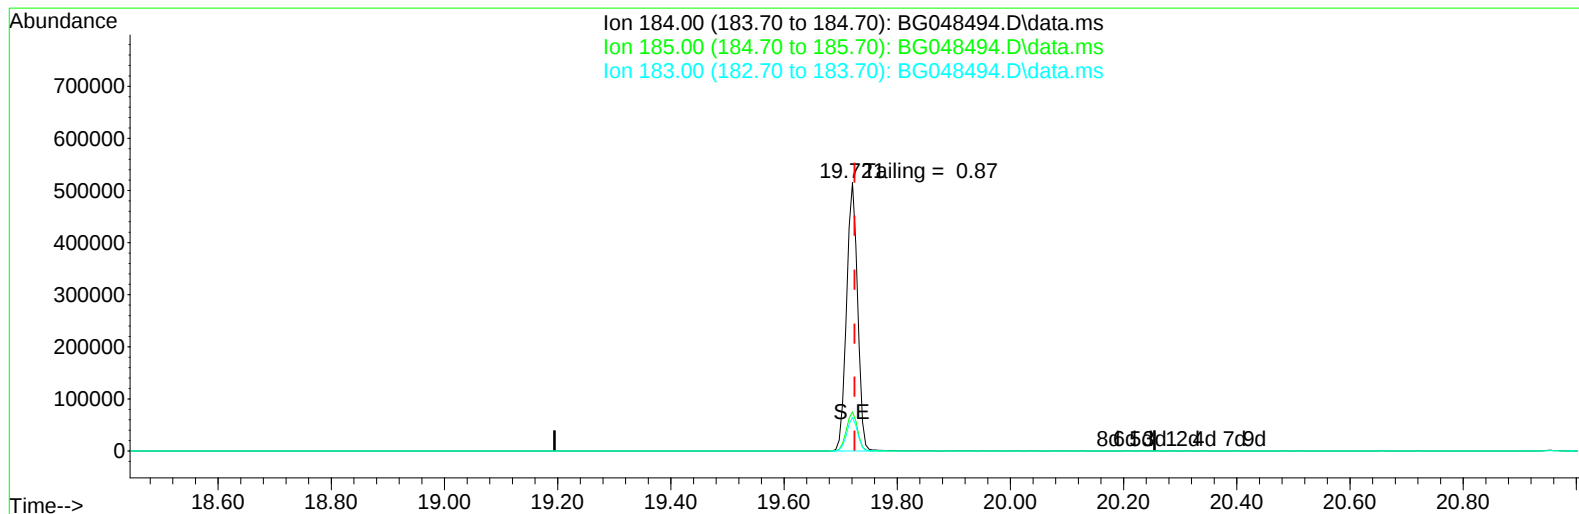

TIC: BG048494.D\data.ms

(77) Benzidine




19.721min (-0.003) 327369.62 ng m

response 696247

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.61
183.00	13.20	12.56
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032521\
Data File : BG048494.D
Acq On : 25 Mar 2021 9:23
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 25 11:54:08 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG031821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 25 02:47:17 2021
Response via : Initial Calibration

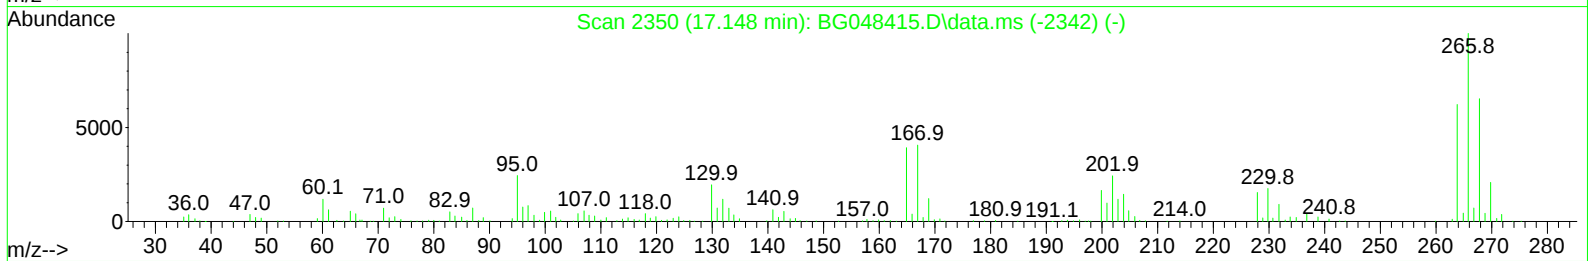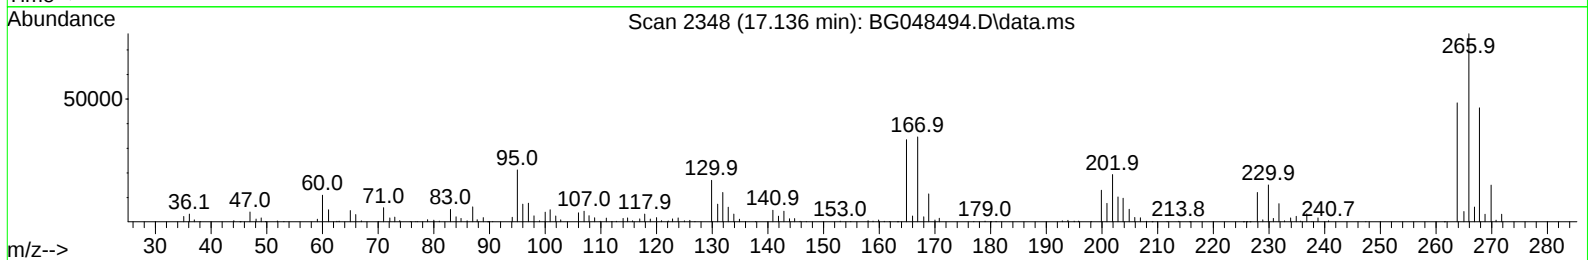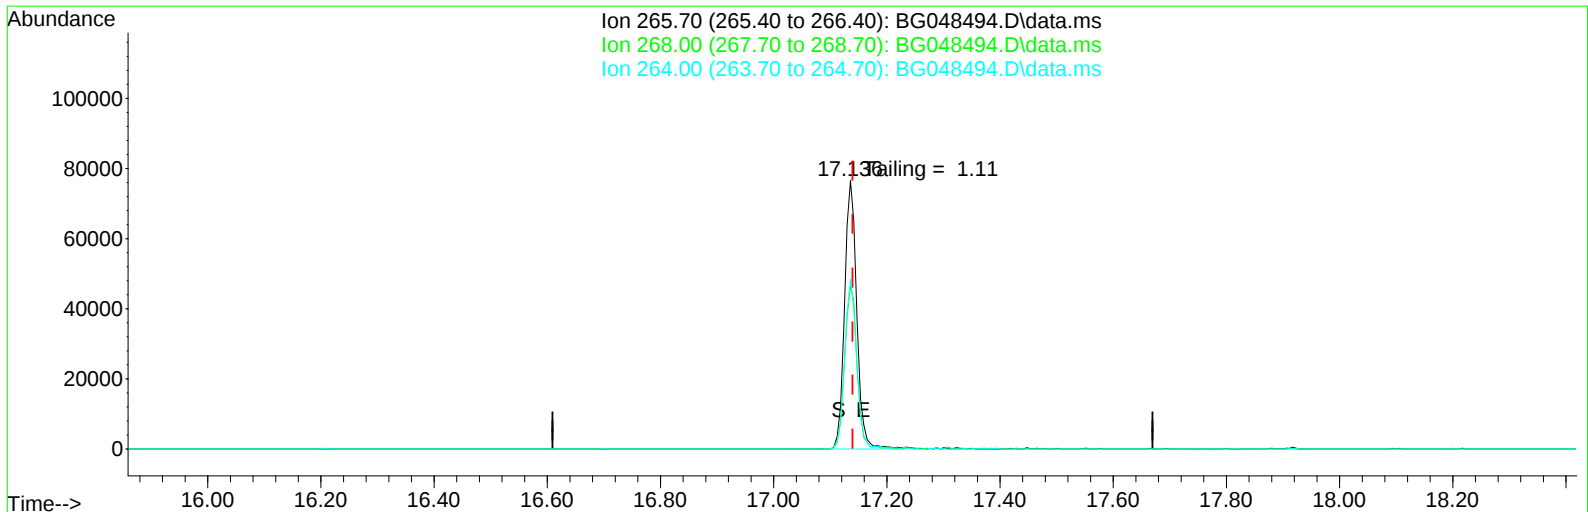

TIC: BG048494.D\data.ms

(70) Pentachlorophenol (C)

17.136min (-0.003) 22261.13 ng

response 113436

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	60.69
264.00	61.60	63.29
0.00	0.00	0.00