
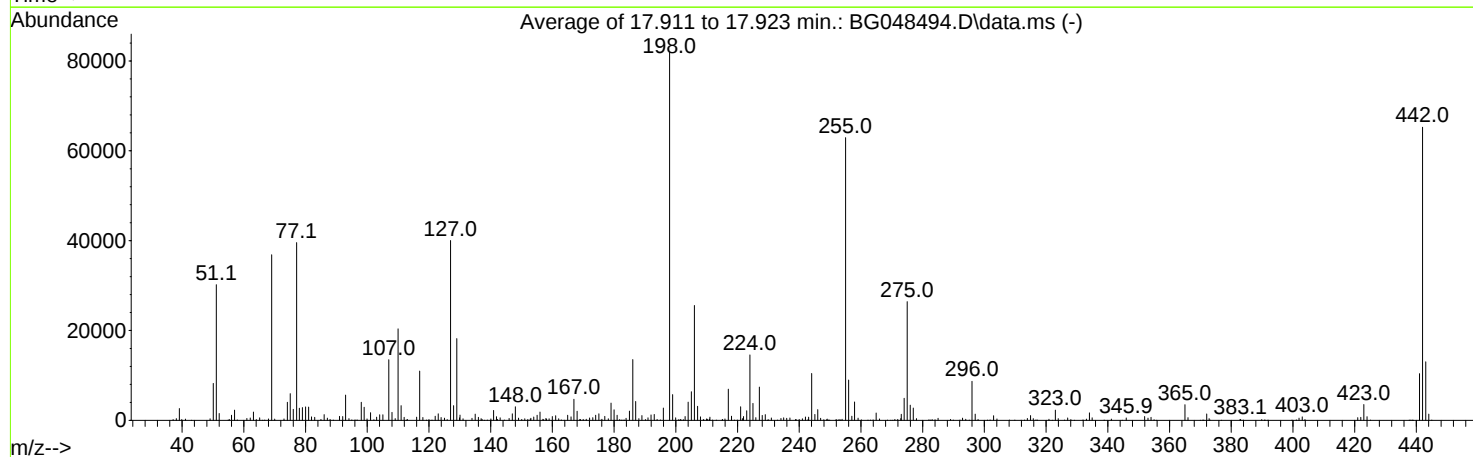


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032521\
 Data File : BG048494.D
 Acq On : 25 Mar 2021 9:23
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG031821.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Mar 25 02:47:17 2021

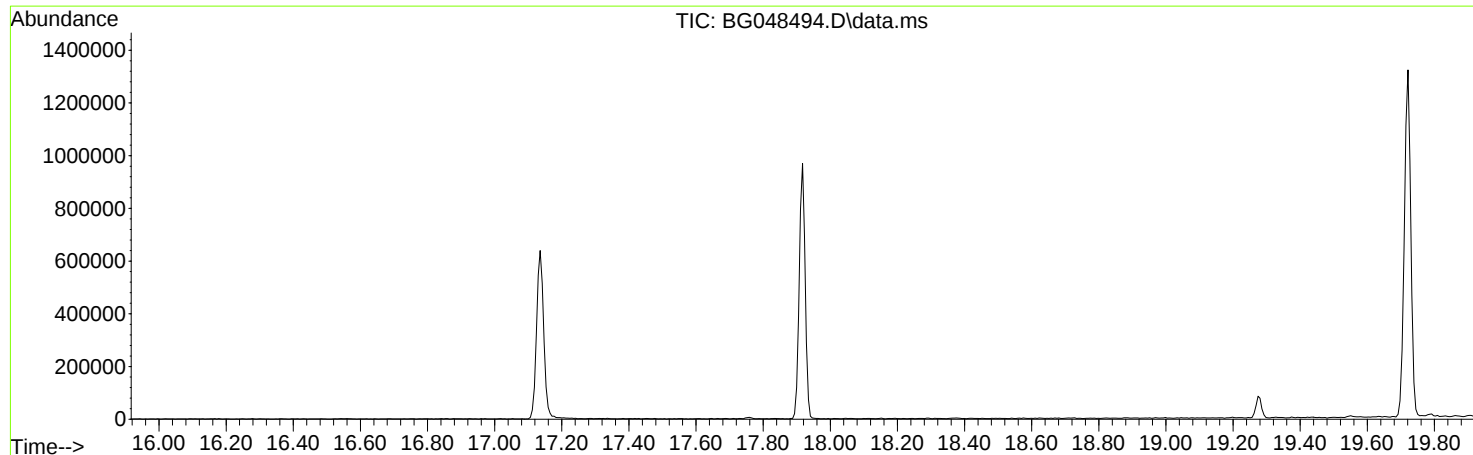

AutoFind: Scans 2480, 2481, 2482; Background Corrected with Scan 2473

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.9	30219	PASS
68	69	0.00	2	0.9	333	PASS
69	198	0.00	100	45.0	36861	PASS
70	69	0.00	2	0.8	285	PASS
127	198	10	80	48.9	40032	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	81885	PASS
199	198	5	9	7.0	5727	PASS
275	198	10	60	32.3	26421	PASS
365	198	1	100	4.3	3495	PASS
441	198	0.01	100	12.7	10419	PASS
442	198	50	100	79.7	65256	PASS
443	442	15	24	20.0	13030	PASS




DDT Breakdown

Date	Instrument Name	DFTPP Data File
3/25/2021	BNA_G	<u>BG048494.D</u>
Compound Name	Response	Retention Time
DDT	351432	20.95
DDD	2213	20.5
DDE	457	19.99
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
2670	354102	0.75

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032521\
Data File : BG048494.D
Acq On : 25 Mar 2021 9:23
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Mar 25 11:54:08 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG031821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 25 02:47:17 2021
Response via : Initial Calibration

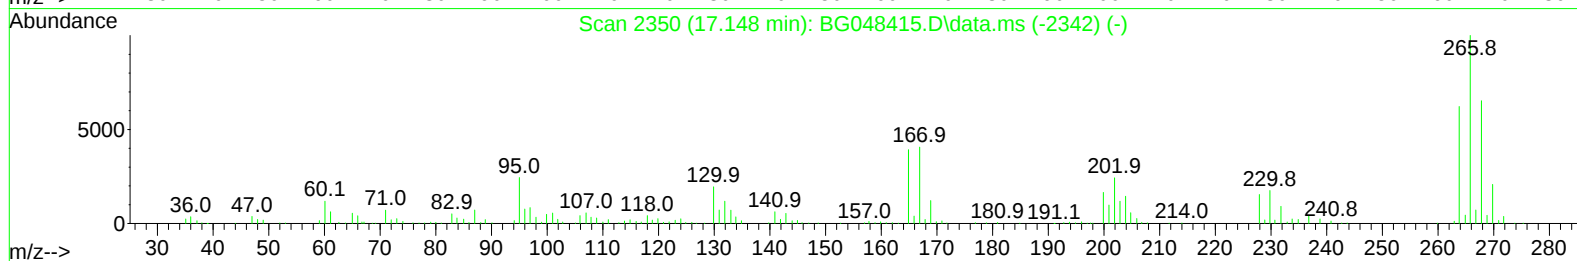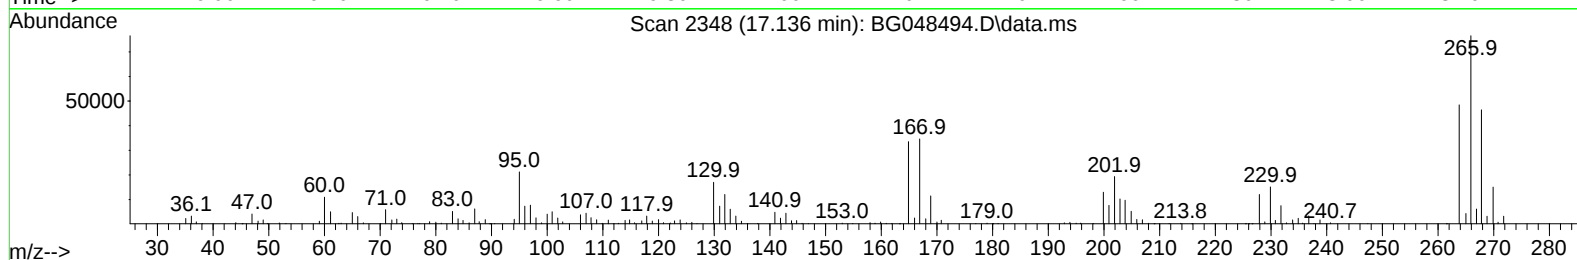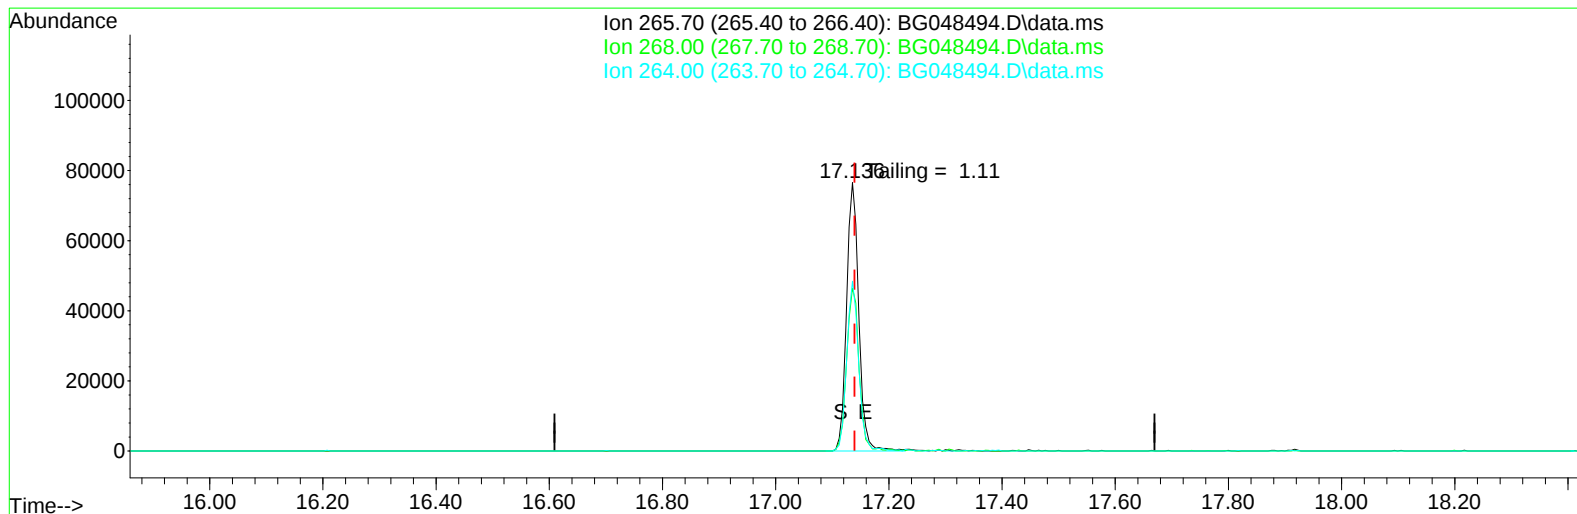

TIC: BG048494.D\data.ms

(70) Pentachlorophenol (C)

17.136min (-0.003) 22261.13 ng




response 113436

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	60.69
264.00	61.60	63.29
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032521\
Data File : BG048494.D
Acq On : 25 Mar 2021 9:23
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Mar 25 11:54:08 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG031821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 25 02:47:17 2021
Response via : Initial Calibration

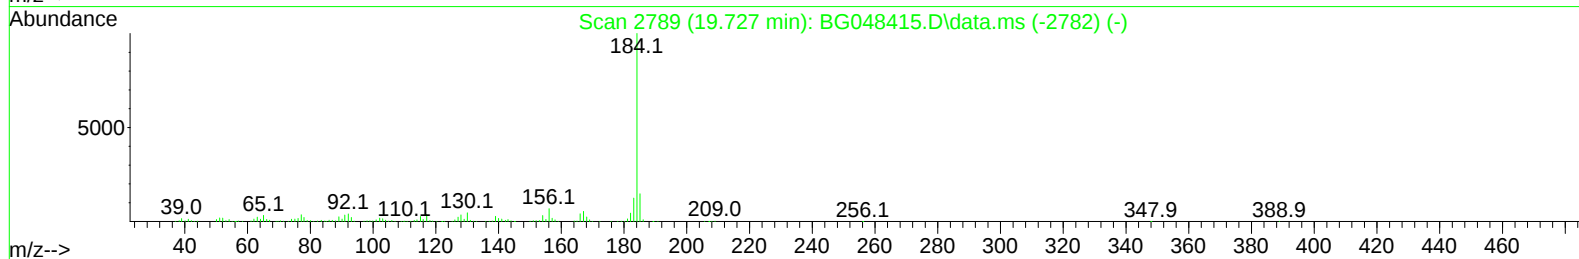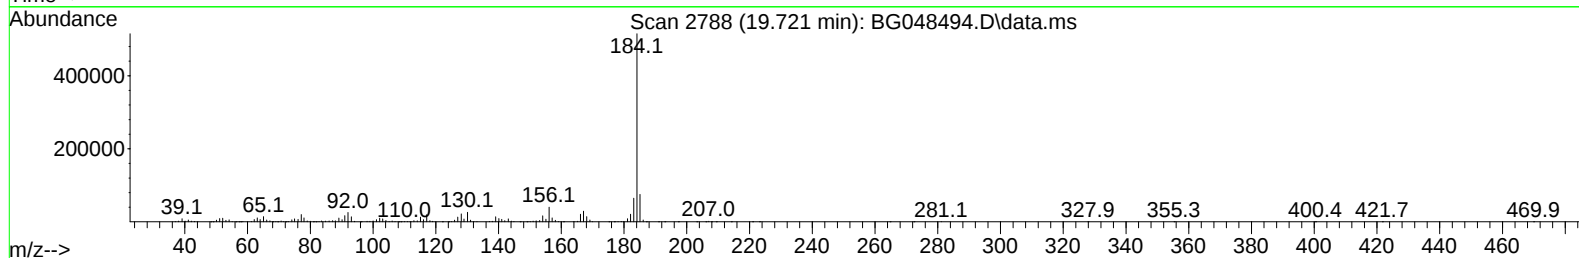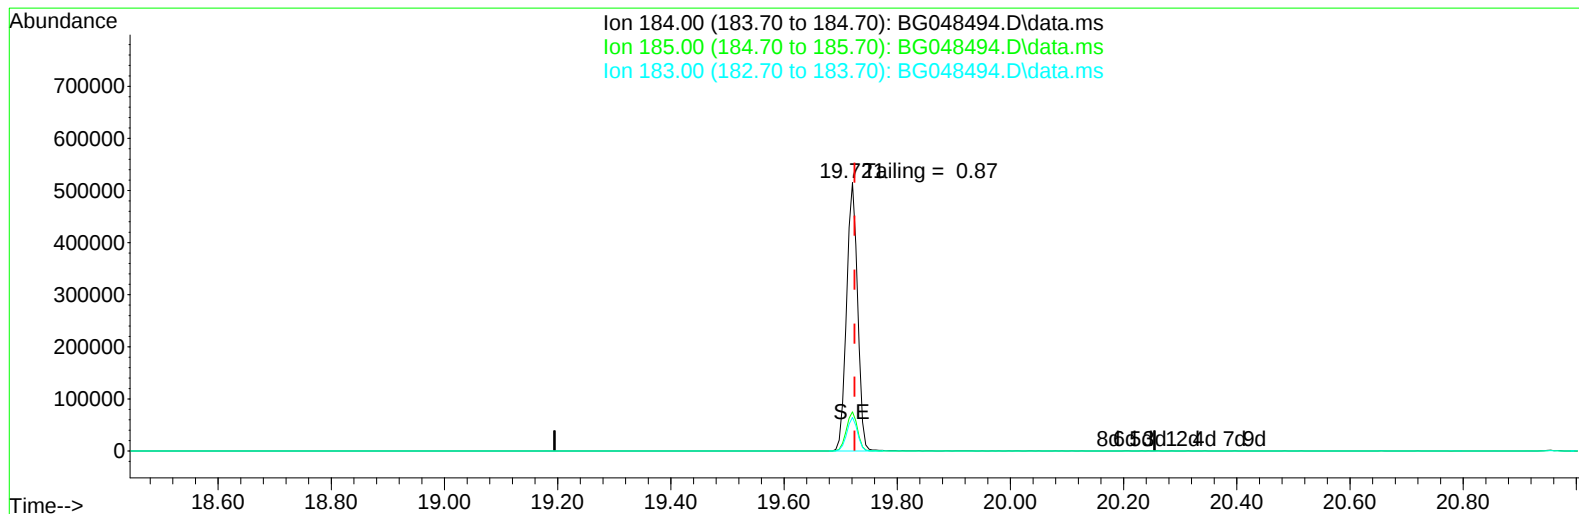

TIC: BG048494.D\data.ms

(77) Benzidine

19.721min (-0.003) 327369.62 ng m

response 696247

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.61
183.00	13.20	12.56
0.00	0.00	0.00