

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG032615\
 Data File : BG016162.D
 Acq On : 27 Mar 2015 5:04
 Operator : TP/IZ
 Sample : G1653-13
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 FD8

Quant Time: Mar 27 15:43:44 2015
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG032515.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Mar 26 15:24:59 2015
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.79	152	51148	20.00	ng	0.00
21) Naphthalene-d8	10.58	136	227161	20.00	ng	0.00
38) Acenaphthene-d10	14.41	164	144015	20.00	ng	0.00
63) Phenanthrene-d10	17.15	188	313689	20.00	ng	0.00
75) Chrysene-d12	21.32	240	326253	20.00	ng	0.00
86) Perylene-d12	23.61	264	315610	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.38	112	351648	115.06	ng	0.00
7) Phenol-d6	6.96	99	504734	118.65	ng	0.00
23) Nitrobenzene-d5	8.94	82	256292	69.96	ng	0.00
41) 2,4,6-Tribromophenol	15.90	330	189648	114.68	ng	0.00
44) 2-Fluorobiphenyl	13.04	172	562189	65.34	ng	0.00
78) Terphenyl-d14	19.78	244	790707	61.04	ng	0.00
Target Compounds						
49) Dimethylphthalate	13.87	163	23150	2.29	ng	Qvalue 97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG032615\
Data File : BG016162.D
Acq On : 27 Mar 2015 5:04
Operator : TP/IZ
Sample : G1653-13
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
FD8

Quant Time: Mar 27 15:43:44 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG032515.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 26 15:24:59 2015
Response via : Initial Calibration

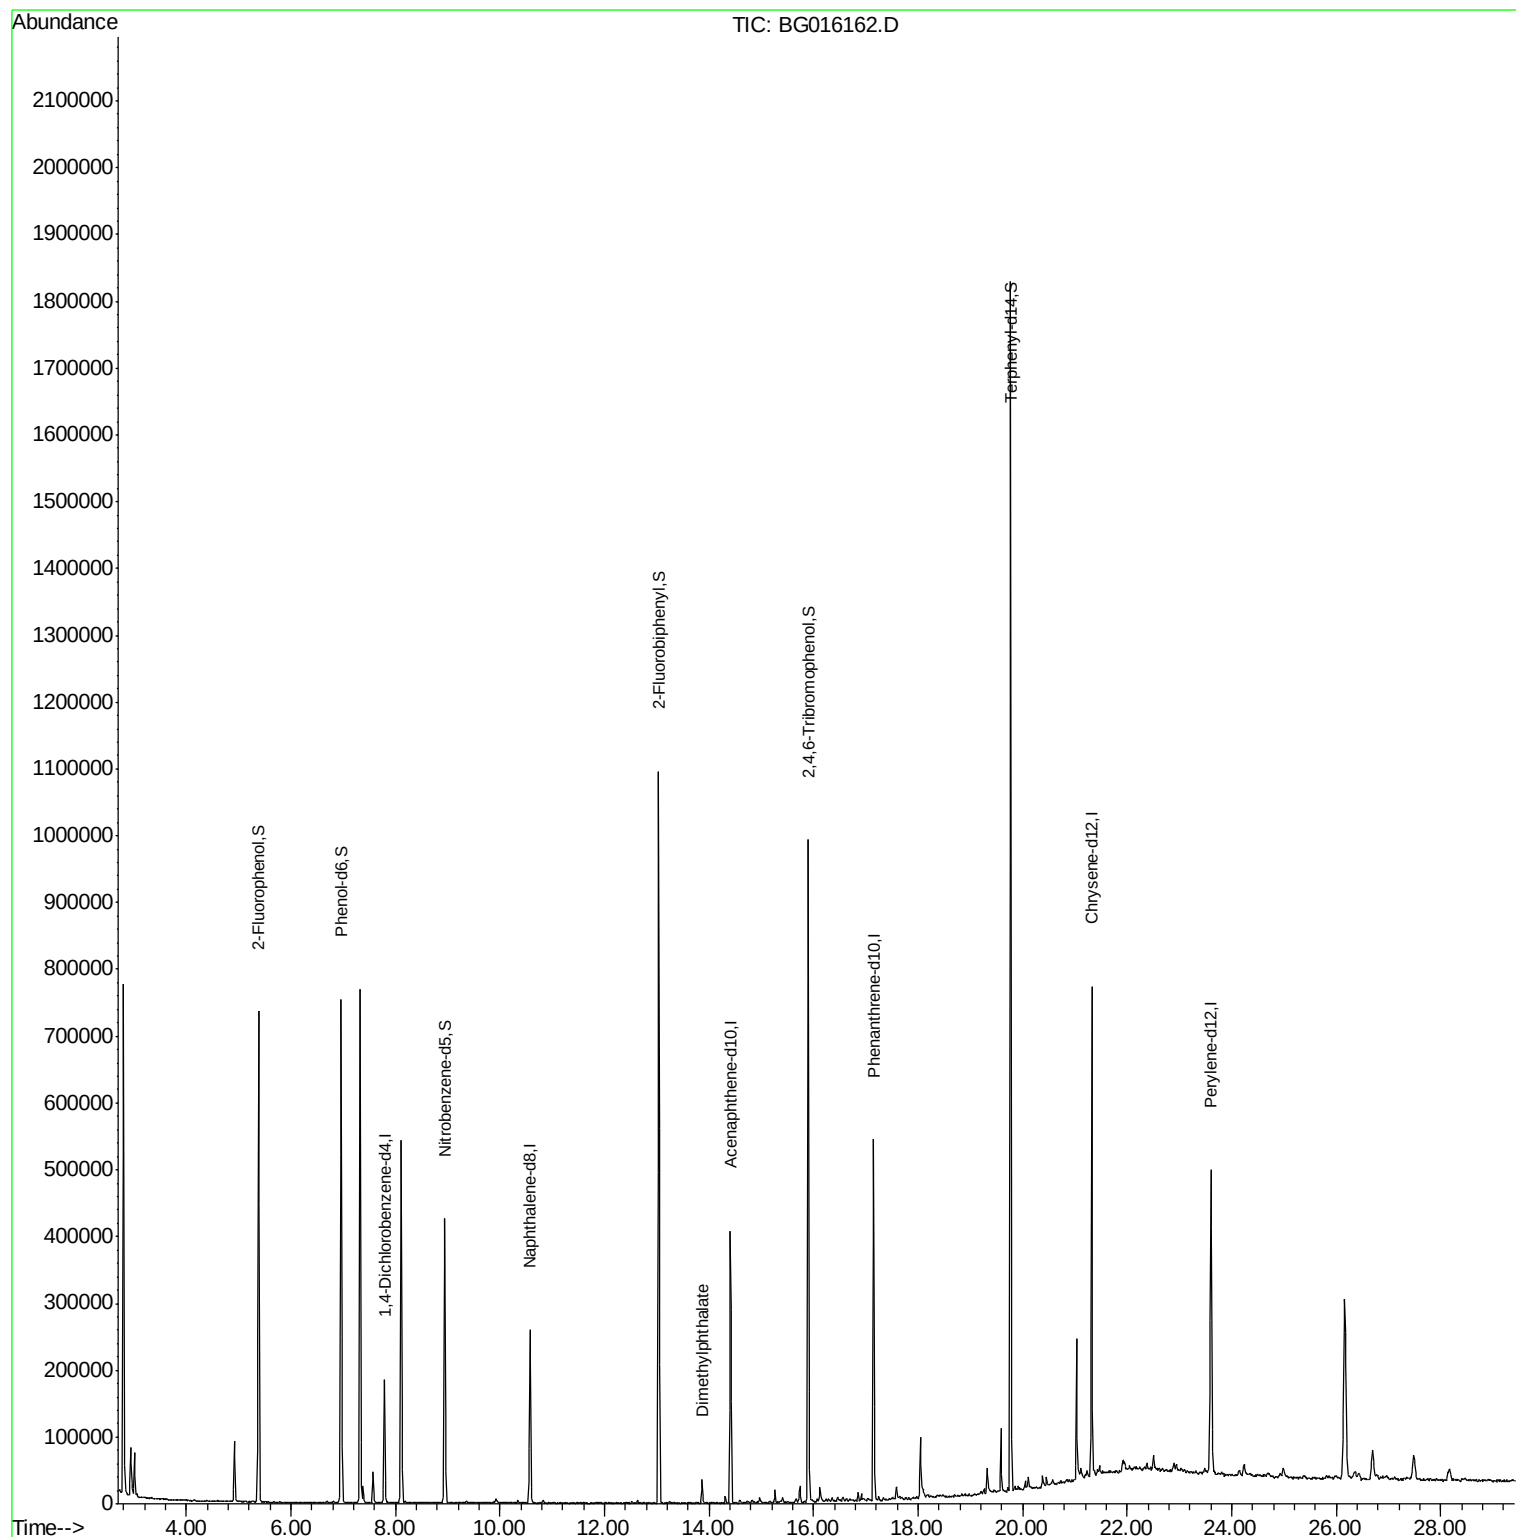

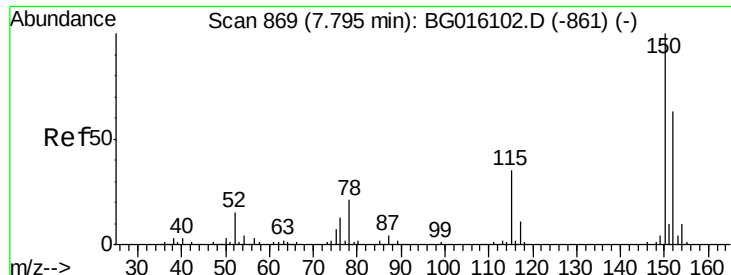

#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 7.79 min Scan# 869

Delta R.T. -0.00 min

Lab File: BG016162.D

Acq: 27 Mar 2015 5:04

Instrument :

BNA_G

ClientSampleId :

FD8


Tgt Ion:152 Resp: 51148

Ion Ratio Lower Upper

152 100

150 156.3 126.1 189.1




115 55.5 43.7 65.5

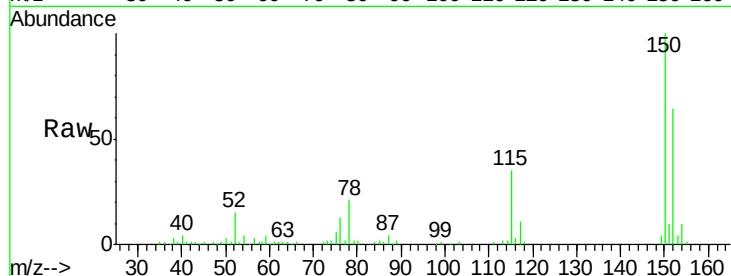

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

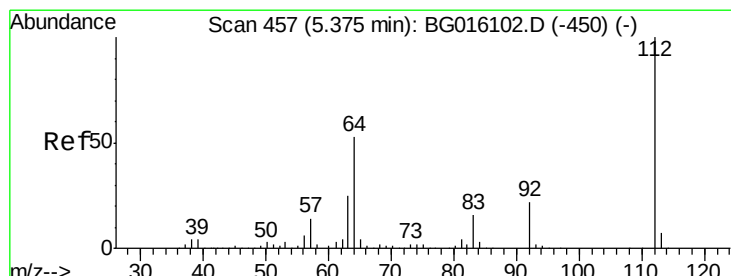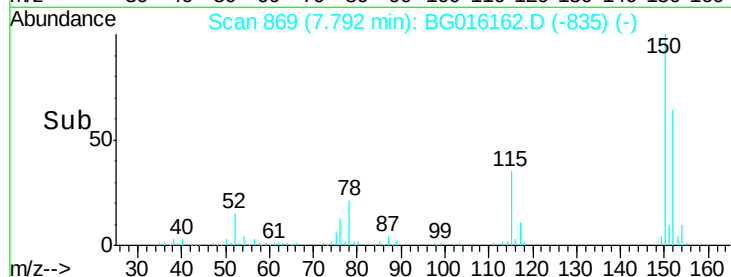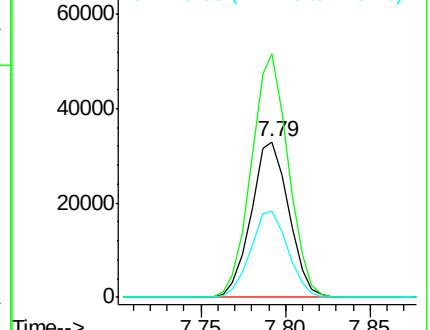

#5

2-Fluorophenol

Concen: 115.06 ng

RT: 5.38 min Scan# 458

Delta R.T. 0.00 min

Lab File: BG016162.D

Acq: 27 Mar 2015 5:04


Tgt Ion:112 Resp: 351648

Ion Ratio Lower Upper

112 100

64 52.5 42.6 64.0



63 24.9 19.9 29.9

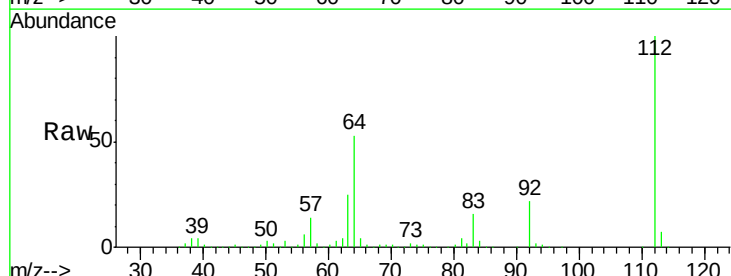


Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BGC

Ion 63.00 (62.70 to 63.70): BGC

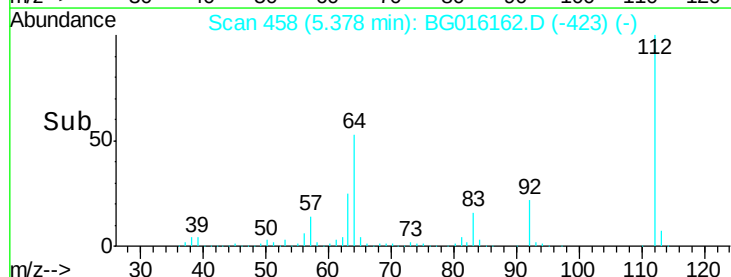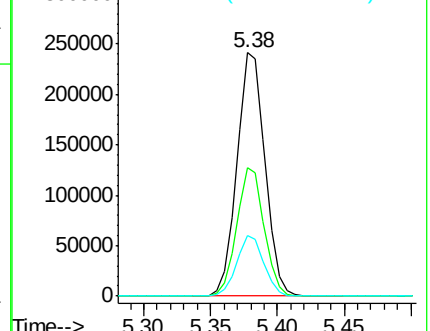

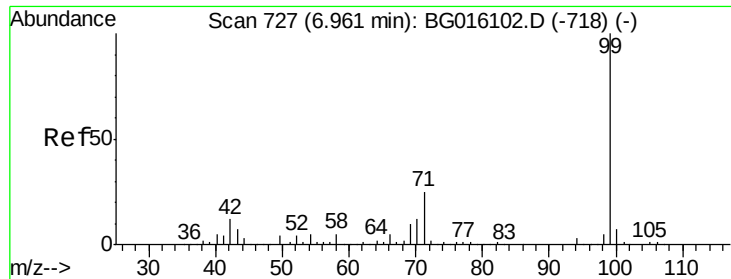

#7

Phenol-d6

Concen: 118.65 ng

RT: 6.96 min Scan# 728

Delta R.T. 0.00 min

Lab File: BG016162.D

Acq: 27 Mar 2015 5:04

Instrument :

BNA_G

ClientSampleId :

FD8


Tgt Ion: 99 Resp: 504734

Ion Ratio Lower Upper




99 100

42 11.5 9.4 14.0

71 25.4 19.9 29.9

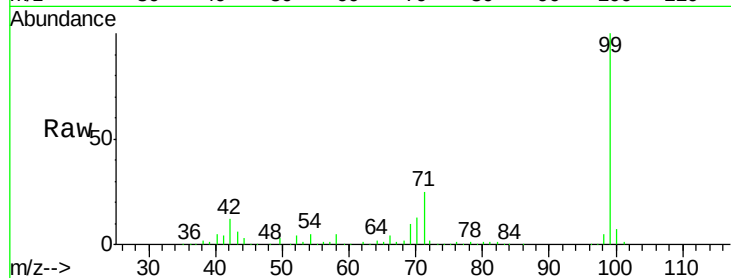

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

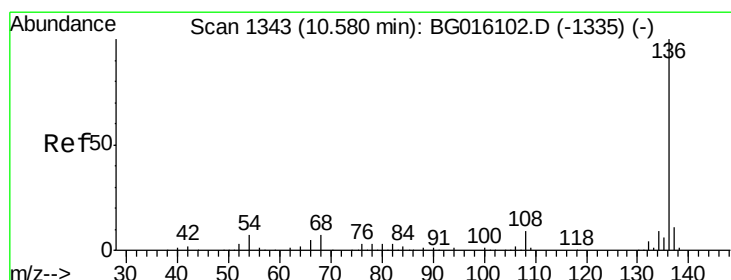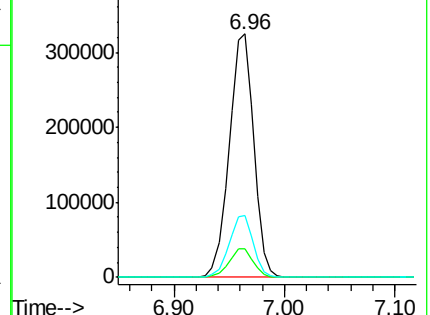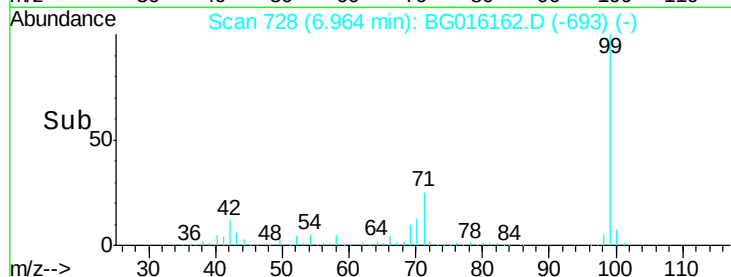

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 10.58 min Scan# 1343

Delta R.T. -0.00 min

Lab File: BG016162.D

Acq: 27 Mar 2015 5:04

Tgt Ion: 136 Resp: 227161


Ion Ratio Lower Upper

136 100



137 11.0 9.0 13.4


54 6.5 5.5 8.3

68 6.9 6.0 9.0

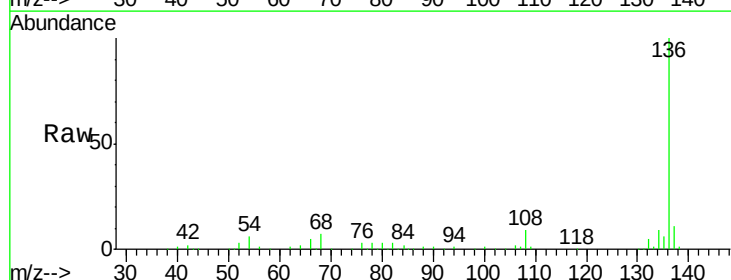

Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC

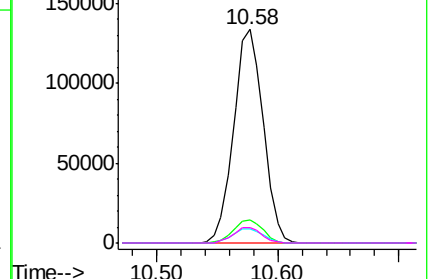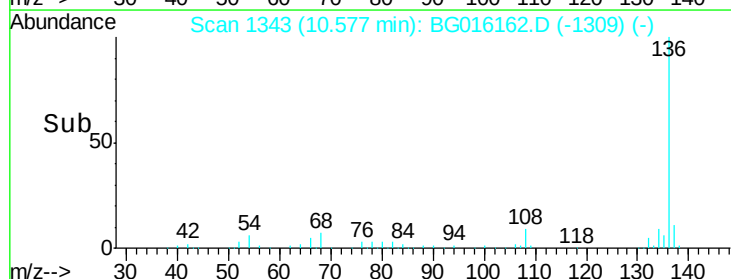


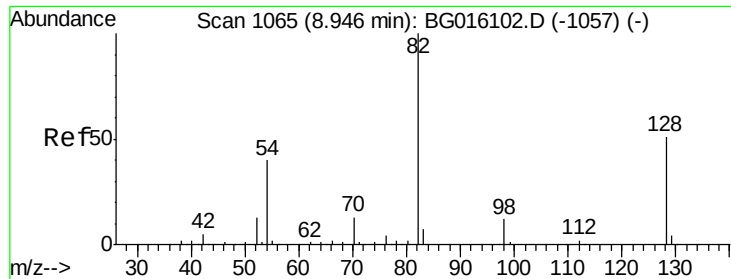




#23
 Nitrobenzene-d5
 Concen: 69.96 ng
 RT: 8.94 min Scan# 1065
 Delta R.T. -0.00 min
 Lab File: BG016162.D
 Acq: 27 Mar 2015 5:04

Instrument :
 BNA_G
 ClientSampleId :
 FD8

Tgt Ion	Ratio	Lower	Upper
82	100		
128	50.9	40.4	60.6
54	39.8	32.1	48.1

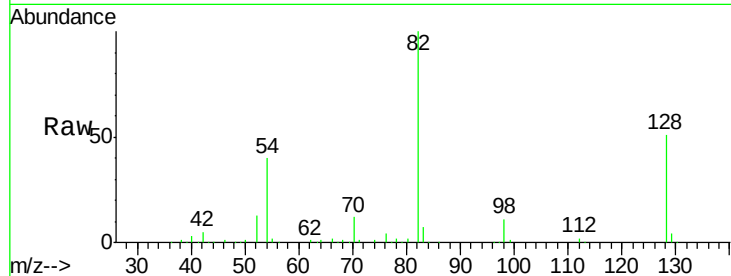


Abundance Ion 82.00 (81.70 to 82.70): BGC
 Ion 128.00 (127.70 to 128.70): BGC
 Ion 54.00 (53.70 to 54.70): BGC

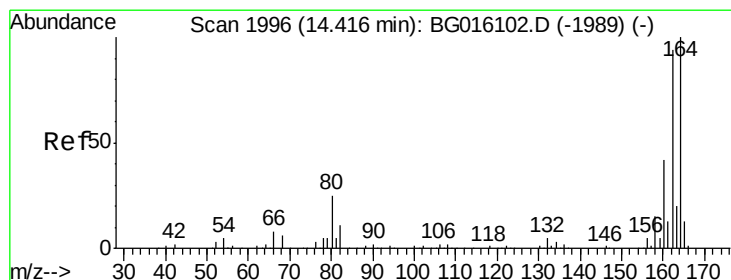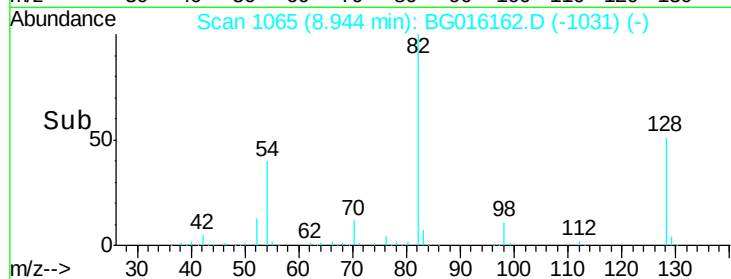
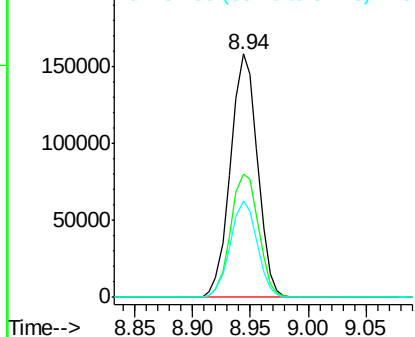



#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 14.41 min Scan# 1996
 Delta R.T. -0.00 min
 Lab File: BG016162.D
 Acq: 27 Mar 2015 5:04

Tgt Ion	Ratio	Lower	Upper
164	100		
162	94.3	75.2	112.8
160	41.4	33.9	50.9

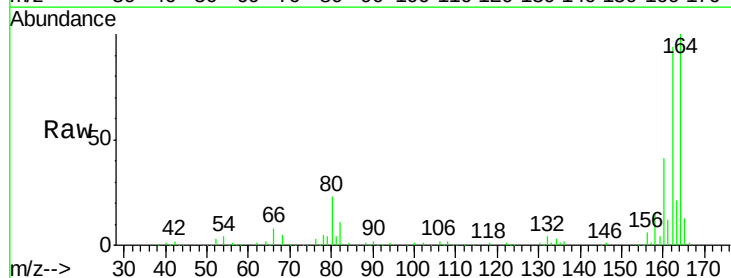

Abundance Ion 164.00 (163.70 to 164.70): BGC
 Ion 162.00 (161.70 to 162.70): BGC
 Ion 160.00 (159.70 to 160.70): BGC

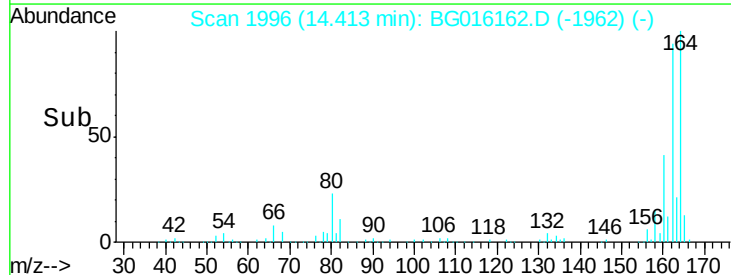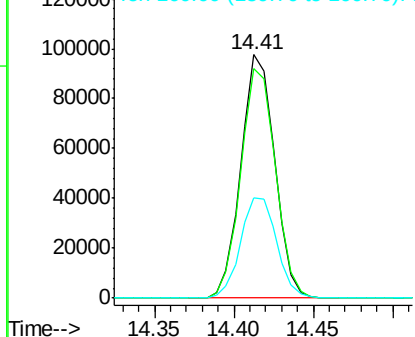


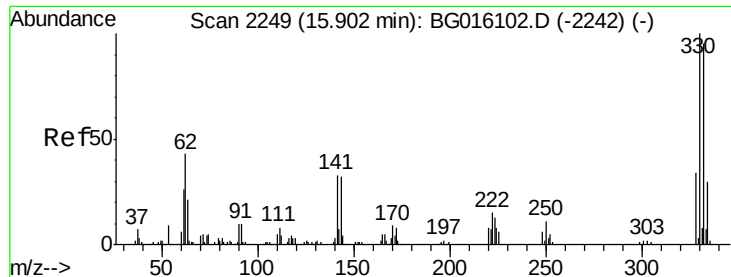




#41
 2,4,6-Tribromophenol
 Concen: 114.68 ng
 RT: 15.90 min Scan# 2249
 Delta R.T. -0.00 min
 Lab File: BG016162.D
 Acq: 27 Mar 2015 5:04

Instrument :
 BNA_G
 ClientSampleId :
 FD8

Tgt Ion:330 Resp: 189648
 Ion Ratio Lower Upper
 330 100
 332 96.1 76.6 114.8
 141 32.1 26.2 39.4

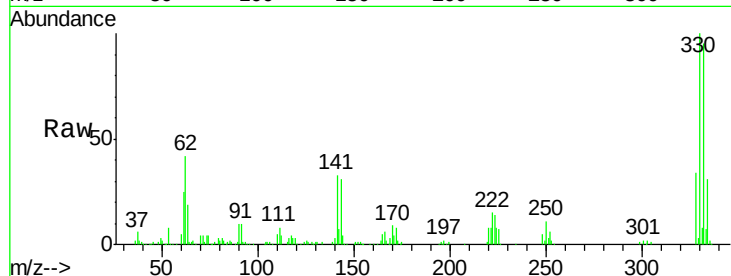


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

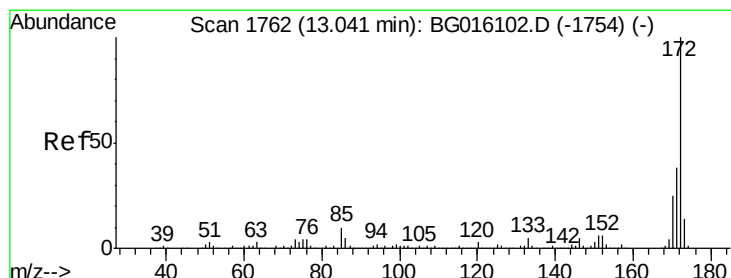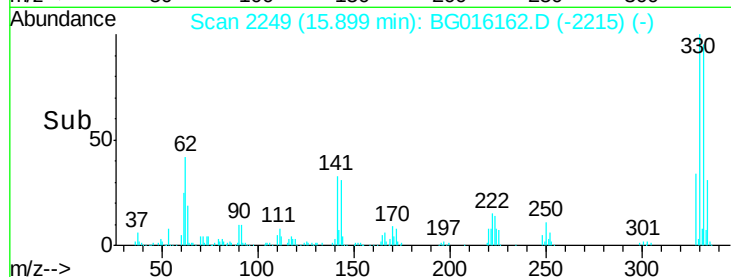
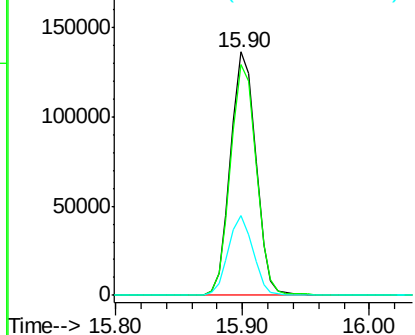



#44
 2-Fluorobiphenyl
 Concen: 65.34 ng
 RT: 13.04 min Scan# 1762
 Delta R.T. -0.00 min
 Lab File: BG016162.D
 Acq: 27 Mar 2015 5:04

Tgt Ion:172 Resp: 562189
 Ion Ratio Lower Upper
 172 100
 171 36.6 30.3 45.5
 170 24.3 19.8 29.8

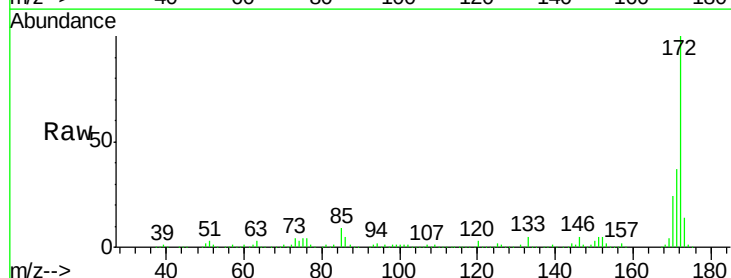

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

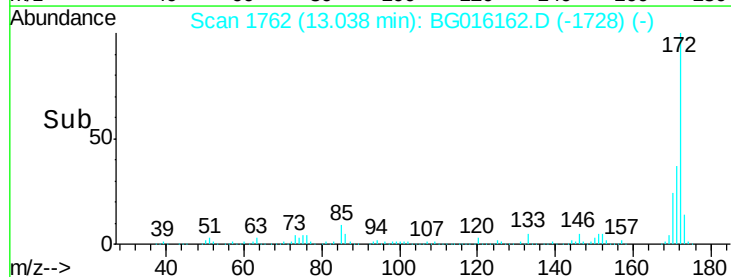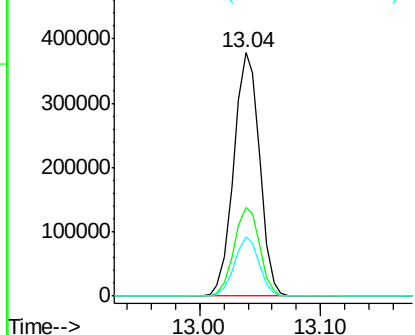

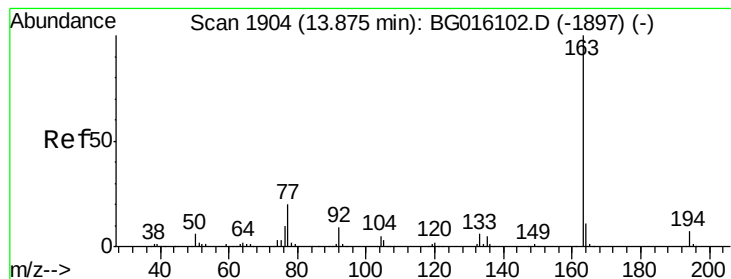

#49

Dimethylphthalate

Concen: 2.29 ng

RT: 13.87 min Scan# 1904

Delta R.T. -0.00 min

Lab File: BG016162.D

Acq: 27 Mar 2015 5:04

Instrument :

BNA_G

ClientSampleId :

FD8


Tgt Ion:163 Resp: 23150

Ion Ratio Lower Upper

163 100

194 5.5 5.4 8.0




164 10.0 8.6 13.0

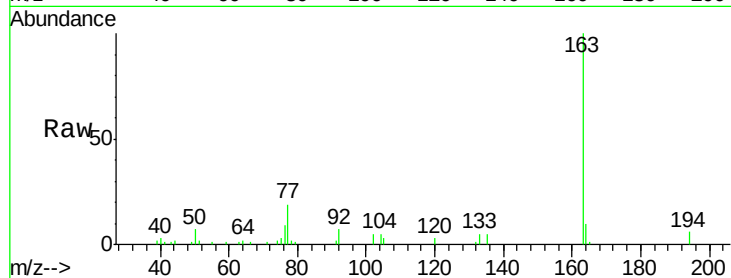

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

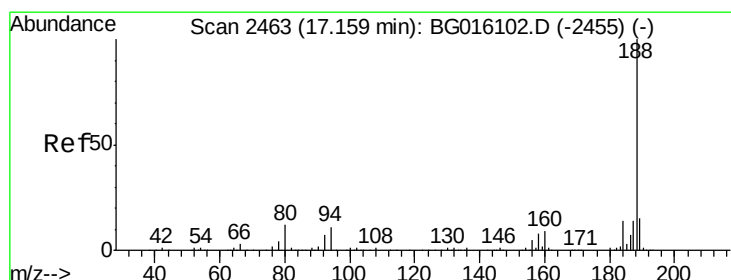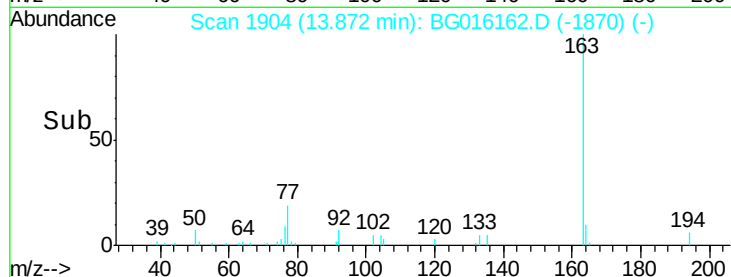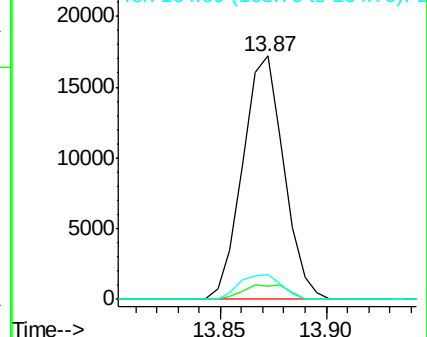

#63

Phenanthrene-d10

Concen: 20.00 ng

RT: 17.15 min Scan# 2462

Delta R.T. -0.01 min

Lab File: BG016162.D

Acq: 27 Mar 2015 5:04


Tgt Ion:188 Resp: 313689

Ion Ratio Lower Upper

188 100

94 12.4 9.1 13.7



80 12.4 9.8 14.8

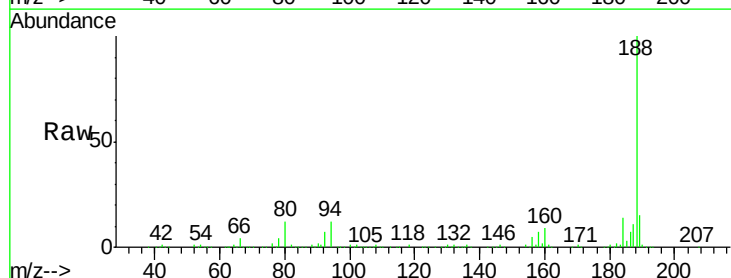


Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BG0

Ion 80.00 (79.70 to 80.70): BG0

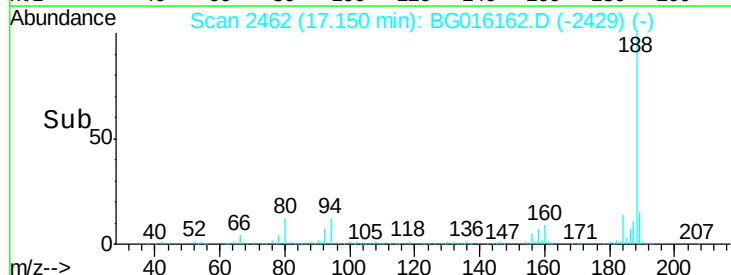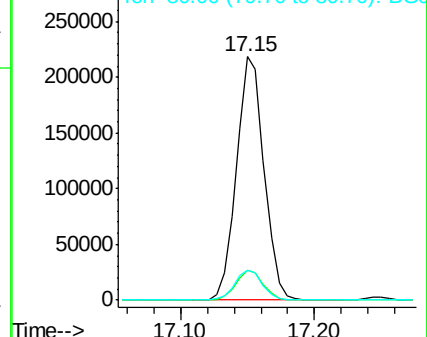

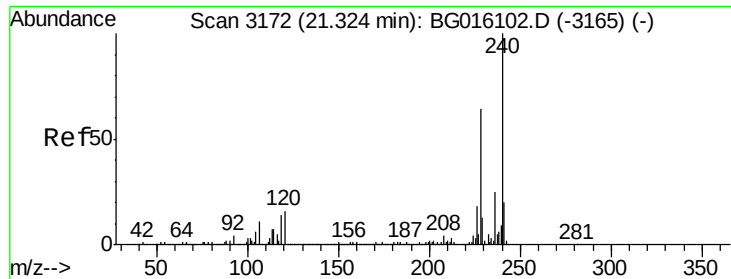

#75

Chrysene-d12

Concen: 20.00 ng

RT: 21.32 min Scan# 3172

Delta R.T. -0.00 min

Lab File: BG016162.D

Acq: 27 Mar 2015 5:04

Instrument :

BNA_G

ClientSampleId :

FD8


Tgt Ion:240 Resp: 326253

Ion Ratio Lower Upper

240 100

120 15.1 13.0 19.4




236 25.9 20.2 30.2

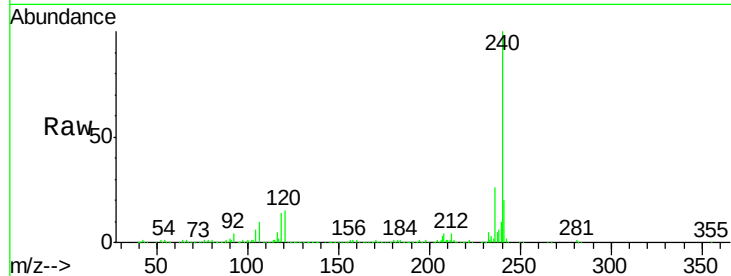

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

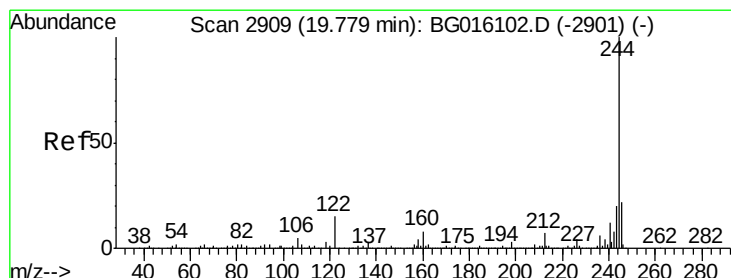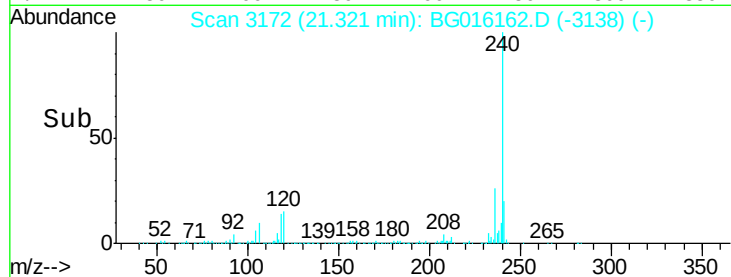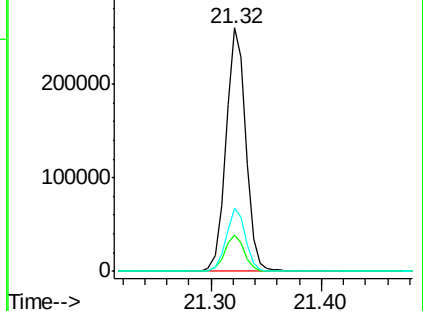

#78

Terphenyl-d14

Concen: 61.04 ng

RT: 19.78 min Scan# 2909

Delta R.T. -0.00 min

Lab File: BG016162.D

Acq: 27 Mar 2015 5:04


Tgt Ion:244 Resp: 790707

Ion Ratio Lower Upper

244 100

212 7.0 5.9 8.9



122 14.6 12.2 18.2

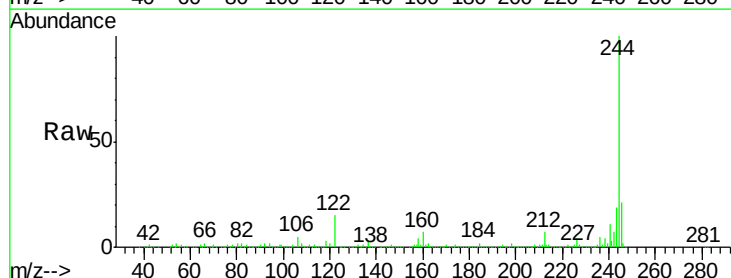


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

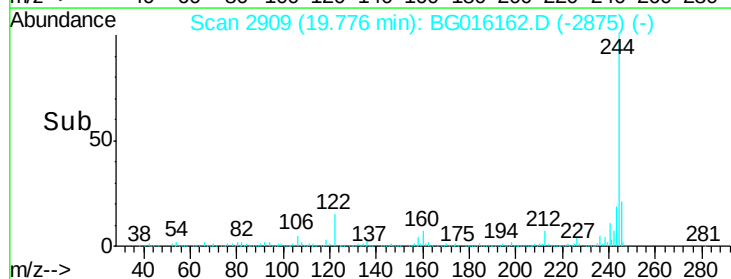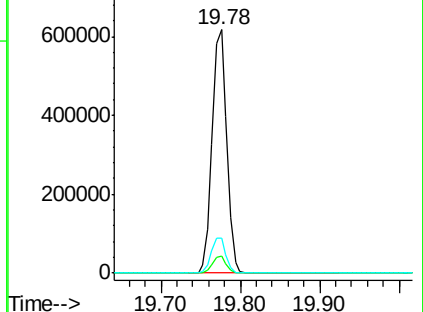

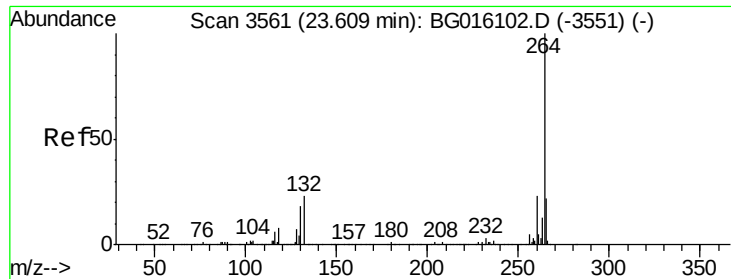

#86
Perylene-d12
Concen: 20.00 ng
RT: 23.61 min Scan# 3561
Delta R.T. -0.00 min
Lab File: BG016162.D
Acq: 27 Mar 2015 5:04

Instrument :
BNA_G
ClientSampleId :
FD8

Tgt Ion	Ratio	Lower	Upper
264	100		
260	23.4	18.4	27.6
265	22.0	17.3	25.9

