


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG032615\
 Data File : BG016136.D
 Acq On : 26 Mar 2015 12:27
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG032515.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Mar 26 15:24:59 2015

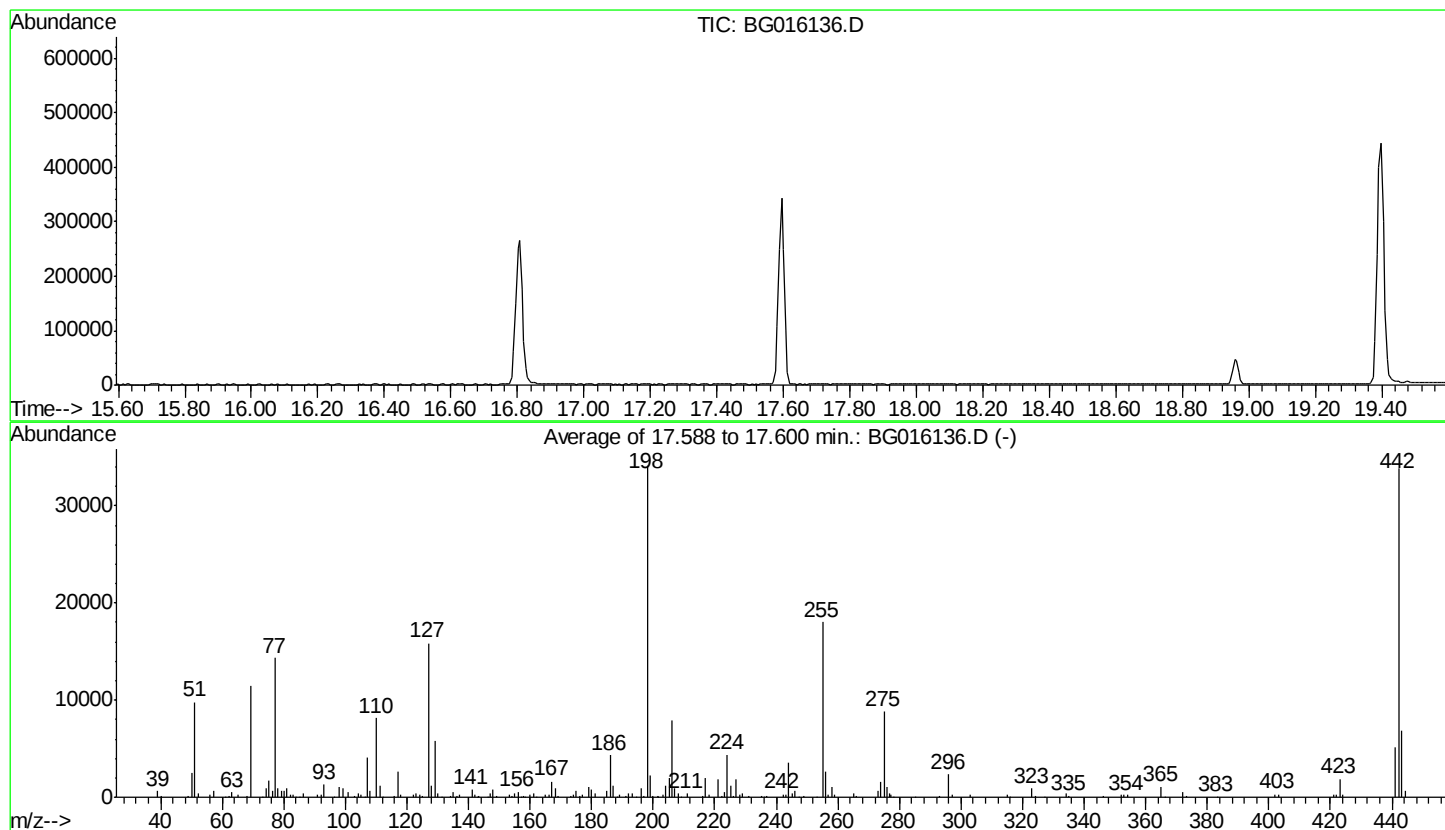

AutoFind: Scans 2536, 2537, 2538; Background Corrected with Scan 2530

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	28.6	9757	PASS
68	69	0.00	2	0.7	82	PASS
69	198	0.00	100	33.7	11505	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	46.5	15878	PASS
197	198	0.00	2	0.3	114	PASS
198	198	100	100	100.0	34141	PASS
199	198	5	9	6.7	2284	PASS
275	198	10	60	25.8	8815	PASS
365	198	1	100	3.2	1096	PASS
441	442	0.01	24	15.3	5183	PASS
442	198	50	100	99.1	33850	PASS
443	442	15	24	20.2	6840	PASS