


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG032615\
 Data File : BG016155.D
 Acq On : 26 Mar 2015 23:51
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG032515.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Mar 26 15:24:59 2015

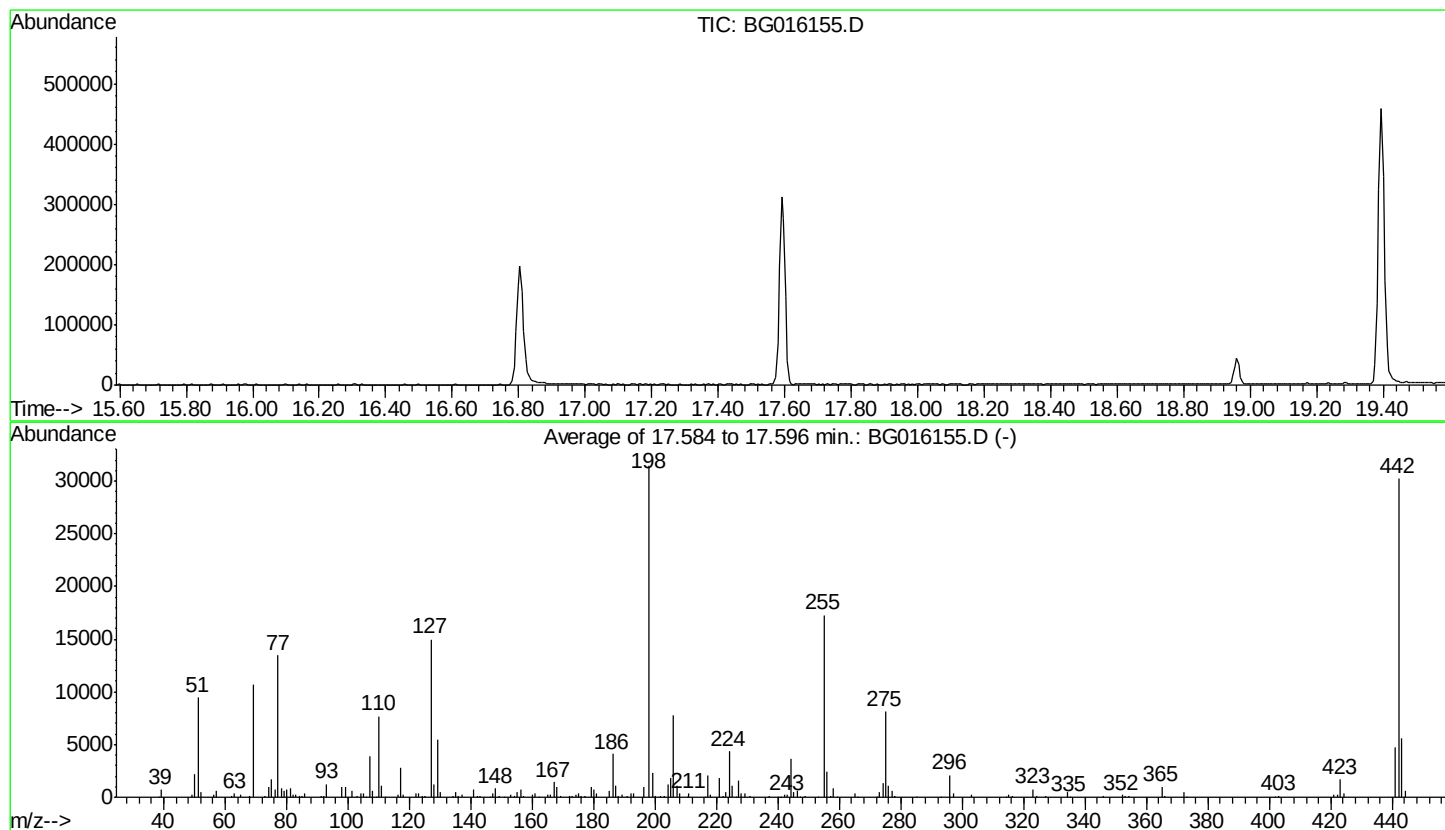

AutoFind: Scans 2536, 2537, 2538; Background Corrected with Scan 2530

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.0	9424	PASS
68	69	0.00	2	0.9	96	PASS
69	198	0.00	100	34.2	10749	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	47.6	14961	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	31458	PASS
199	198	5	9	7.2	2256	PASS
275	198	10	60	25.7	8085	PASS
365	198	1	100	3.2	1010	PASS
441	442	0.01	24	15.7	4751	PASS
442	198	50	100	96.0	30192	PASS
443	442	15	24	18.7	5648	PASS