


Data Path : Z:\HPCHEM1\BNA G\DATA\BG032618\
 Data File : BG033323.D
 Acq On : 26 Mar 2018 11:08
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG031918.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Mar 23 15:11:46 2018



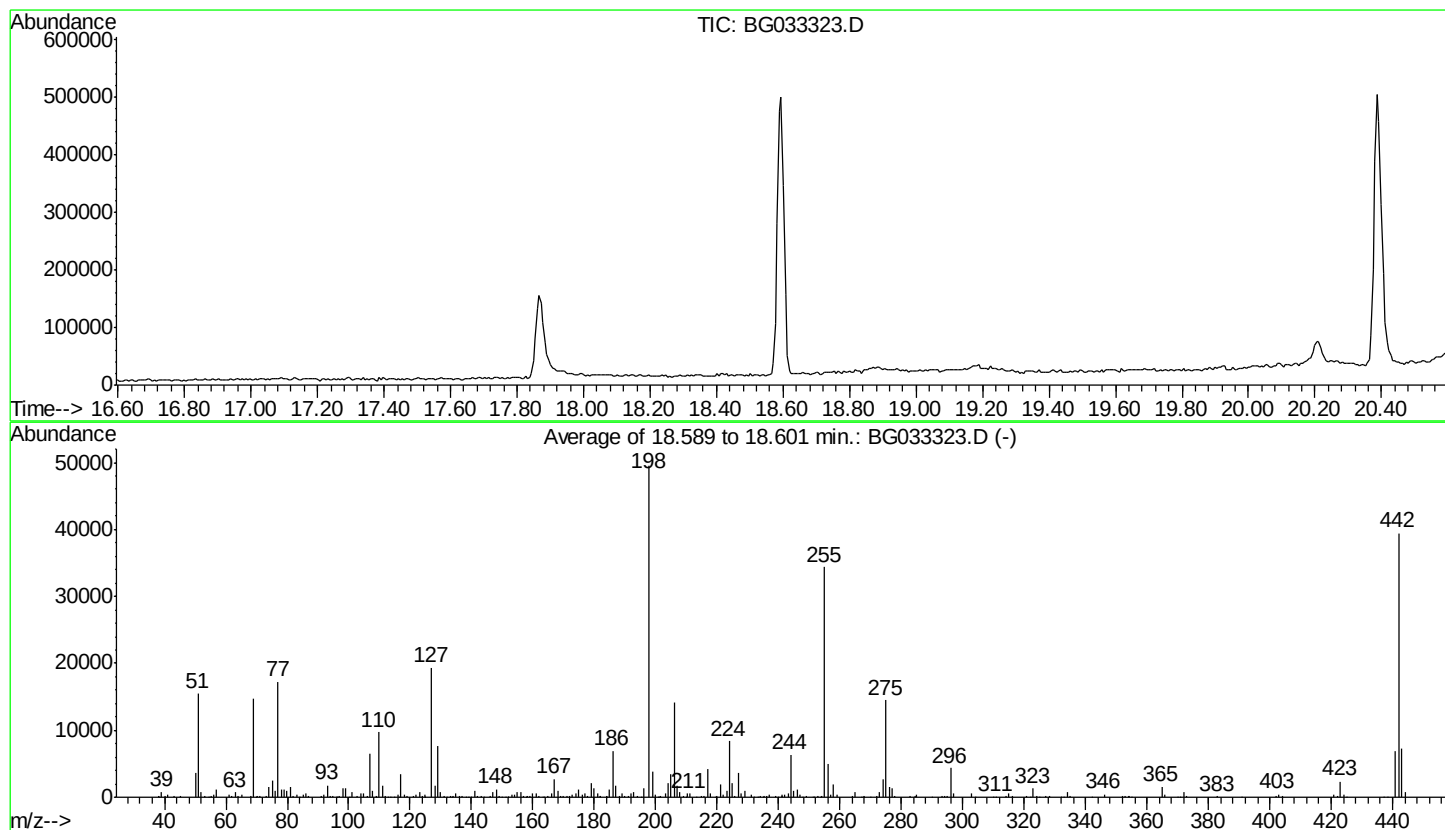


AutoFind: Scans 2604, 2605, 2606; Background Corrected with Scan 2597

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.1	15412	PASS
68	69	0.00	2	1.4	204	PASS
69	198	0.00	100	29.9	14816	PASS
70	69	0.00	2	1.7	249	PASS
127	198	10	80	39.0	19322	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	49541	PASS
199	198	5	9	7.7	3807	PASS
275	198	10	60	29.2	14458	PASS
365	198	1	100	3.3	1617	PASS
441	443	0.01	100	95.7	6902	PASS
442	198	50	100	79.7	39477	PASS
443	442	15	24	18.3	7214	PASS

Data Path : Z:\HPCHEM1\BNA G\DATA\BG032618\
Data File : BG033323.D
Acq On : 26 Mar 2018 11:08
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 27 11:17:11 2018
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG031918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 23 15:11:46 2018
Response via : Initial Calibration

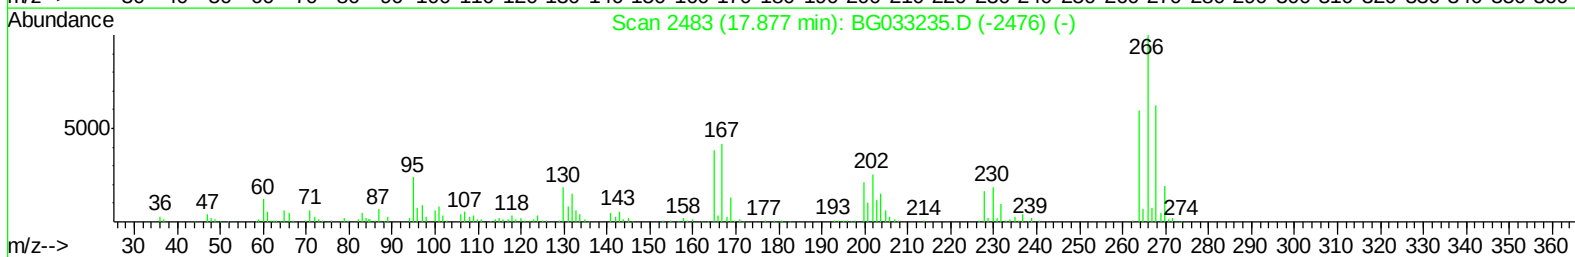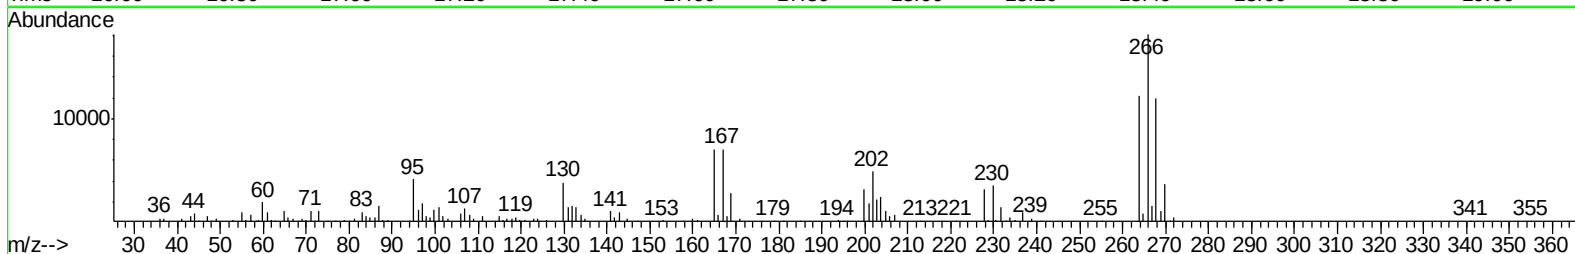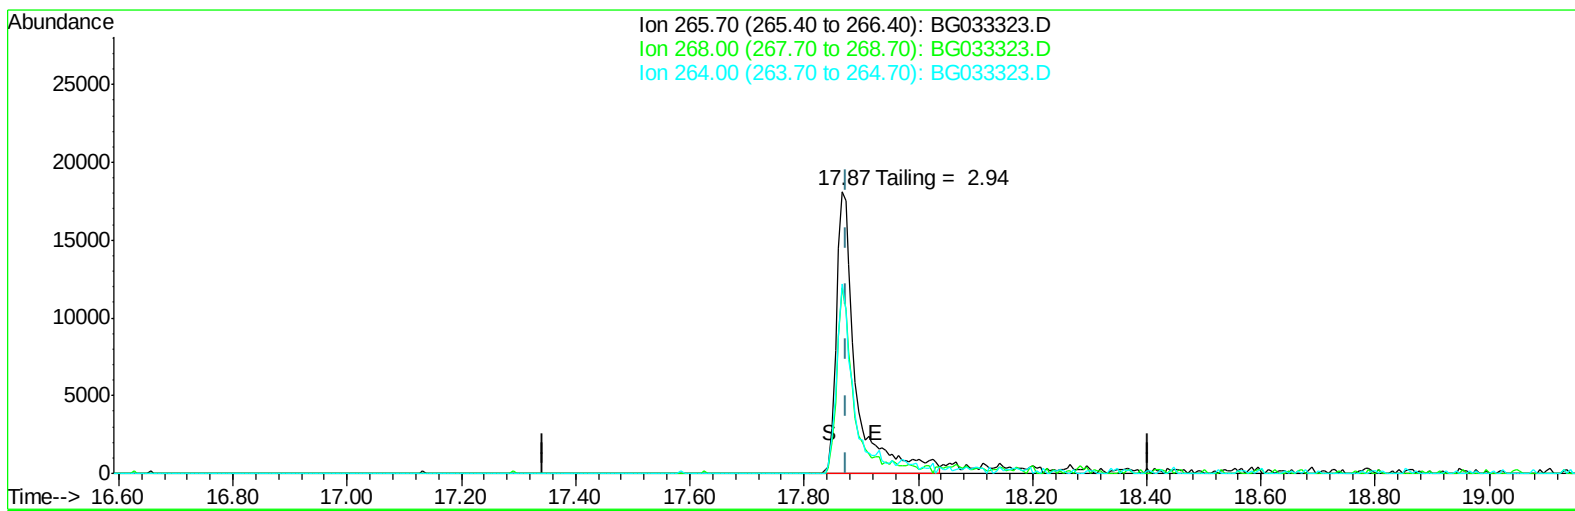

TIC: BG033323.D

(69) Pentachlorophenol (C)




17.866min (-0.008) 70552.04ng

response 40812

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	65.96
264.00	62.00	67.10
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA G\DATA\BG032618\
Data File : BG033323.D
Acq On : 26 Mar 2018 11:08
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 27 11:17:11 2018
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG031918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 23 15:11:46 2018
Response via : Initial Calibration

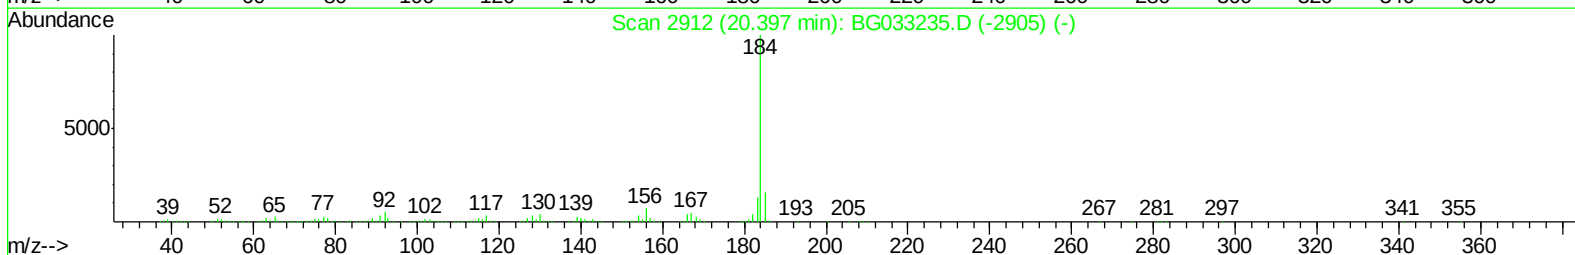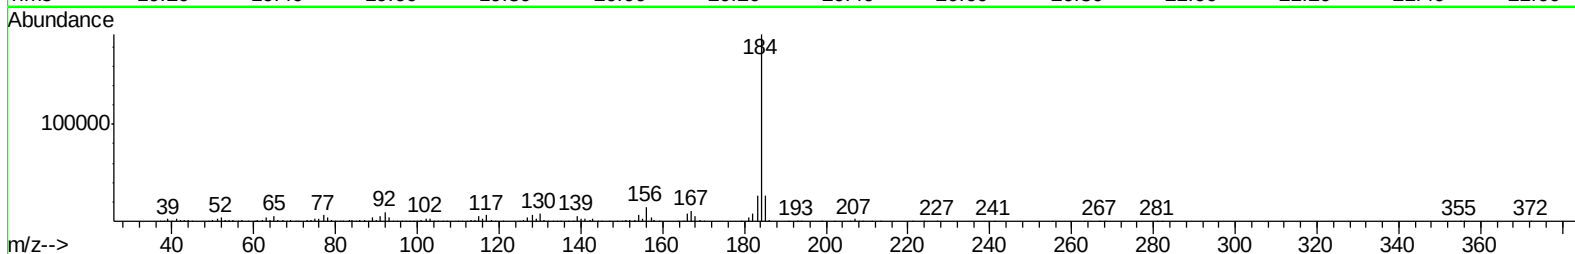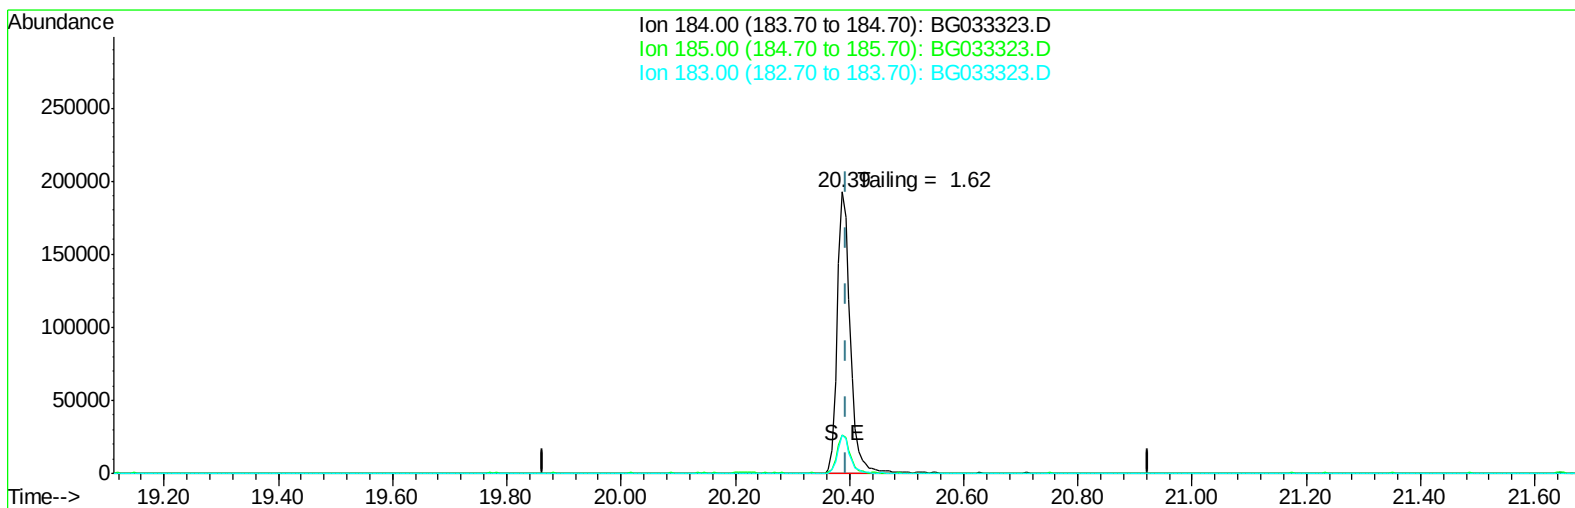

TIC: BG033323.D

(76) Benzidine

20.387min (-0.008) 179586.21ng

response 301947

Ion	Exp%	Act%
184.00	100	100
185.00	13.90	13.56
183.00	13.30	13.60
0.00	0.00	0.00