


Data Path : Z:\HPCHEM1\BNA G\DATA\BG032618\  
 Data File : BG033342.D  
 Acq On : 26 Mar 2018 23:03  
 Operator : SJ/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA\_G\METHODS\8270-BG031918.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Fri Mar 23 15:11:46 2018



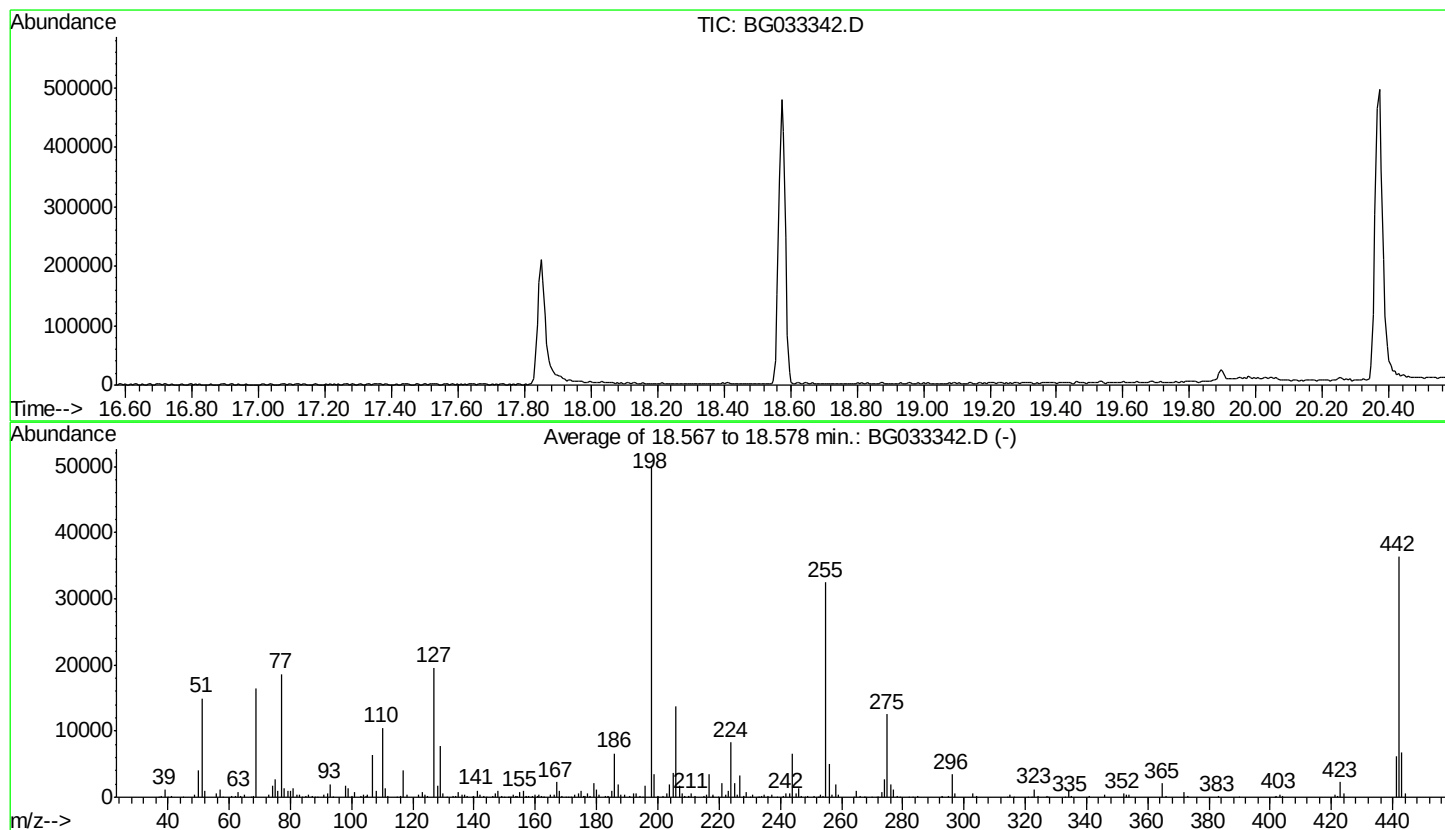


AutoFind: Scans 2600, 2601, 2602; Background Corrected with Scan 2593

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 51             | 198             | 10              | 80              | 29.9         | 15001      | PASS                |
| 68             | 69              | 0.00            | 2               | 1.0          | 171        | PASS                |
| 69             | 198             | 0.00            | 100             | 32.9         | 16485      | PASS                |
| 70             | 69              | 0.00            | 2               | 0.0          | 0          | PASS                |
| 127            | 198             | 10              | 80              | 39.1         | 19621      | PASS                |
| 197            | 198             | 0.00            | 2               | 0.0          | 0          | PASS                |
| 198            | 198             | 100             | 100             | 100.0        | 50149      | PASS                |
| 199            | 198             | 5               | 9               | 6.9          | 3459       | PASS                |
| 275            | 198             | 10              | 60              | 25.0         | 12554      | PASS                |
| 365            | 198             | 1               | 100             | 4.1          | 2047       | PASS                |
| 441            | 443             | 0.01            | 100             | 91.3         | 6261       | PASS                |
| 442            | 198             | 50              | 100             | 72.5         | 36338      | PASS                |
| 443            | 442             | 15              | 24              | 18.9         | 6859       | PASS                |

Data Path : Z:\HPCHEM1\BNA G\DATA\BG032618\  
Data File : BG033342.D  
Acq On : 26 Mar 2018 23:03  
Operator : SJ/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 27 11:15:17 2018  
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG031918.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Fri Mar 23 15:11:46 2018  
Response via : Initial Calibration

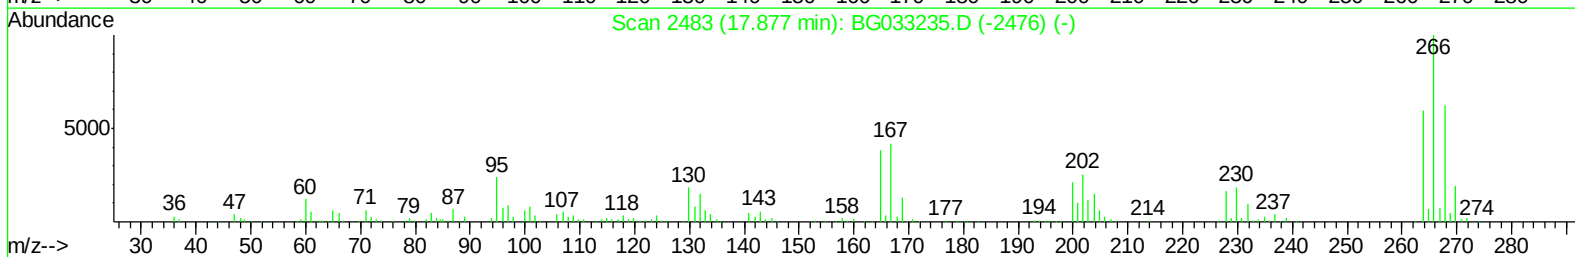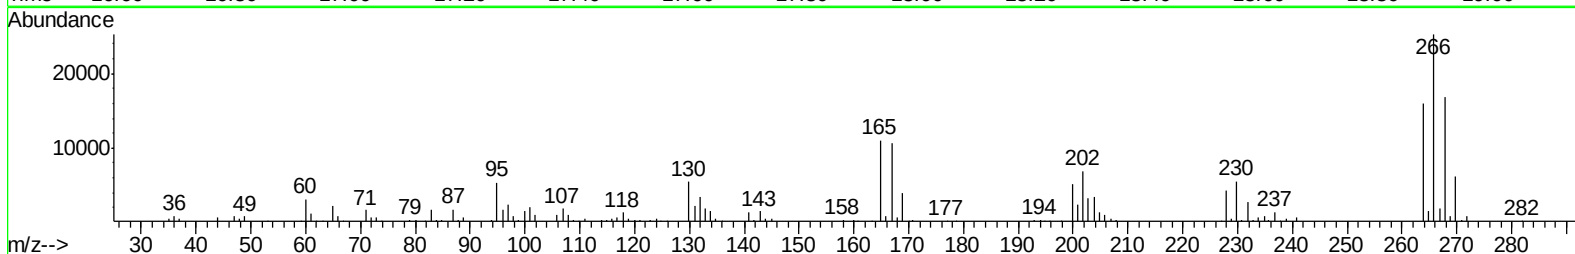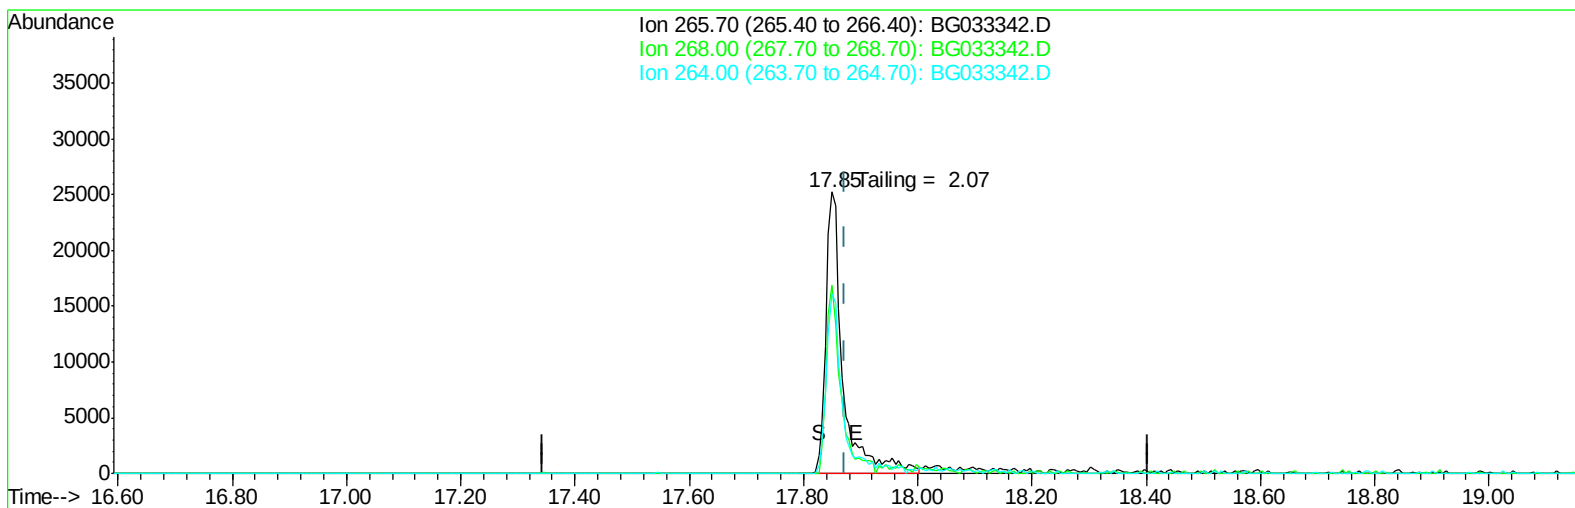

TIC: BG033342.D

(69) Pentachlorophenol (C)




17.850min (-0.024) 17025.53ng

response 48809

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 265.70 | 100   | 100   |
| 268.00 | 63.90 | 70.24 |
| 264.00 | 62.00 | 63.46 |
| 0.00   | 0.00  | 0.00  |

Data Path : Z:\HPCHEM1\BNA G\DATA\BG032618\  
Data File : BG033342.D  
Acq On : 26 Mar 2018 23:03  
Operator : SJ/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 27 11:15:17 2018  
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG031918.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Fri Mar 23 15:11:46 2018  
Response via : Initial Calibration

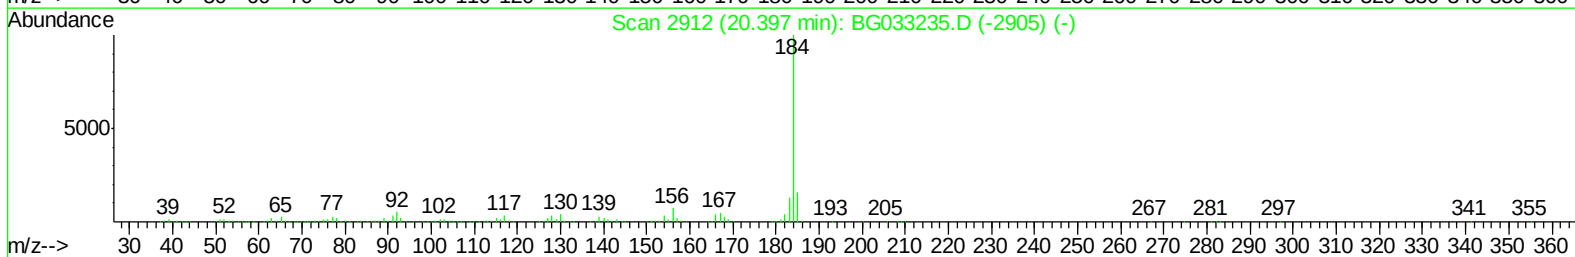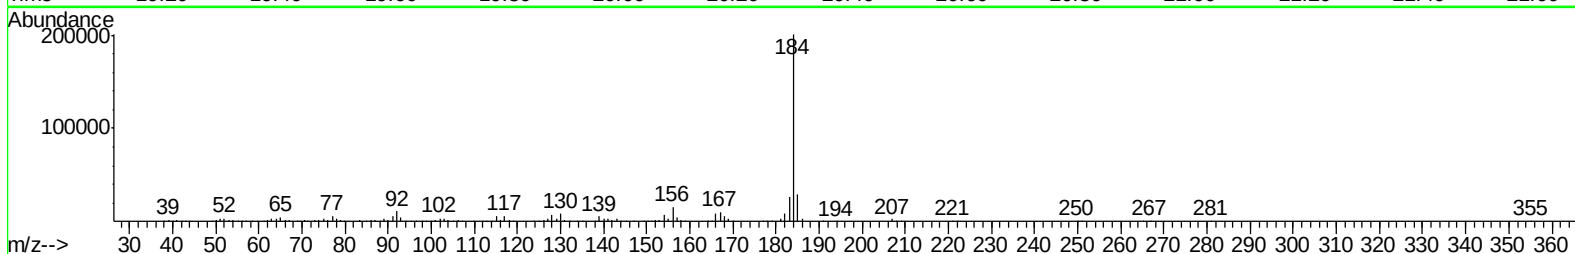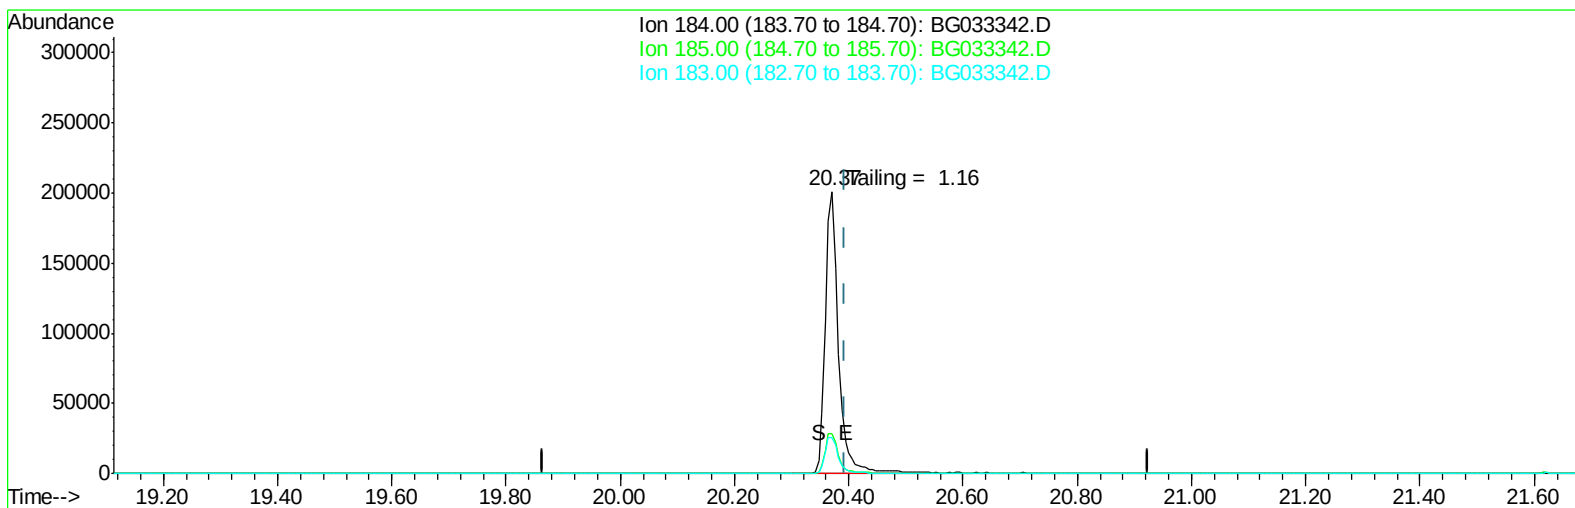

TIC: BG033342.D

(76) Benzidine

20.370min (-0.024) 0.00ng

response 319998

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 184.00 | 100   | 100   |
| 185.00 | 13.90 | 14.27 |
| 183.00 | 13.30 | 12.84 |
| 0.00   | 0.00  | 0.00  |