


Data Path : \\74.0.250.170\svoasrv\HPCHEM1\BNA_G\Data\BG032618\
 Data File : BG033323.D
 Acq On : 26 Mar 2018 11:08
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG031918.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Mar 23 15:11:46 2018

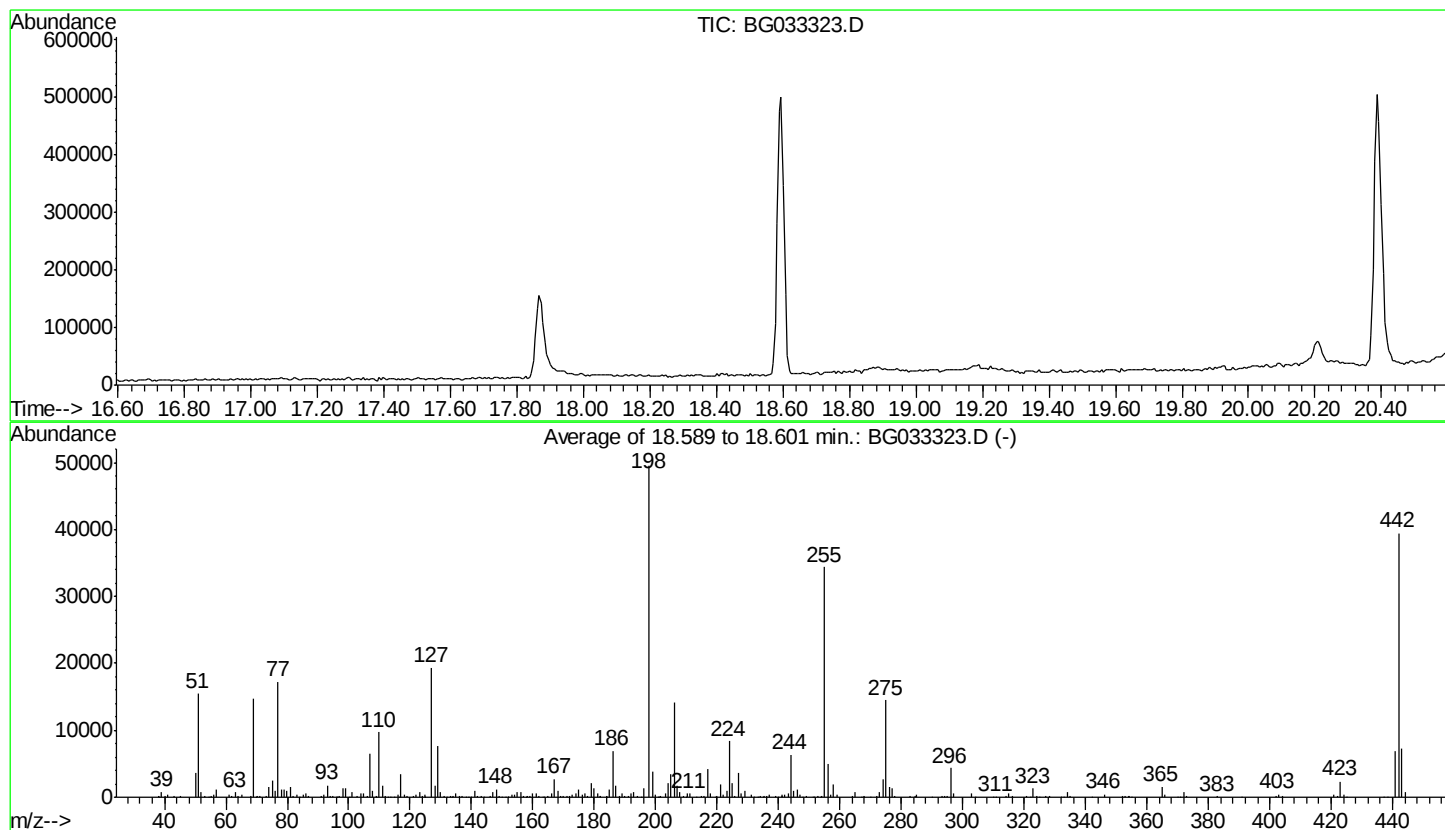

AutoFind: Scans 2604, 2605, 2606; Background Corrected with Scan 2597

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.1	15412	PASS
68	69	0.00	2	1.4	204	PASS
69	198	0.00	100	29.9	14816	PASS
70	69	0.00	2	1.7	249	PASS
127	198	10	80	39.0	19322	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	49541	PASS
199	198	5	9	7.7	3807	PASS
275	198	10	60	29.2	14458	PASS
365	198	1	100	3.3	1617	PASS
441	443	0.01	100	95.7	6902	PASS
442	198	50	100	79.7	39477	PASS
443	442	15	24	18.3	7214	PASS