

Data Path : Z:\HPCHEM1\BNA G\DATA\BG032715\
 Data File : BG016180.D
 Acq On : 27 Mar 2015 17:44
 Operator : TP/IZ
 Sample : G1647-06
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :

Quant Time: Mar 28 03:32:38 2015
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM01.2-EPA-BG031715.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Mar 28 03:20:39 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.79	152	49232	20.00	ng/ul	0.01
18) Naphthalene-d8	10.57	136	226427	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.41	164	142400	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.15	188	305187	20.00	ng/ul	0.00
75) Chrysene-d12	21.32	240	308461	20.00	ng/ul	0.00
83) Perylene-d12	23.61	264	307296	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	0.00	96	0	0.00	ng/uL	
5) Phenol-d5	6.96	99	140330	32.01	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.12	67	74987	30.69	ng/ul	0.00
9) 2-Chlorophenol-d4	7.32	132	109154	32.07	ng/ul	0.00
13) 4-Methylphenol-d8	8.49	113	106912	32.15	ng/ul	0.00
19) Nitrobenzene-d5	8.94	128	61390	34.13	ng/ul	0.00
22) 2-Nitrophenol-d4	9.66	143	71604	41.54	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.20	165	104940	32.94	ng/ul	0.00
29) 4-Chloroaniline-d4	10.71	131	155607	35.41	ng/ul	0.00
43) Dimethylphthalate-d6	13.82	166	336678	36.27	ng/ul	0.00
46) Acenaphthylene-d8	14.11	160	432675	33.52	ng/ul	0.00
51) 4-Nitrophenol-d4	14.61	143	71733	32.35	ng/ul	0.00
57) Fluorene-d10	15.40	176	305807	32.94	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.52	200	45146	28.31	ng/ul	0.00
70) Anthracene-d10	17.25	188	460342	33.02	ng/ul	0.00
76) Pyrene-d10	19.54	212	468027	33.93	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.46	264	389633	29.07	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
44) Dimethylphthalate	13.87	163	131467	12.48	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG032715\
Data File : BG016180.D
Acq On : 27 Mar 2015 17:44
Operator : TP/IZ
Sample : G1647-06
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :

Quant Time: Mar 28 03:32:38 2015
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM01.2-EPA-BG031715.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Mar 28 03:20:39 2015
Response via : Initial Calibration

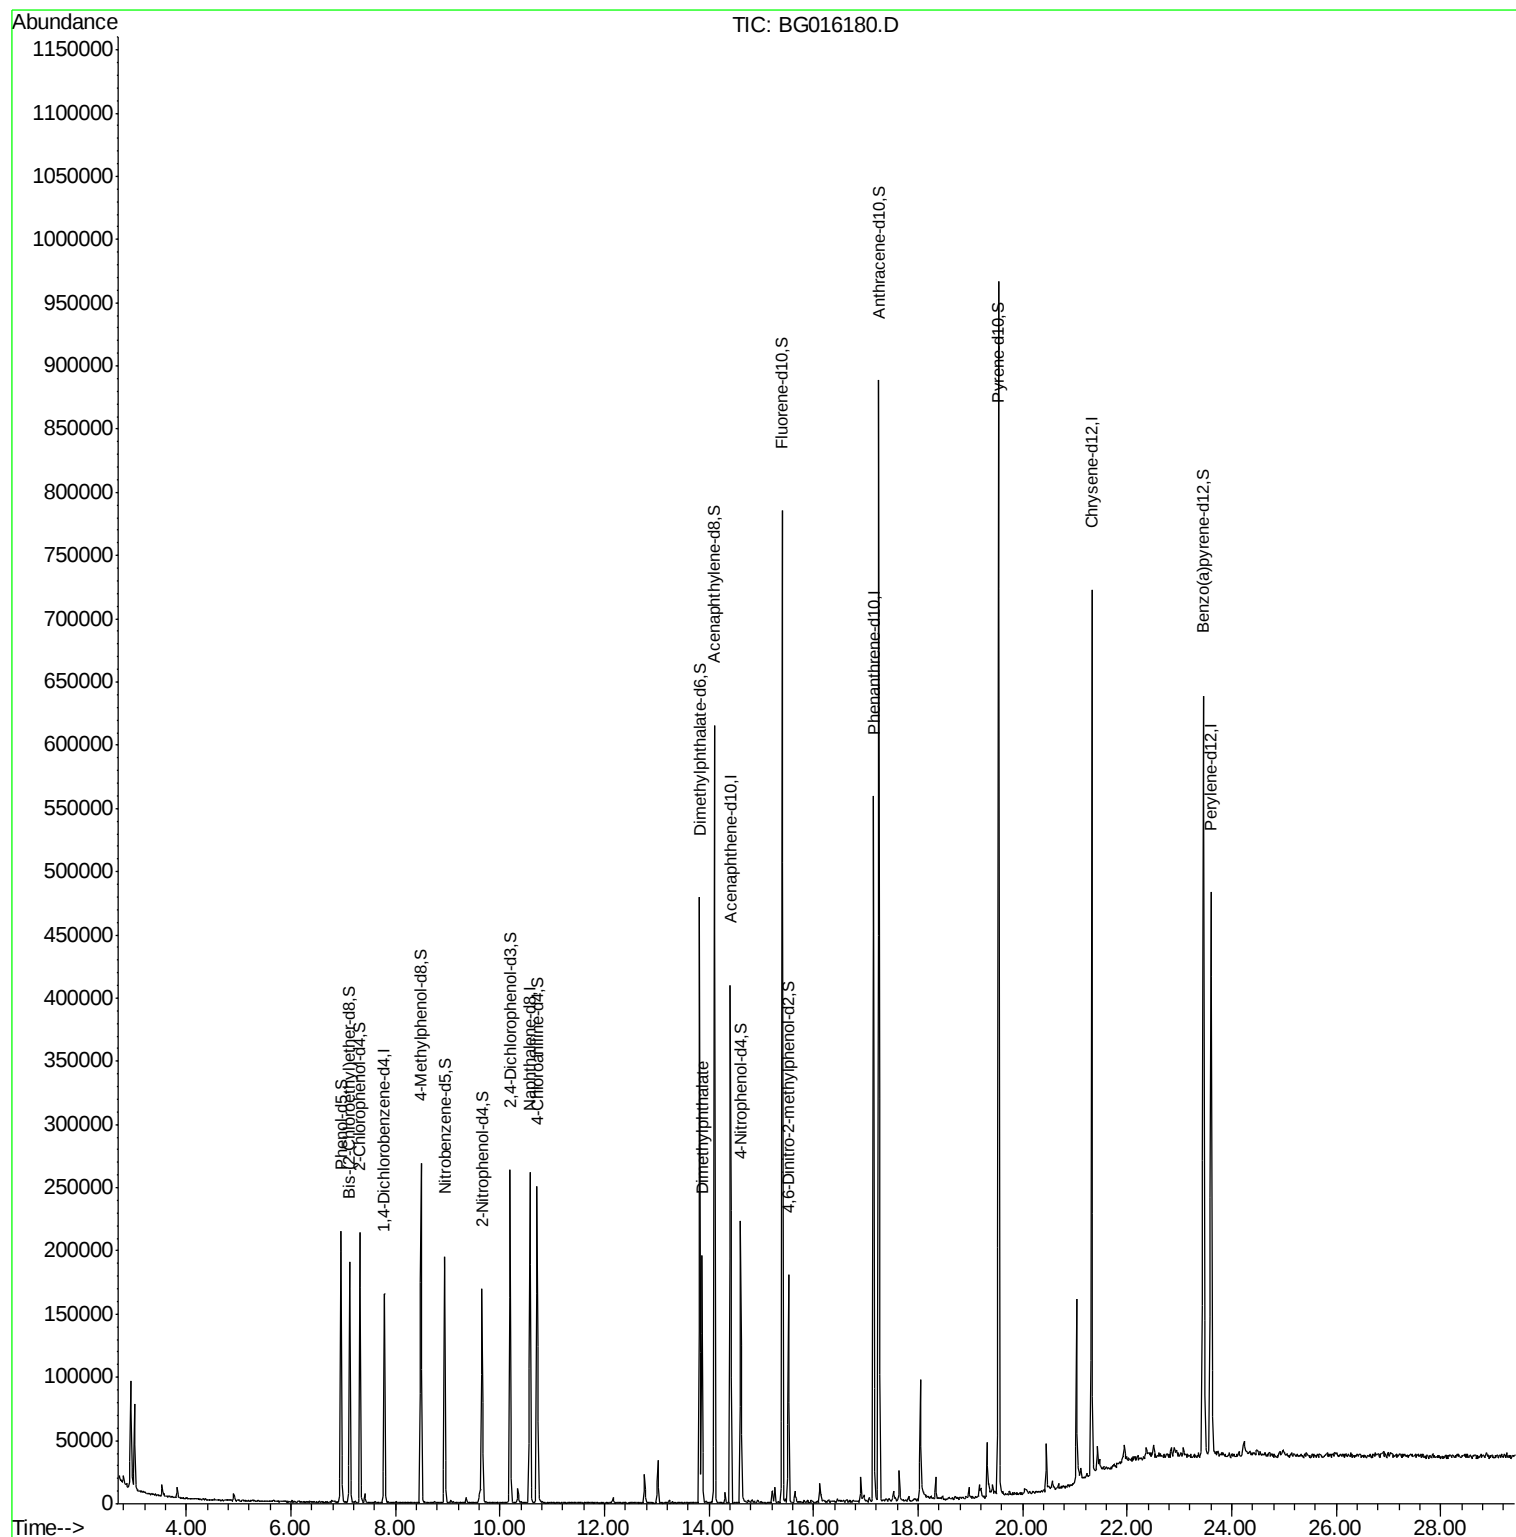

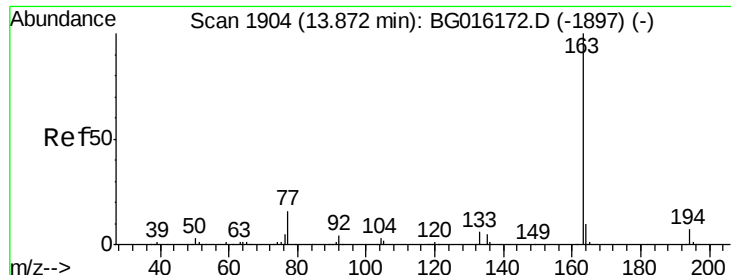

#44
 Dimethylphthalate
 Concen: 12.48 ng/ul
 RT: 13.87 min Scan# 1904
 Delta R.T. 0.00 min
 Lab File: BG016180.D
 Acq: 27 Mar 2015 17:44

Instrument :
 BNA_G
 ClientSampleId :

Tot Ion	Ratio	Lower	Upper
163	100		
194	7.1	5.4	8.0
164	9.4	8.2	12.4

