

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG032715\
 Data File : BG016179.D
 Acq On : 27 Mar 2015 17:09
 Operator : TP/IZ
 Sample : G1647-04
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0AC3

Quant Time: Mar 28 03:32:29 2015
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM01.2-EPA-BG031715.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Mar 28 03:20:39 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.79	152	51855	20.00	ng/ul	0.01
18) Naphthalene-d8	10.58	136	240629	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.41	164	148706	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.15	188	314334	20.00	ng/ul	0.00
75) Chrysene-d12	21.32	240	321485	20.00	ng/ul	0.00
83) Perylene-d12	23.61	264	310279	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	0.00	96	0	0.00	ng/uL	
5) Phenol-d5	6.96	99	161107	34.89	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.13	67	82172	31.93	ng/ul	0.01
9) 2-Chlorophenol-d4	7.32	132	123800	34.53	ng/ul	0.00
13) 4-Methylphenol-d8	8.49	113	123419	35.24	ng/ul	0.00
19) Nitrobenzene-d5	8.94	128	67061	35.08	ng/ul	0.00
22) 2-Nitrophenol-d4	9.66	143	74495	40.67	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.19	165	116859	34.52	ng/ul	0.00
29) 4-Chloroaniline-d4	10.71	131	168754	36.14	ng/ul	0.00
43) Dimethylphthalate-d6	13.82	166	354624	36.58	ng/ul	0.00
46) Acenaphthylene-d8	14.11	160	462226	34.29	ng/ul	0.00
51) 4-Nitrophenol-d4	14.61	143	71424	30.85	ng/ul	0.00
57) Fluorene-d10	15.40	176	325737	33.60	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.52	200	37259	22.68	ng/ul	0.00
70) Anthracene-d10	17.25	188	485128	33.79	ng/ul	0.00
76) Pyrene-d10	19.54	212	496552	34.54	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.46	264	412051	30.45	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
44) Dimethylphthalate	13.87	163	143020	13.00	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG032715\
Data File : BG016179.D
Acq On : 27 Mar 2015 17:09
Operator : TP/IZ
Sample : G1647-04
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0AC3

Quant Time: Mar 28 03:32:29 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM01.2-EPA-BG031715.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Mar 28 03:20:39 2015
Response via : Initial Calibration

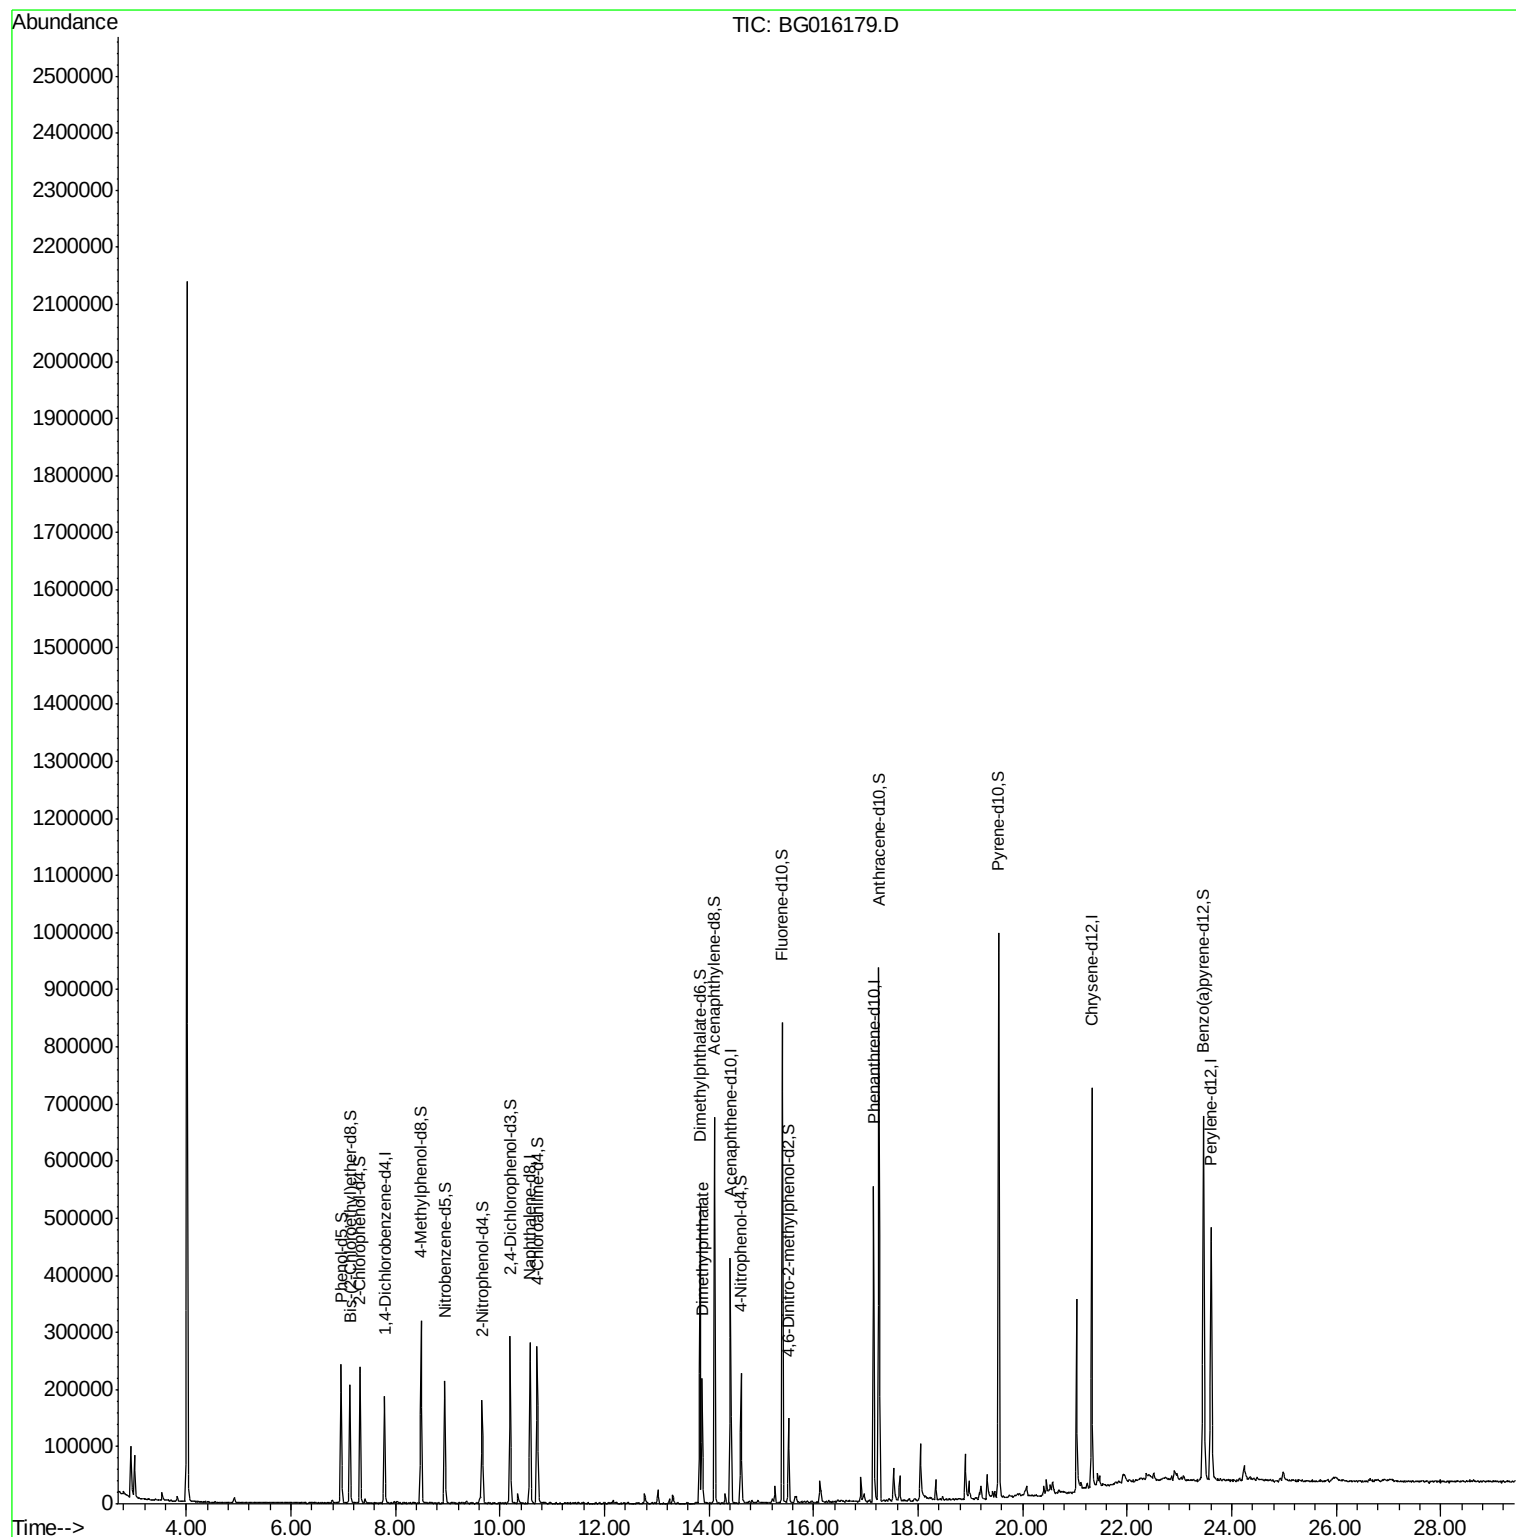

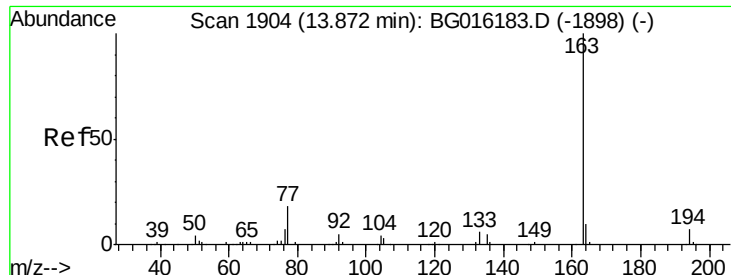

#44

Dimethylphthalate

Concen: 13.00 ng/ul

RT: 13.87 min Scan# 1904

Delta R.T. -0.00 min

Lab File: BG016179.D


Acq: 27 Mar 2015 17:09

Instrument :

BNA_G

ClientSampleId :

C0AC3

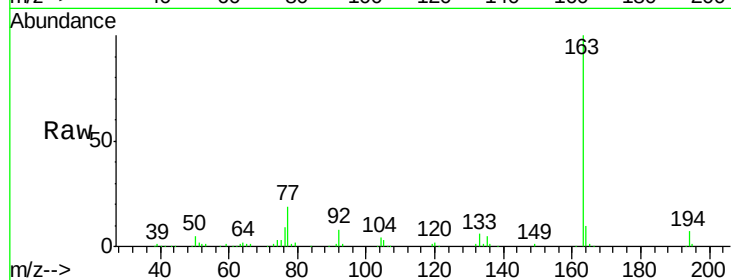

Tgt Ion:	163	Resp:	143020
Ion	Ratio	Lower	Upper
163	100		
194	6.9	5.4	8.0
164	9.8	8.2	12.4

