

Data Path : Z:\HPCHEM1\BNA G\DATA\BG032717\
 Data File : BG026441.D
 Acq On : 27 Mar 2017 20:31
 Operator : SJ/MA
 Sample : I2358-14
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :

Quant Time: Mar 28 01:24:04 2017
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM-EPA-BG032717MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Mar 28 01:23:51 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.05	152	172946	20.00	ng/ul	0.00
18) Naphthalene-d8	10.84	136	718745	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.65	164	418641	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.38	188	997130	20.00	ng/ul	0.00
77) Chrysene-d12	21.62	240	1157774	20.00	ng/ul	0.00
85) Perylene-d12	24.80	264	1135777	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.47	96	19911	5.51	ng/uL	0.00
5) Phenol-d5	7.21	99	79118	6.21	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.36	67	204657	28.67	ng/ul	0.00
9) 2-Chlorophenol-d4	7.58	132	262689	23.00	ng/ul	0.00
13) 4-Methylphenol-d8	8.75	113	154604	15.07	ng/ul	0.00
19) Nitrobenzene-d5	9.20	128	150554	29.31	ng/ul	0.00
22) 2-Nitrophenol-d4	9.93	143	180721	30.02	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.47	165	295854	26.78	ng/ul	0.00
29) 4-Chloroaniline-d4	10.98	131	36404	3.31	ng/ul	0.00
43) Dimethylphthalate-d6	14.05	166	997584	30.77	ng/ul	0.00
46) Acenaphthylene-d8	14.34	160	1199696	29.70	ng/ul	0.00
51) 4-Nitrophenol-d4	14.85	143	33101	5.25	ng/ul	0.00
57) Fluorene-d10	15.63	176	907649	30.82	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.75	200	176780	27.57	ng/ul	0.00
70) Anthracene-d10	17.48	188	1412192	31.19	ng/ul	0.00
78) Pyrene-d10	19.76	212	1621830	31.41	ng/ul	0.00
89) Benzo(a)pyrene-d12	24.59	264	1606536	32.92	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
44) Dimethylphthalate	14.10	163	34387	1.09	ng/ul#	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG032717\
Data File : BG026441.D
Acq On : 27 Mar 2017 20:31
Operator : SJ/MA
Sample : I2358-14
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :

Quant Time: Mar 28 01:24:04 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM-EPA-BG032717MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Mar 28 01:23:51 2017
Response via : Initial Calibration

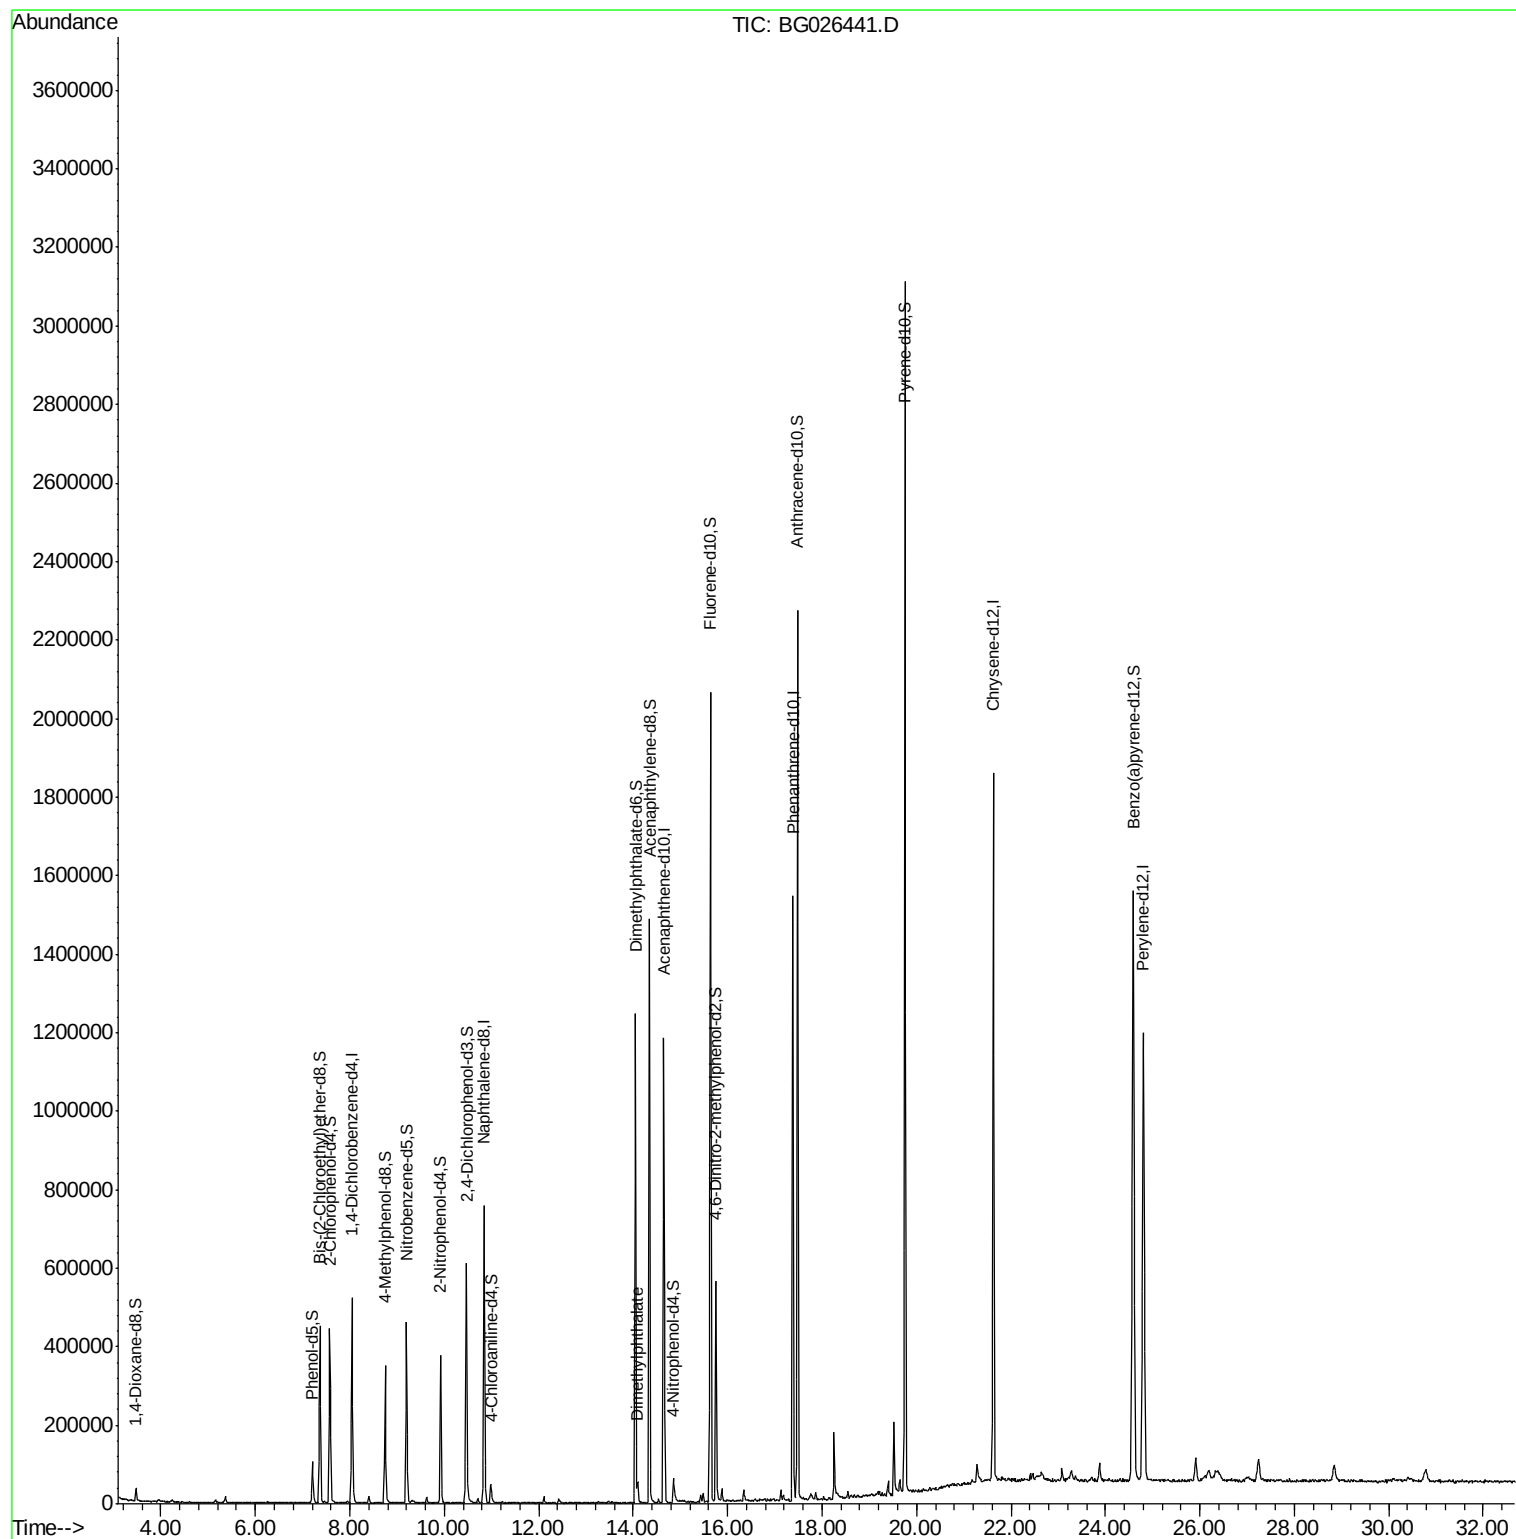

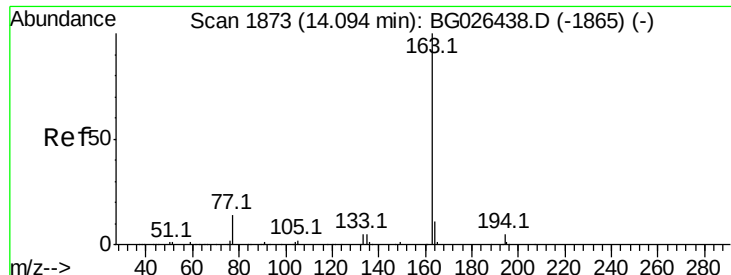

#44

Dimethylphthalate

Concen: 1.09 ng/ul

RT: 14.10 min Scan# 1874

Delta R.T. 0.00 min

Lab File: BG026441.D

Acq: 27 Mar 2017 20:31

Instrument :

BNA_G

ClientSampleId :



Tot Ion:163 Resp: 34387

Ion Ratio Lower Upper

163 100

194 3.6 3.2 4.8

164 12.0 7.8 11.8#

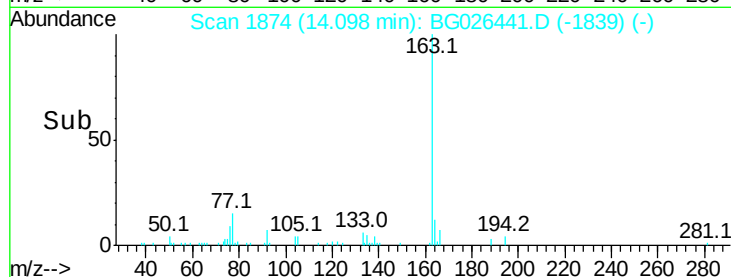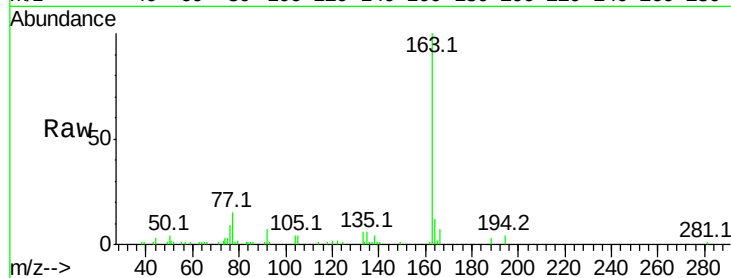

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

