
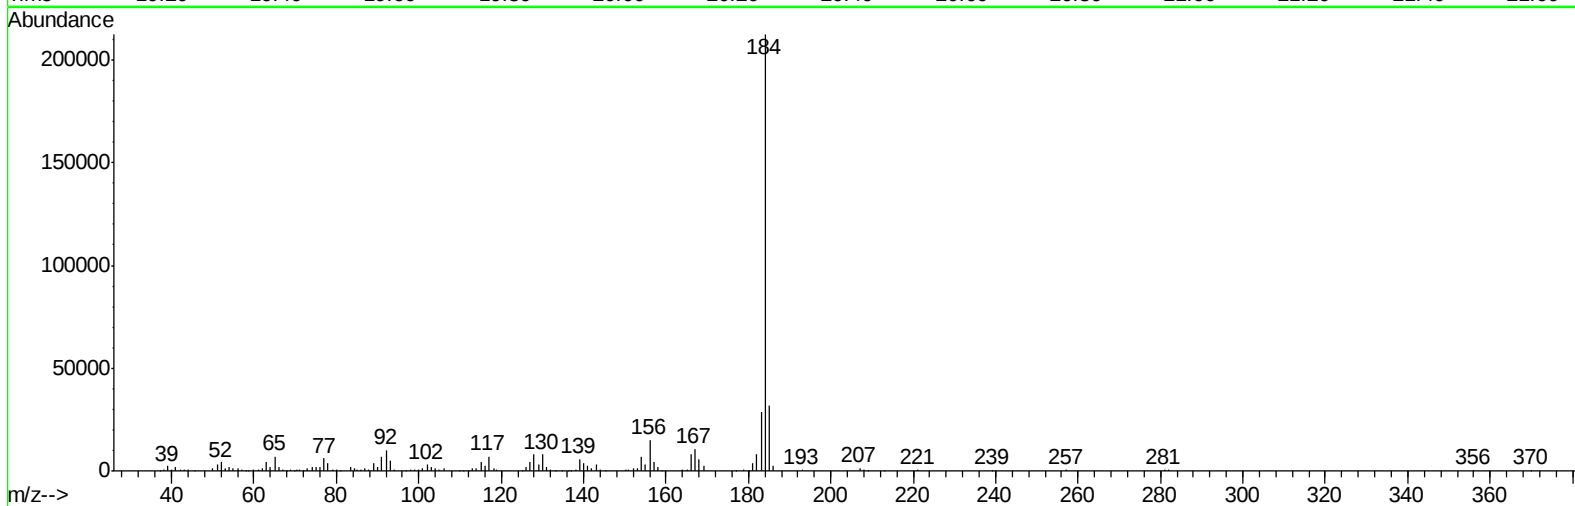


Data Path : Z:\HPCHEM1\BNA G\DATA\BG032718\
Data File : BG033361.D
Acq On : 27 Mar 2018 14:34
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 28 09:11:38 2018
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG031918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 23 15:11:46 2018
Response via : Initial Calibration

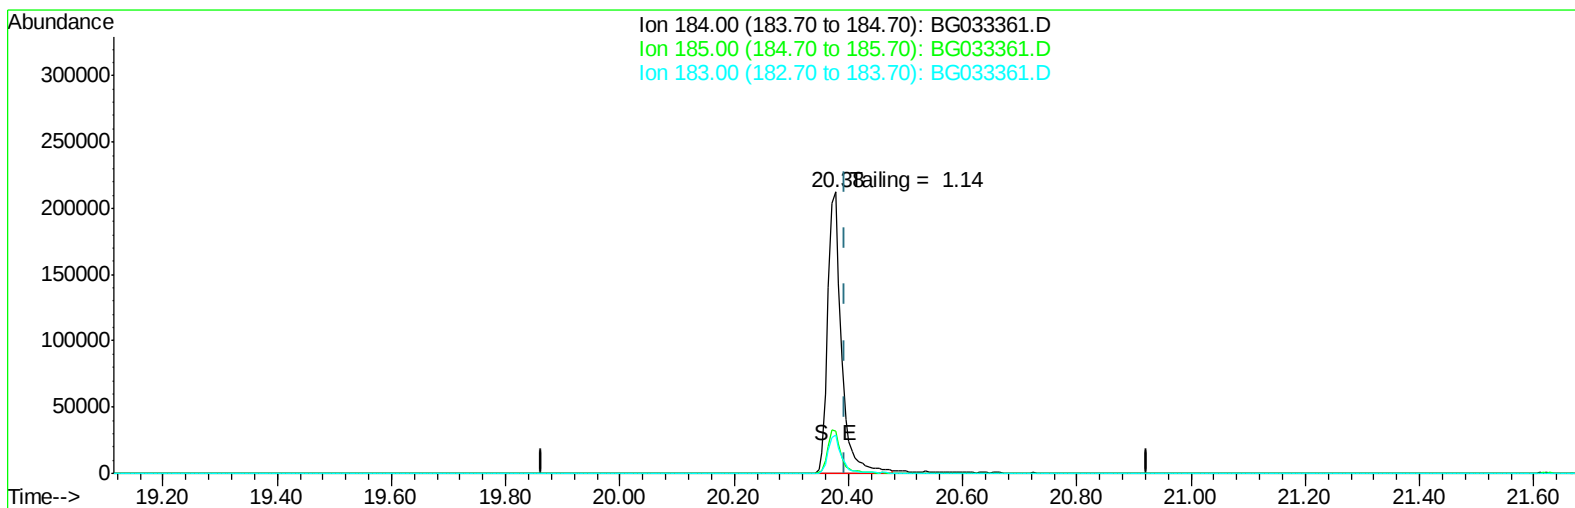

TIC: BG033361.D

(76) Benzidine



20.377min (-0.018) 0.00ng

response 358374

Ion	Exp%	Act%
184.00	100	100
185.00	13.90	14.89
183.00	13.30	13.53
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA G\DATA\BG032718\
Data File : BG033361.D
Acq On : 27 Mar 2018 14:34
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 28 09:11:38 2018
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG031918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 23 15:11:46 2018
Response via : Initial Calibration

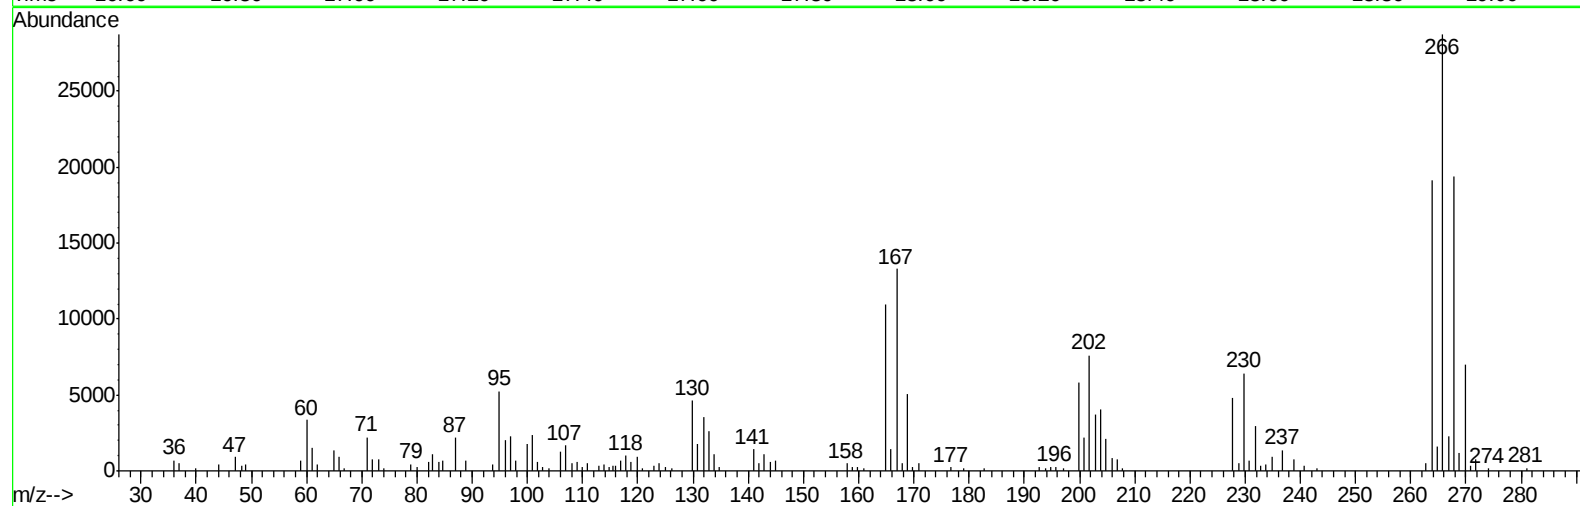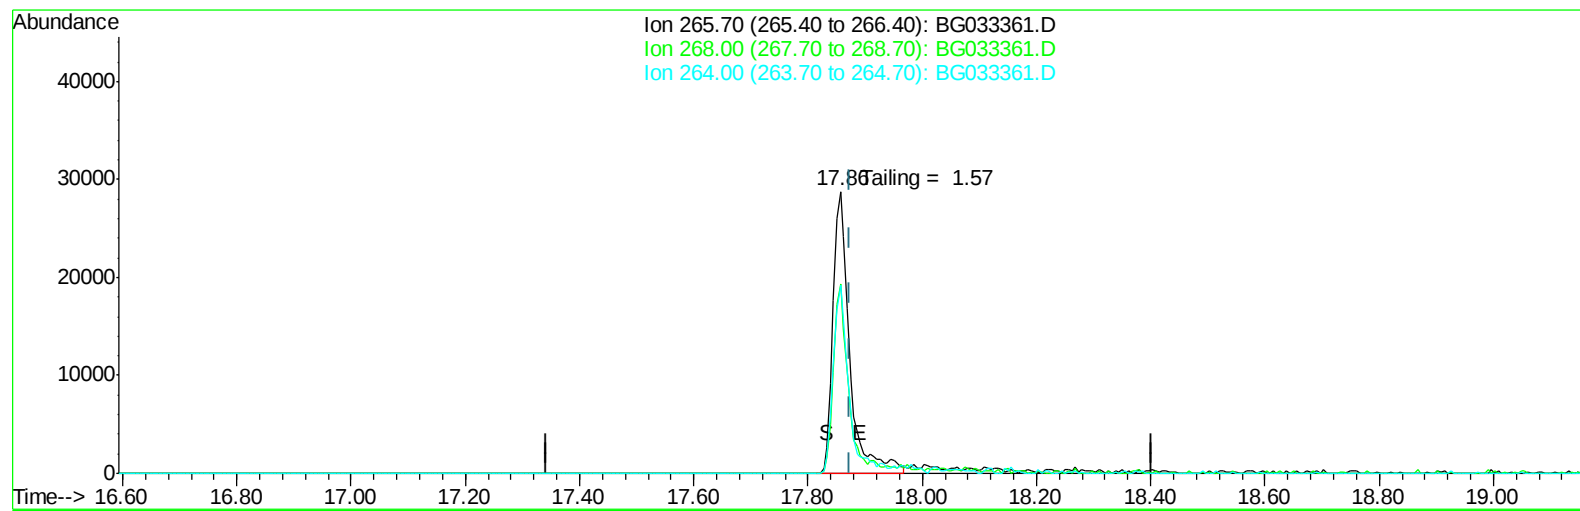

TIC: BG033361.D

(69) Pentachlorophenol (C)

17.856min (-0.018) 22629.19ng

response 56211

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	71.52
264.00	62.00	66.66
0.00	0.00	0.00