
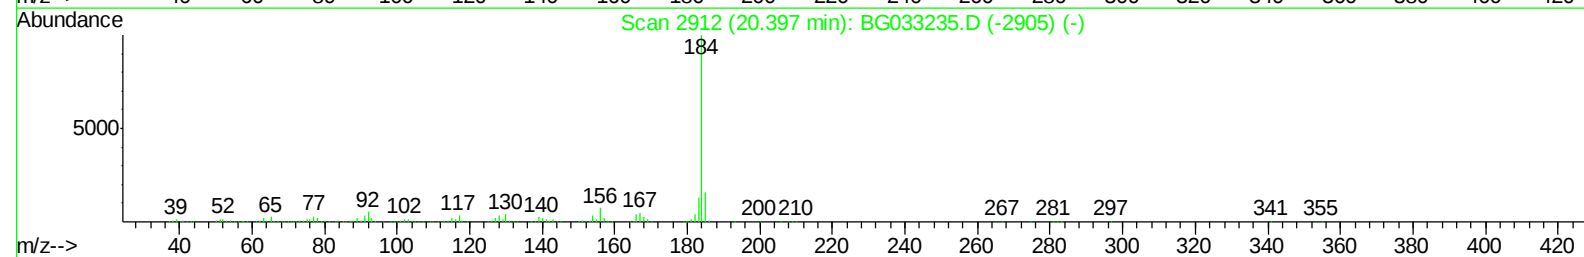
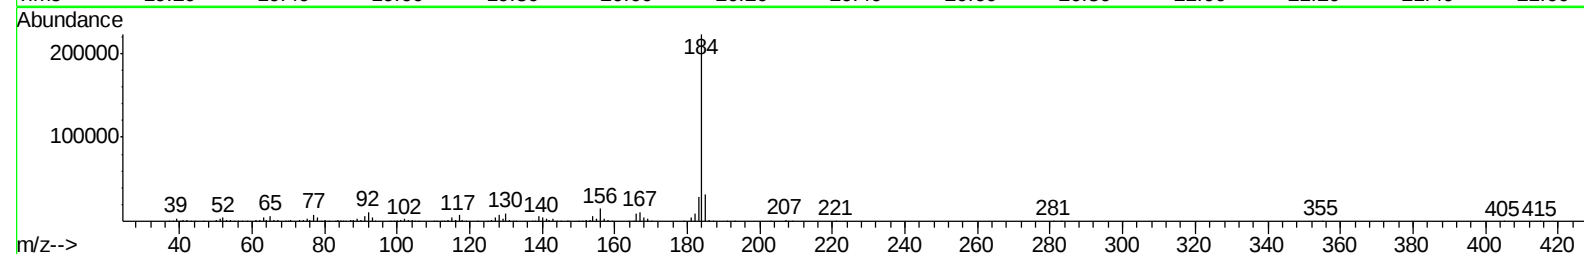


Data Path : Z:\HPCHEM1\BNA G\DATA\BG032718\
 Data File : BG033380.D
 Acq On : 28 Mar 2018 3:05
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 28 09:14:13 2018
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG031918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Mar 23 15:11:46 2018
 Response via : Initial Calibration

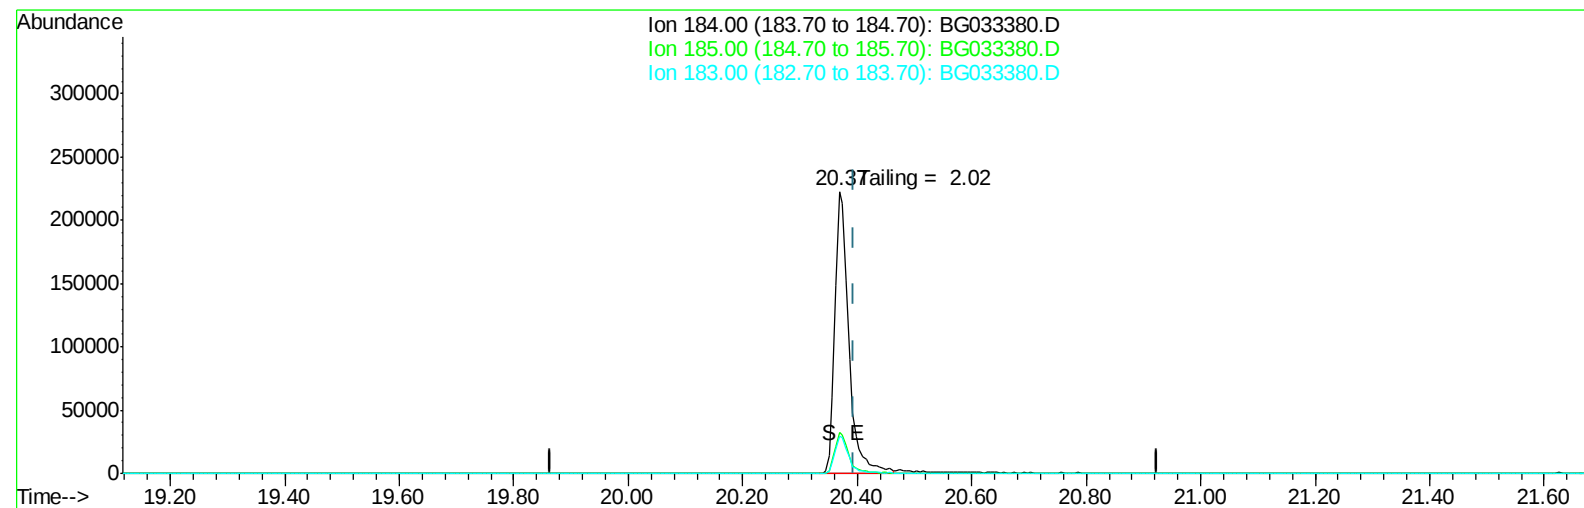

TIC: BG033380.D

(76) Benzidine




20.369min (-0.026) 0.00ng

response 380051

Ion	Exp%	Act%
184.00	100	100
185.00	13.90	14.77
183.00	13.30	13.01
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA G\DATA\BG032718\
Data File : BG033380.D
Acq On : 28 Mar 2018 3:05
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 28 09:14:13 2018
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG031918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 23 15:11:46 2018
Response via : Initial Calibration

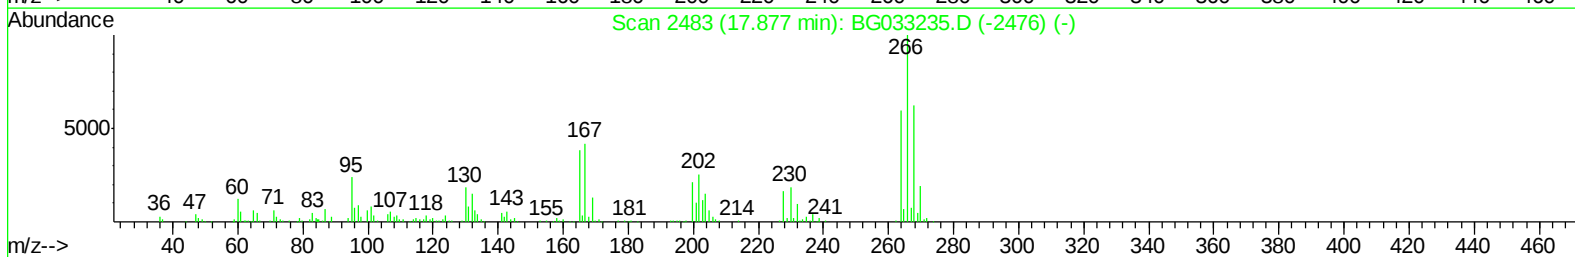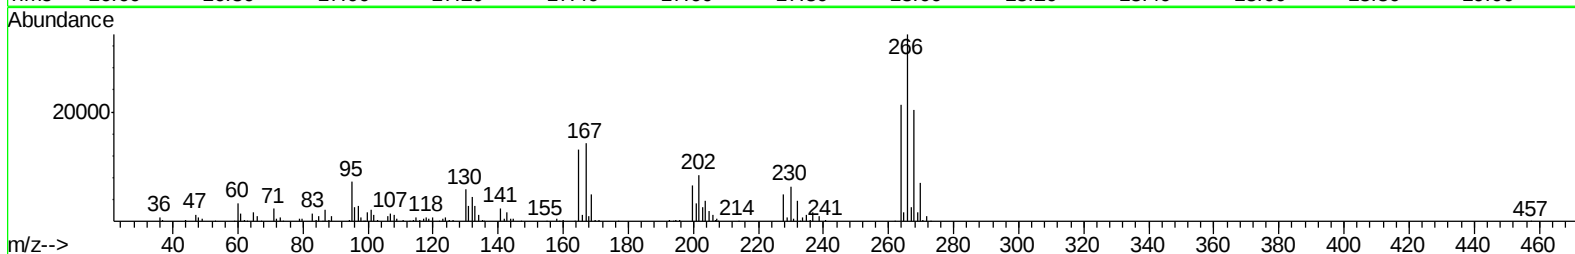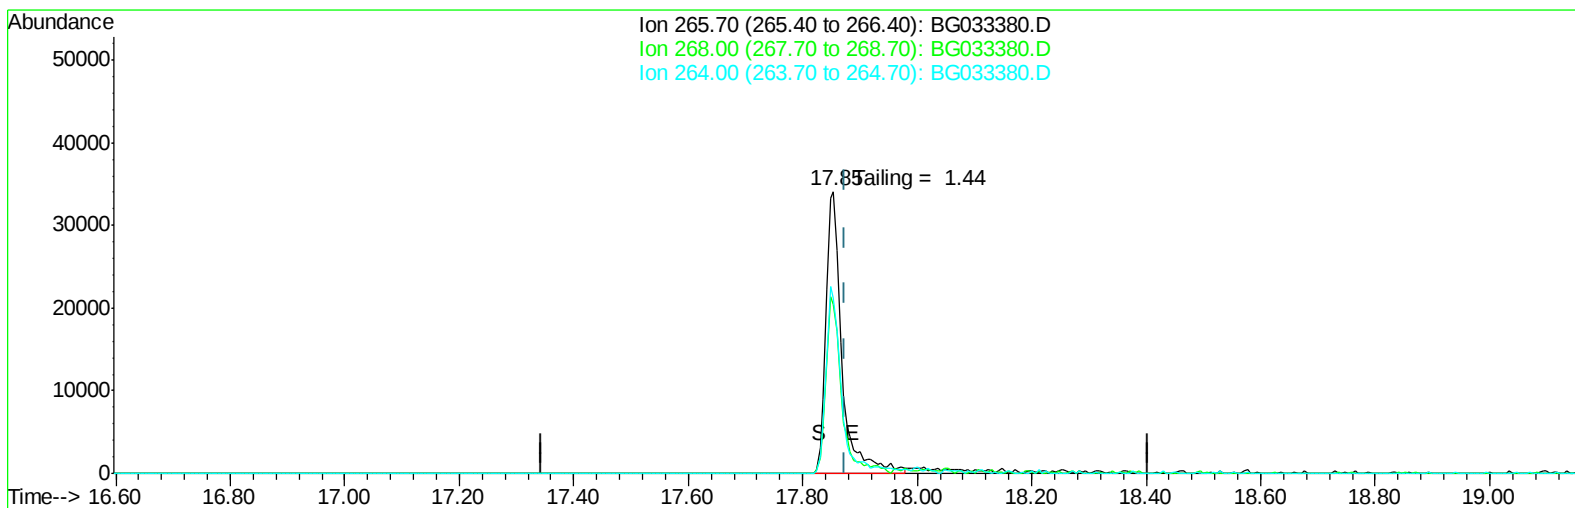

TIC: BG033380.D

(69) Pentachlorophenol (C)

17.854min (-0.020) 16058.16ng

response 65297

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	59.98
264.00	62.00	62.33
0.00	0.00	0.00