


Data Path : Z:\HPCHEM1\BNA G\Data\BG032718\
 Data File : BG033361.D
 Acq On : 27 Mar 2018 14:34
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG031918.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Mar 23 15:11:46 2018

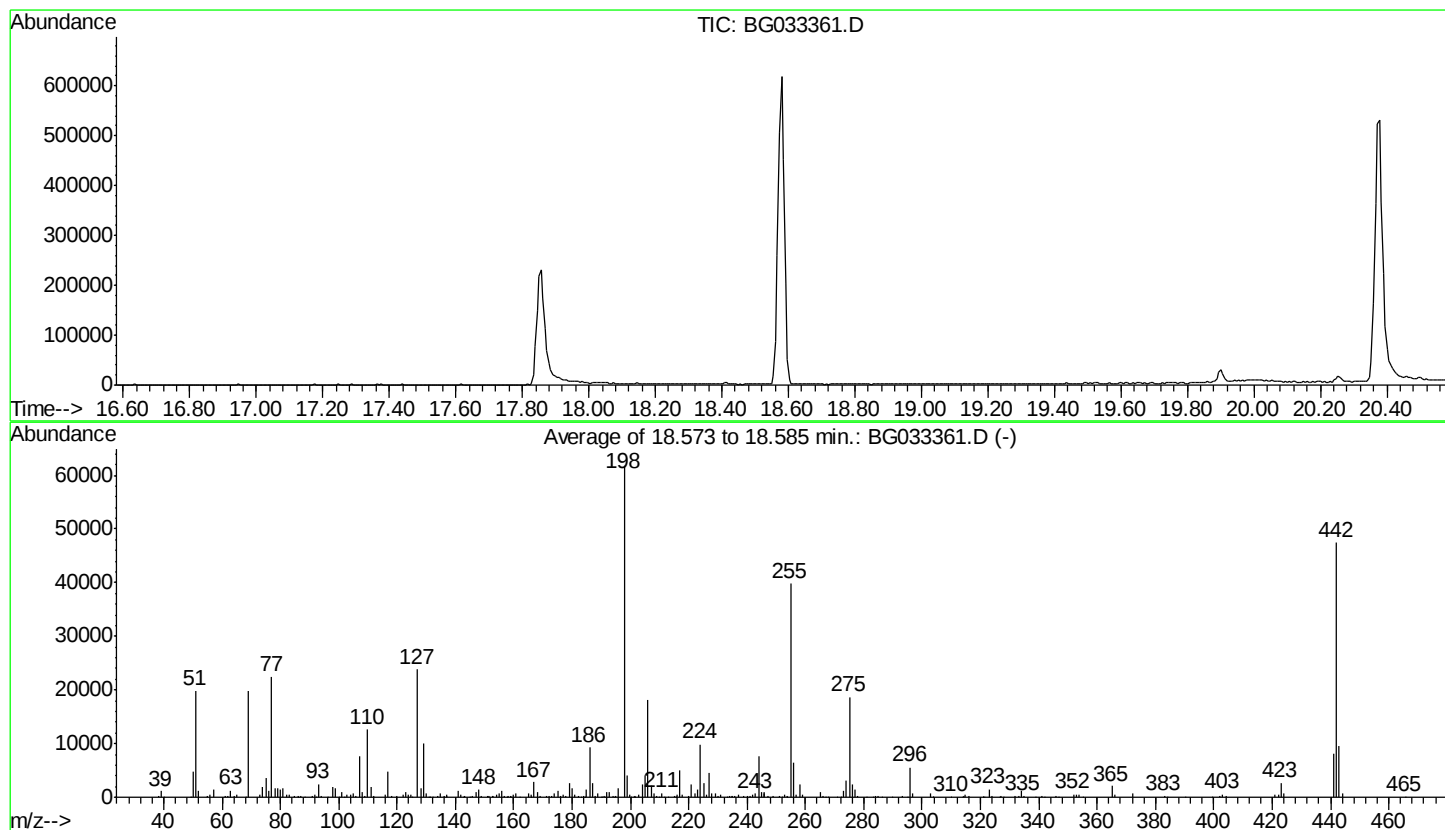

AutoFind: Scans 2601, 2602, 2603; Background Corrected with Scan 2594

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.1	19843	PASS
68	69	0.00	2	0.4	81	PASS
69	198	0.00	100	32.2	19930	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	38.5	23778	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	61808	PASS
199	198	5	9	6.4	3957	PASS
275	198	10	60	30.2	18694	PASS
365	198	1	100	3.5	2138	PASS
441	443	0.01	100	85.1	8179	PASS
442	198	50	100	76.8	47458	PASS
443	442	15	24	20.3	9615	PASS