


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG032719\
 Data File : BG040174.D
 Acq On : 27 Mar 2019 16:23
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG032719.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Mar 28 05:47:00 2019

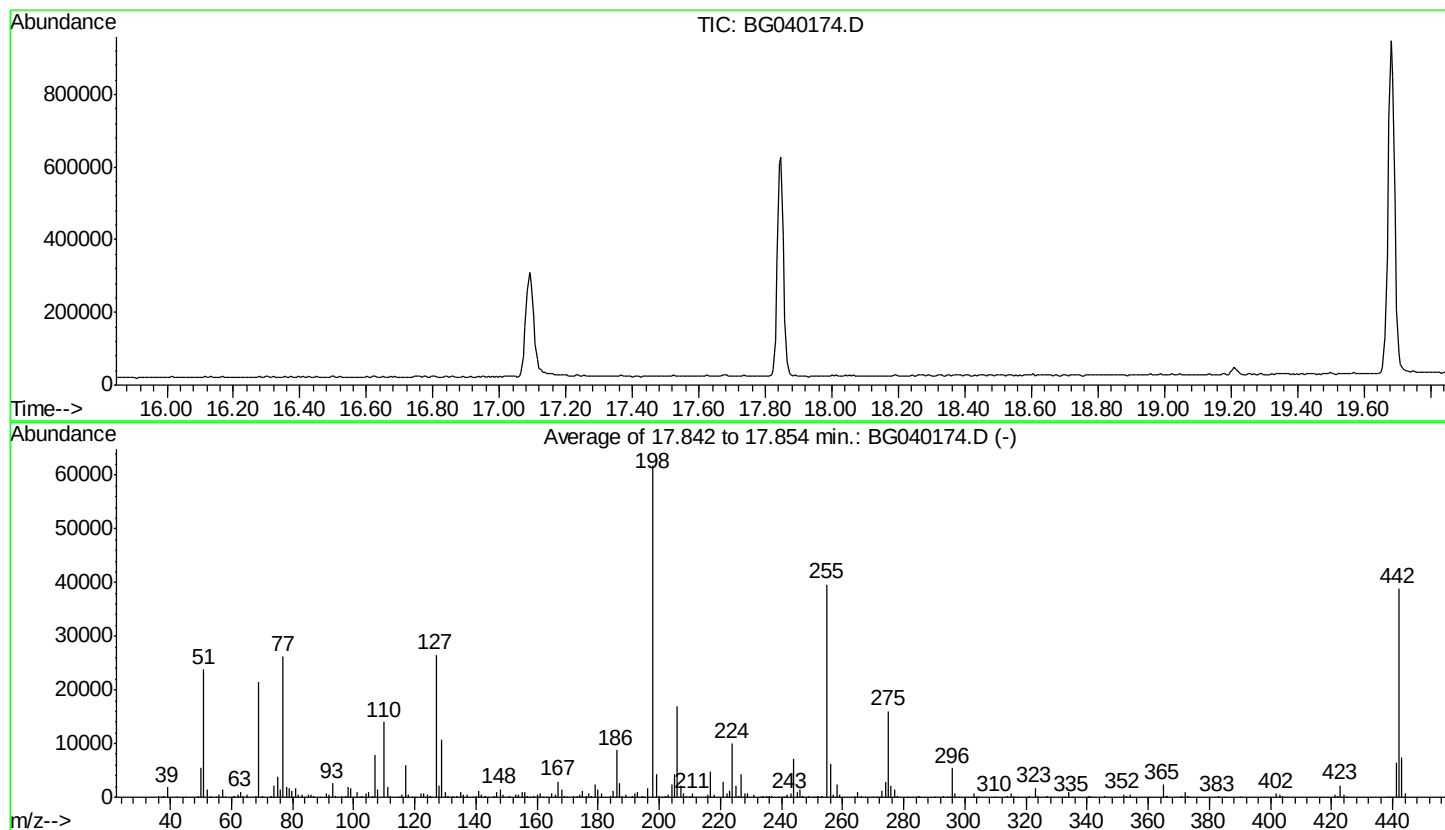

AutoFind: Scans 2511, 2512, 2513; Background Corrected with Scan 2504

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.6	23846	PASS
68	69	0.00	2	1.4	298	PASS
69	198	0.00	100	34.6	21359	PASS
70	69	0.00	2	1.3	286	PASS
127	198	10	80	42.9	26525	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	61786	PASS
199	198	5	9	6.9	4269	PASS
275	198	10	60	26.1	16101	PASS
365	198	1	100	3.7	2297	PASS
441	198	0.01	100	10.4	6430	PASS
442	198	50	100	62.9	38866	PASS
443	442	15	24	19.2	7445	PASS