

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG032816\
 Data File : BG021523.D
 Acq On : 28 Mar 2016 12:58
 Operator : UM/SJ
 Sample : PB89199BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK99

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG031616.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.373	89	91	97	rBV3	1164	1955	0.51%	0.062%
2	3.455	102	105	109	rVB4	1902	2613	0.68%	0.083%
3	4.025	200	202	203	rBV	849	556	0.14%	0.018%
4	4.254	239	241	244	rVB3	735	713	0.19%	0.023%
5	5.047	373	376	379	rBV3	434	642	0.17%	0.020%
6	5.212	402	404	407	rBV3	515	647	0.17%	0.020%
7	5.282	414	416	418	rBV3	757	660	0.17%	0.021%
8	5.694	484	486	489	rBV2	660	578	0.15%	0.018%
9	5.852	512	513	517	rBV3	444	525	0.14%	0.017%
10	6.651	646	649	651	rBV4	491	538	0.14%	0.017%
11	7.339	760	766	770	rBV2	35939	64271	16.73%	2.032%
12	7.380	770	773	780	rVB	31683	49454	12.87%	1.563%
13	7.633	811	816	823	rVB	42184	66593	17.33%	2.105%
14	7.774	839	840	842	rVB2	957	530	0.14%	0.017%
15	7.997	875	878	880	rBV3	759	843	0.22%	0.027%
16	8.056	882	888	895	rVB	28834	47004	12.24%	1.486%
17	8.138	899	902	904	rBV2	570	856	0.22%	0.027%
18	8.843	1016	1022	1033	rVB	50792	86900	22.62%	2.747%
19	8.949	1038	1040	1042	rVB2	724	552	0.14%	0.017%
20	9.084	1061	1063	1066	rVB2	671	615	0.16%	0.019%
21	9.225	1081	1087	1097	rVB	42232	73736	19.19%	2.331%
22	9.342	1106	1107	1110	rBV3	705	621	0.16%	0.020%
23	9.430	1119	1122	1126	rBV3	532	728	0.19%	0.023%
24	9.618	1152	1154	1156	rVB3	884	712	0.19%	0.023%
25	9.648	1156	1159	1160	rBV2	749	768	0.20%	0.024%
26	9.695	1165	1167	1173	rVB3	502	788	0.21%	0.025%
27	9.947	1204	1210	1217	rBV	38072	64857	16.88%	2.050%
28	10.036	1223	1225	1228	rBV3	621	790	0.21%	0.025%
29	10.564	1308	1315	1328	rBV	45942	83216	21.66%	2.631%
30	10.723	1338	1342	1345	rVB3	451	637	0.17%	0.020%
31	10.811	1356	1357	1360	rBV3	654	720	0.19%	0.023%
32	10.864	1360	1366	1372	rVV	41517	72328	18.83%	2.286%
33	10.970	1381	1384	1386	rVB3	727	734	0.19%	0.023%
34	11.011	1386	1391	1398	rBV4	6671	12759	3.32%	0.403%

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG032816\
 Data File : BG021523.D
 Acq On : 28 Mar 2016 12:58
 Operator : UM/SJ
 Sample : PB89199BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK99

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG031616.M
 Title : SVOA CALIBRATION

35	11.081	1401	1403	1407	rVB3	611	576	0.15%	0.018%
36	11.581	1486	1488	1492	rVB2	569	719	0.19%	0.023%
37	11.740	1513	1515	1518	rBV2	406	531	0.14%	0.017%
38	11.904	1541	1543	1549	rVB3	634	1030	0.27%	0.033%
39	12.157	1584	1586	1589	rBV3	689	626	0.16%	0.020%
40	12.327	1612	1615	1616	rBV2	495	523	0.14%	0.017%
41	12.439	1632	1634	1637	rBV3	573	571	0.15%	0.018%
42	12.873	1705	1708	1710	rVB3	514	561	0.15%	0.018%
43	13.020	1730	1733	1735	rBV3	487	635	0.17%	0.020%
44	13.567	1824	1826	1829	rVB3	595	761	0.20%	0.024%
45	13.608	1832	1833	1838	rVV3	567	728	0.19%	0.023%
46	13.649	1838	1840	1843	rVB3	467	605	0.16%	0.019%
47	13.678	1843	1845	1848	rVB3	778	856	0.22%	0.027%
48	13.714	1848	1851	1852	rBV2	664	743	0.19%	0.023%
49	13.755	1854	1858	1861	rBV3	399	610	0.16%	0.019%
50	14.072	1907	1912	1920	rVB	121683	177677	46.25%	5.617%
51	14.372	1956	1963	1969	rBV	120839	182147	47.41%	5.758%
52	14.671	2009	2014	2021	rBV3	69960	110625	28.80%	3.497%
53	15.042	2073	2077	2079	rVB5	393	540	0.14%	0.017%
54	15.089	2079	2085	2098	rBV2	36044	80854	21.05%	2.556%
55	15.435	2142	2144	2146	rBV2	789	604	0.16%	0.019%
56	15.506	2153	2156	2158	rBV3	547	704	0.18%	0.022%
57	15.664	2175	2183	2191	rBV	163706	245355	63.87%	7.756%
58	15.788	2199	2204	2214	rBV	68693	99614	25.93%	3.149%
59	15.899	2219	2223	2227	rBV4	968	1771	0.46%	0.056%
60	15.970	2234	2235	2240	rBV3	605	675	0.18%	0.021%
61	16.076	2252	2253	2257	rBV3	666	815	0.21%	0.026%
62	16.152	2262	2266	2268	rBV2	836	1000	0.26%	0.032%
63	16.363	2299	2302	2305	rBV3	429	548	0.14%	0.017%
64	16.587	2337	2340	2342	rBV2	516	692	0.18%	0.022%
65	16.663	2350	2353	2355	rVB3	447	530	0.14%	0.017%
66	16.698	2355	2359	2362	rVB3	555	651	0.17%	0.021%
67	16.798	2373	2376	2379	rBV3	447	637	0.17%	0.020%
68	16.869	2385	2388	2391	rVB3	1038	988	0.26%	0.031%
69	16.933	2395	2399	2401	rVB3	540	648	0.17%	0.020%
70	17.016	2410	2413	2415	rVB4	636	719	0.19%	0.023%
71	17.074	2421	2423	2426	rBV3	714	868	0.23%	0.027%

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG032816\
 Data File : BG021523.D
 Acq On : 28 Mar 2016 12:58
 Operator : UM/SJ
 Sample : PB89199BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK99

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG031616.M
 Title : SVOA CALIBRATION

72	17.210	2442	2446	2448	rBV3	636	860	0.22%	0.027%
73	17.321	2463	2465	2468	rVB3	731	640	0.17%	0.020%
74	17.415	2475	2481	2488	rVB	104506	155070	40.37%	4.902%
75	17.515	2492	2498	2504	rVB	193598	291902	75.99%	9.227%
76	17.597	2510	2512	2516	rVB4	553	614	0.16%	0.019%
77	17.703	2529	2530	2534	rBV3	846	805	0.21%	0.025%
78	17.779	2539	2543	2544	rVB4	565	690	0.18%	0.022%
79	17.873	2558	2559	2562	rBV3	697	687	0.18%	0.022%
80	18.097	2596	2597	2602	rBV4	530	651	0.17%	0.021%
81	18.273	2625	2627	2628	rVB2	1016	552	0.14%	0.017%
82	18.297	2630	2631	2634	rVV3	663	639	0.17%	0.020%
83	18.349	2638	2640	2642	rBV2	662	527	0.14%	0.017%
84	18.396	2645	2648	2650	rBV4	585	806	0.21%	0.025%
85	18.731	2704	2705	2708	rVB3	599	591	0.15%	0.019%
86	18.767	2708	2711	2712	rBV3	756	624	0.16%	0.020%
87	19.037	2755	2757	2758	rBV	672	526	0.14%	0.017%
88	19.090	2764	2766	2770	rVB4	959	889	0.23%	0.028%
89	19.137	2770	2774	2777	rBV6	948	1592	0.41%	0.050%
90	19.231	2788	2790	2793	rBV3	622	642	0.17%	0.020%
91	19.331	2805	2807	2809	rVB2	1268	921	0.24%	0.029%
92	19.383	2814	2816	2818	rVV3	1121	853	0.22%	0.027%
93	19.430	2822	2824	2828	rVV3	2605	2824	0.74%	0.089%
94	19.477	2831	2832	2835	rVB3	1061	709	0.18%	0.022%
95	19.677	2864	2866	2871	rVB4	2079	2273	0.59%	0.072%
96	19.789	2879	2885	2894	rBV	257776	384155	100.00%	12.144%
97	19.854	2894	2896	2897	rBV2	1409	752	0.20%	0.024%
98	21.675	3200	3206	3212	rBV	135177	214421	55.82%	6.778%
99	24.677	3709	3717	3728	rVB	129107	349461	90.97%	11.047%
100	24.901	3748	3755	3765	rVB2	65394	188567	49.09%	5.961%


Sum of corrected areas: 3163419

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG032816\
Data File : BG021523.D
Acq On : 28 Mar 2016 12:58
Operator : UM/SJ
Sample : PB89199BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK99

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG031616.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

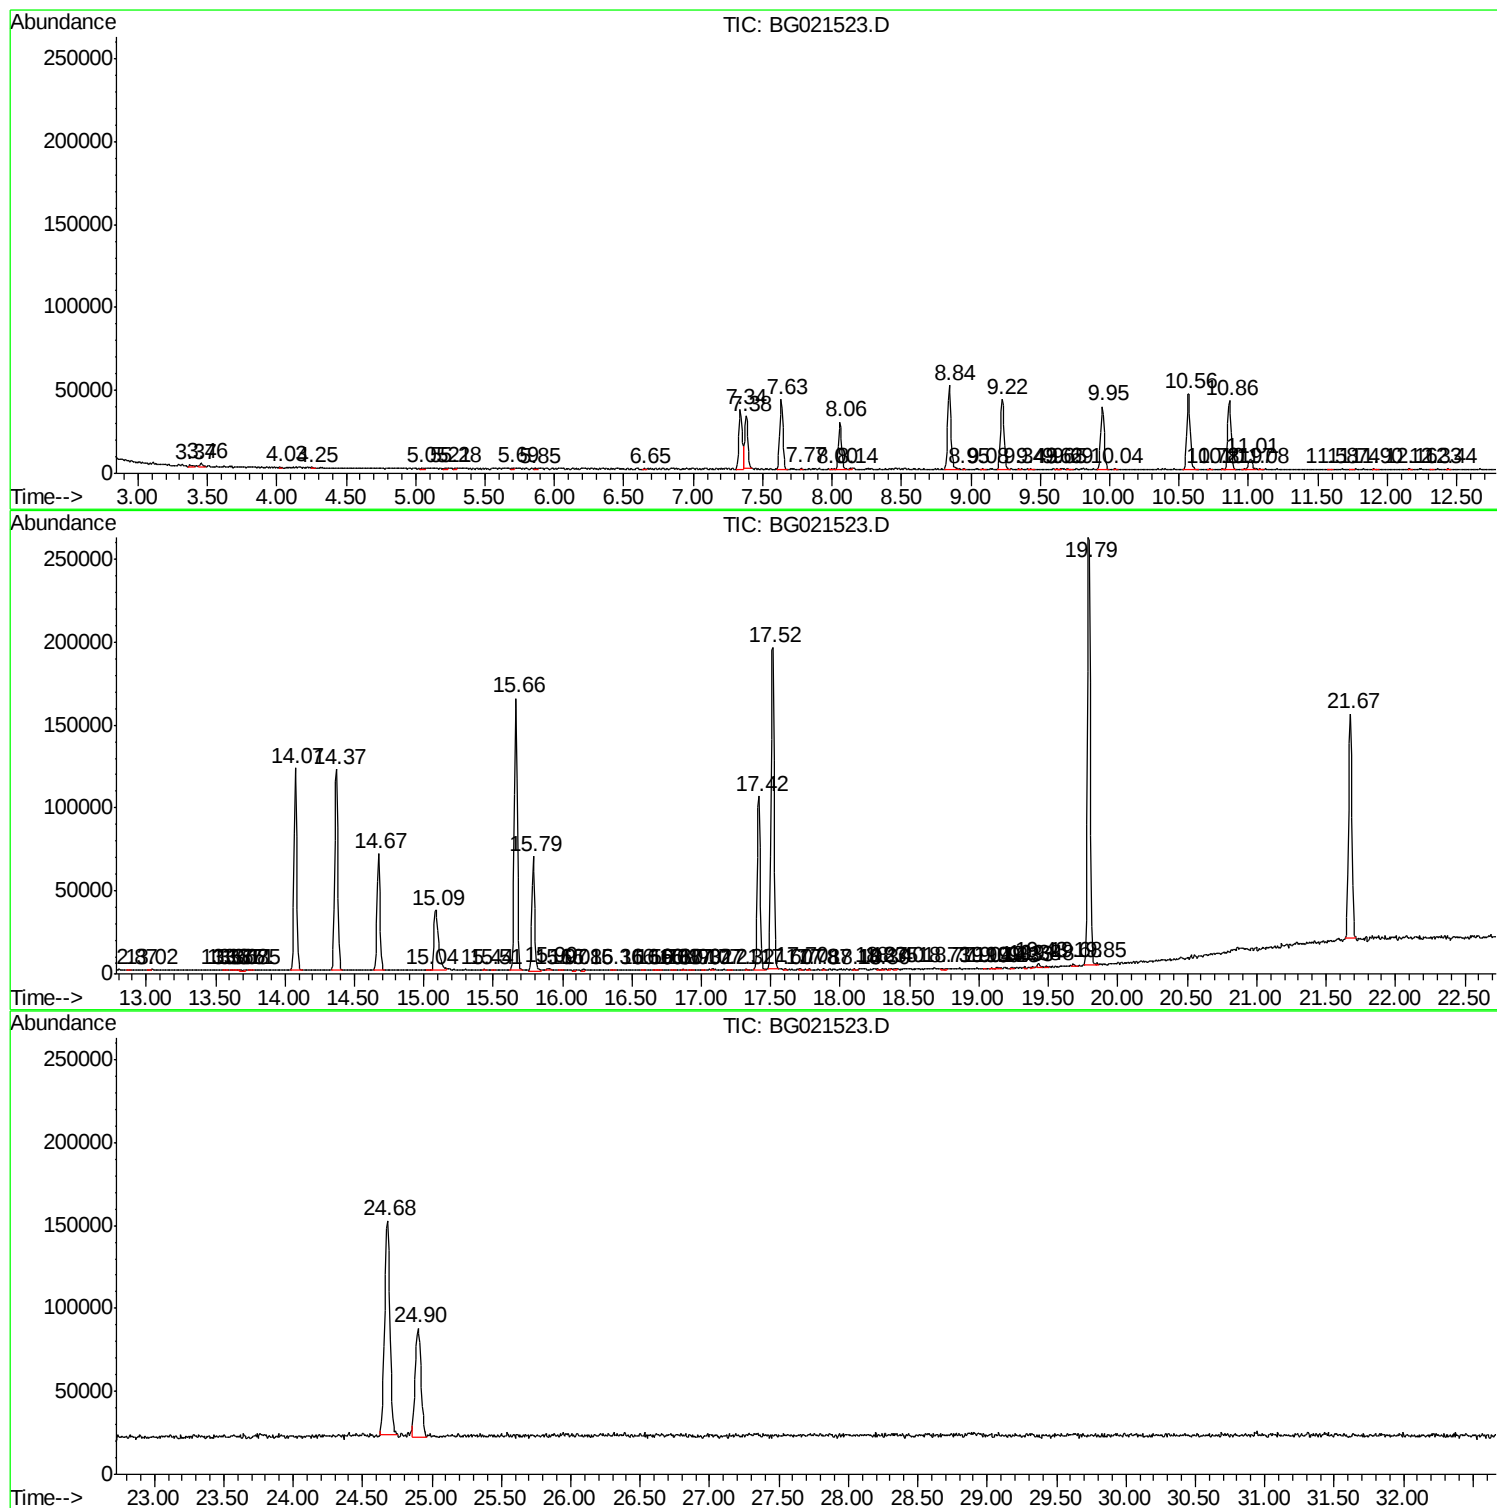

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG032816\
Data File : BG021523.D
Acq On : 28 Mar 2016 12:58
Operator : UM/SJ
Sample : PB89199BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK99

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG031616.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG032816\
Data File : BG021523.D
Acq On : 28 Mar 2016 12:58
Operator : UM/SJ
Sample : PB89199BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK99

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG031616.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc