

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG032817\
 Data File : BG026461.D
 Acq On : 28 Mar 2017 18:42
 Operator : SJ/MA
 Sample : I2372-11
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 G9Y62

Quant Time: Mar 29 01:52:22 2017
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG032717MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Mar 29 01:52:02 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.05	152	166761	20.00	ng/ul	0.00
18) Naphthalene-d8	10.84	136	681572	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.65	164	399361	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.38	188	961285	20.00	ng/ul	0.00
77) Chrysene-d12	21.62	240	1120235	20.00	ng/ul	0.00
85) Perylene-d12	24.80	264	1129646	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.47	96	21061	6.04	ng/uL	0.00
5) Phenol-d5	7.21	99	95025	7.74	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.36	67	246420	35.81	ng/ul	0.00
9) 2-Chlorophenol-d4	7.58	132	319631	29.03	ng/ul	0.00
13) 4-Methylphenol-d8	8.75	113	185720	18.77	ng/ul	0.00
19) Nitrobenzene-d5	9.20	128	188290	38.65	ng/ul	0.00
22) 2-Nitrophenol-d4	9.92	143	223836	39.21	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.47	165	353778	33.77	ng/ul	0.00
29) 4-Chloroaniline-d4	10.98	131	19951	1.91	ng/ul	0.01
43) Dimethylphthalate-d6	14.05	166	1216793	39.35	ng/ul	0.00
46) Acenaphthylene-d8	14.34	160	1459850	37.89	ng/ul	0.00
51) 4-Nitrophenol-d4	14.85	143	35463	5.89	ng/ul	0.01
57) Fluorene-d10	15.64	176	1132215	40.30	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.75	200	223225	36.11	ng/ul	0.00
70) Anthracene-d10	17.48	188	1775028	40.66	ng/ul	0.00
78) Pyrene-d10	19.76	212	2020540	40.44	ng/ul	0.00
89) Benzo(a)pyrene-d12	24.59	264	2045379	42.14	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
56) Diethylphthalate	15.45	149	33930	1.14	ng/ul#	89


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG032817\
Data File : BG026461.D
Acq On : 28 Mar 2017 18:42
Operator : SJ/MA
Sample : I2372-11
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
G9Y62

Quant Time: Mar 29 01:52:22 2017
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG032717MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Mar 29 01:52:02 2017
Response via : Initial Calibration

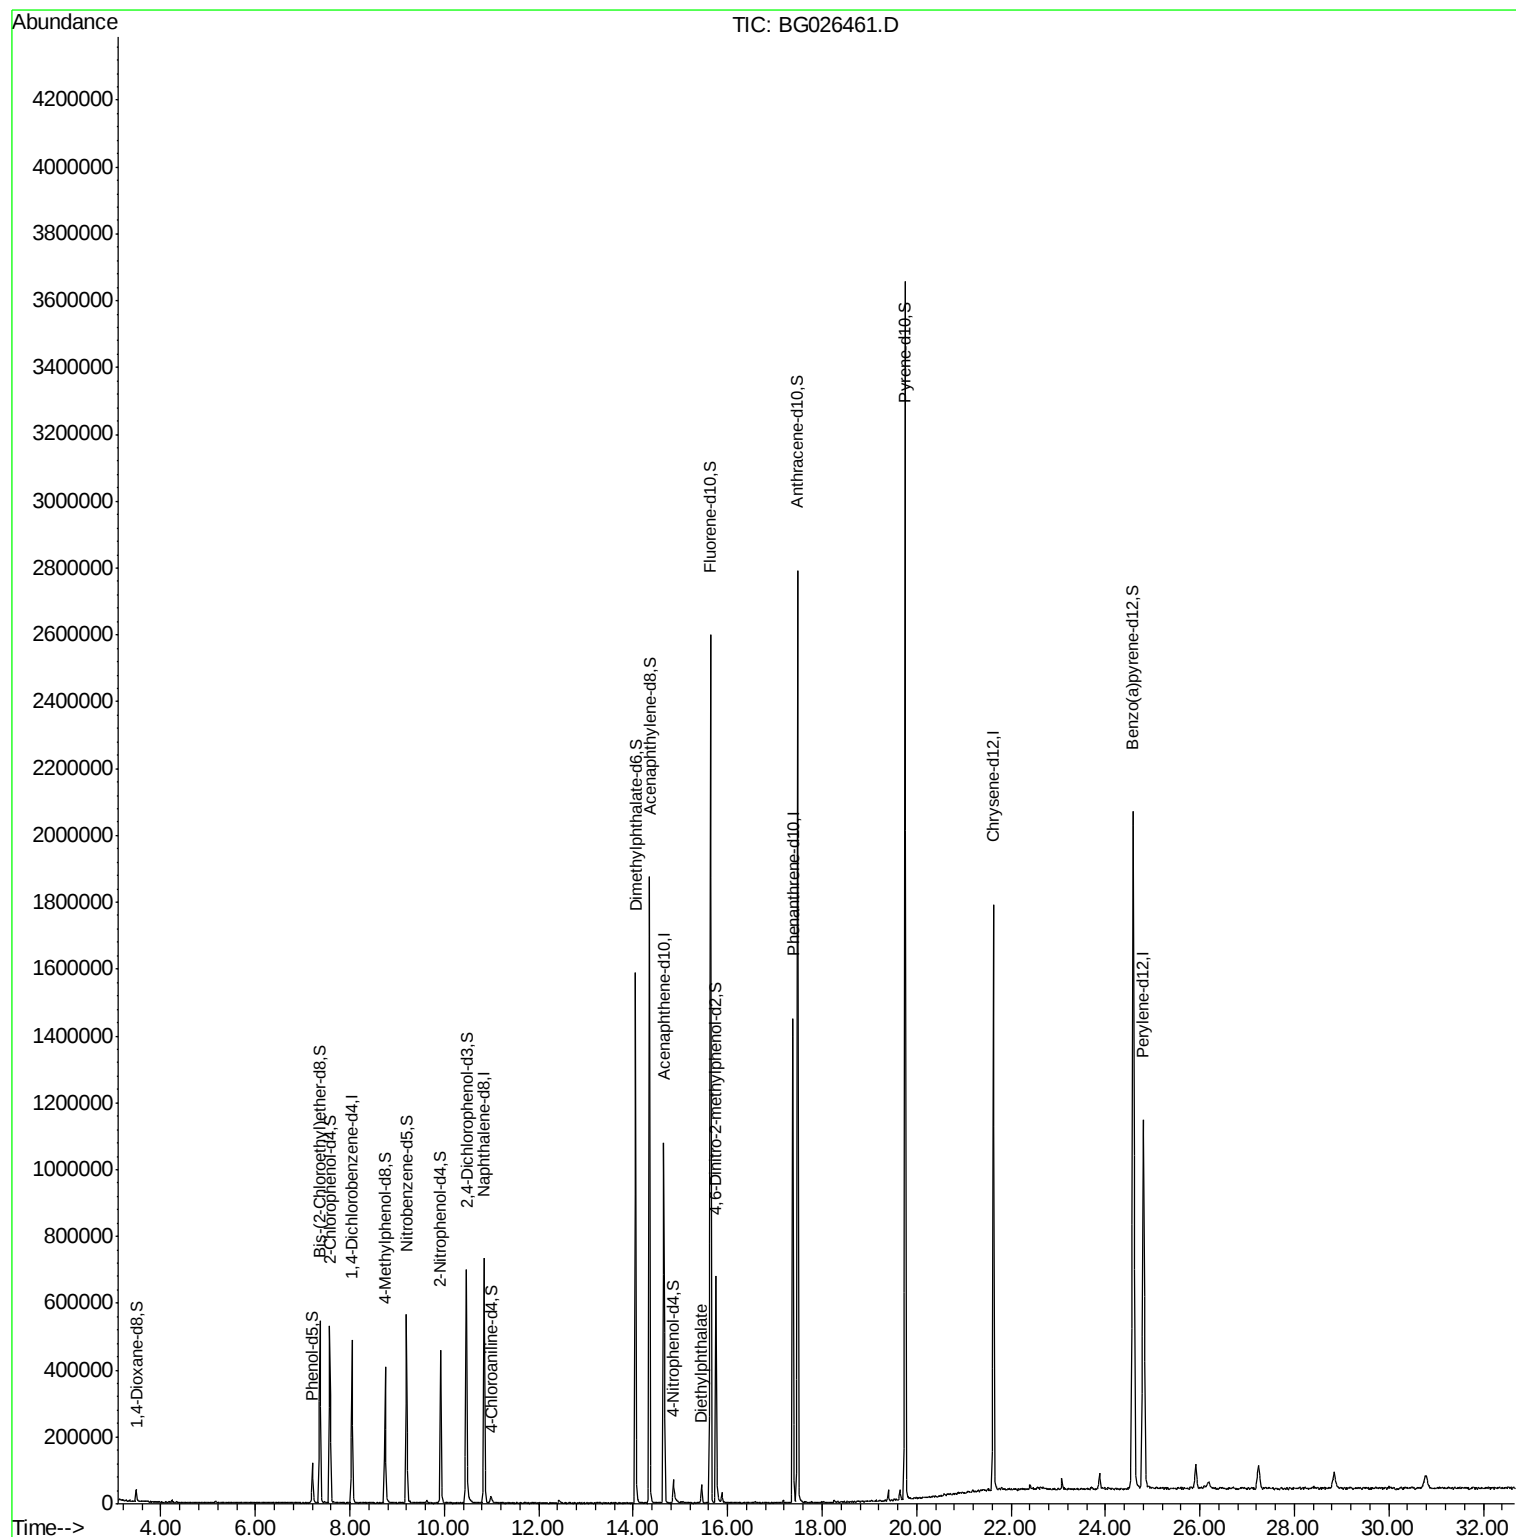

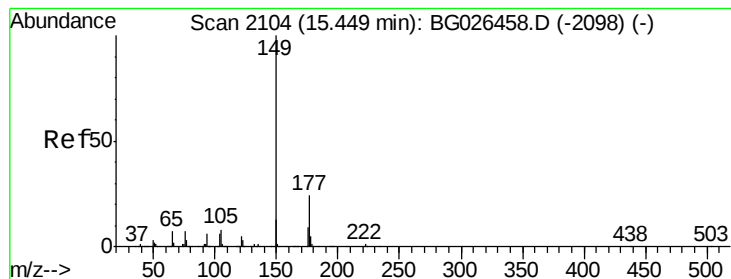

#56
 Diethylphthalate
 Concen: 1.14 ng/ul
 RT: 15.45 min Scan# 2104
 Delta R.T. 0.00 min
 Lab File: BG026461.D
 Acq: 28 Mar 2017 18:42

Instrument :
 BNA_G
 ClientSampleId :
 G9Y62

Tgt Ion	Ratio	Lower	Upper
149	100		
177	28.2	17.4	26.2#
150	14.7	10.0	15.0

