
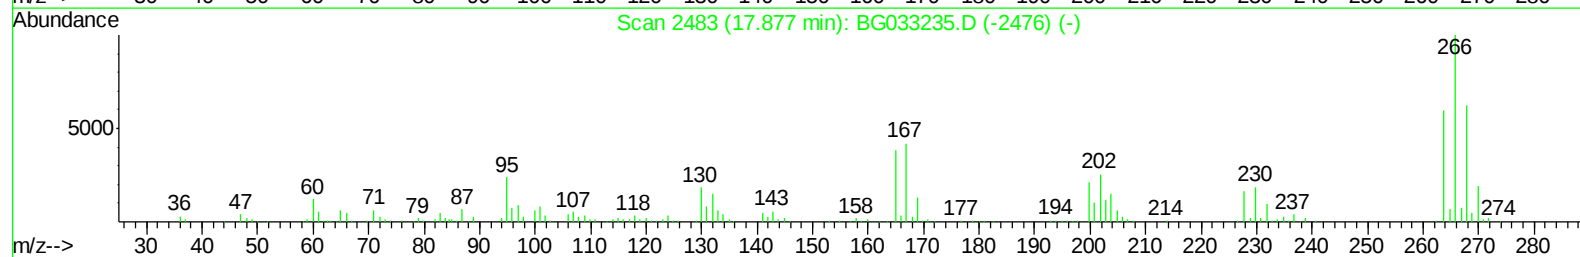
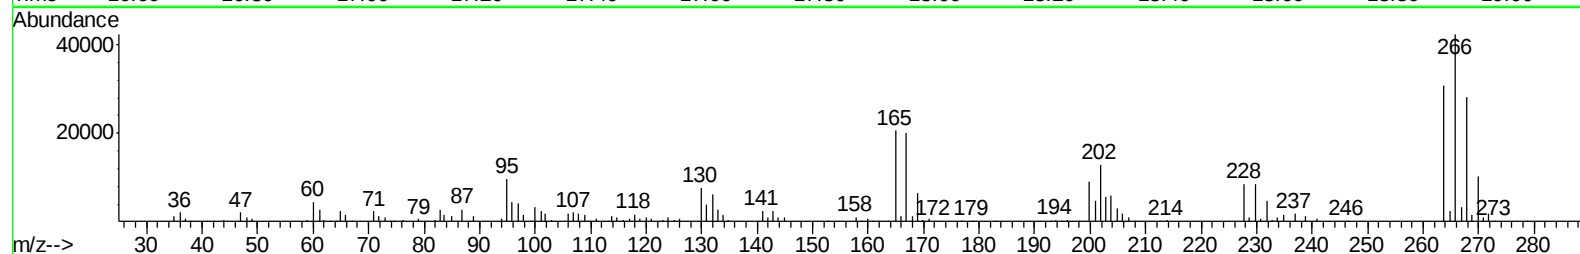


Data Path : Z:\HPCHEM1\BNA G\DATA\BG032818\
Data File : BG033386.D
Acq On : 28 Mar 2018 14:31
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 29 13:24:05 2018
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG031918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 28 18:34:58 2018
Response via : Initial Calibration

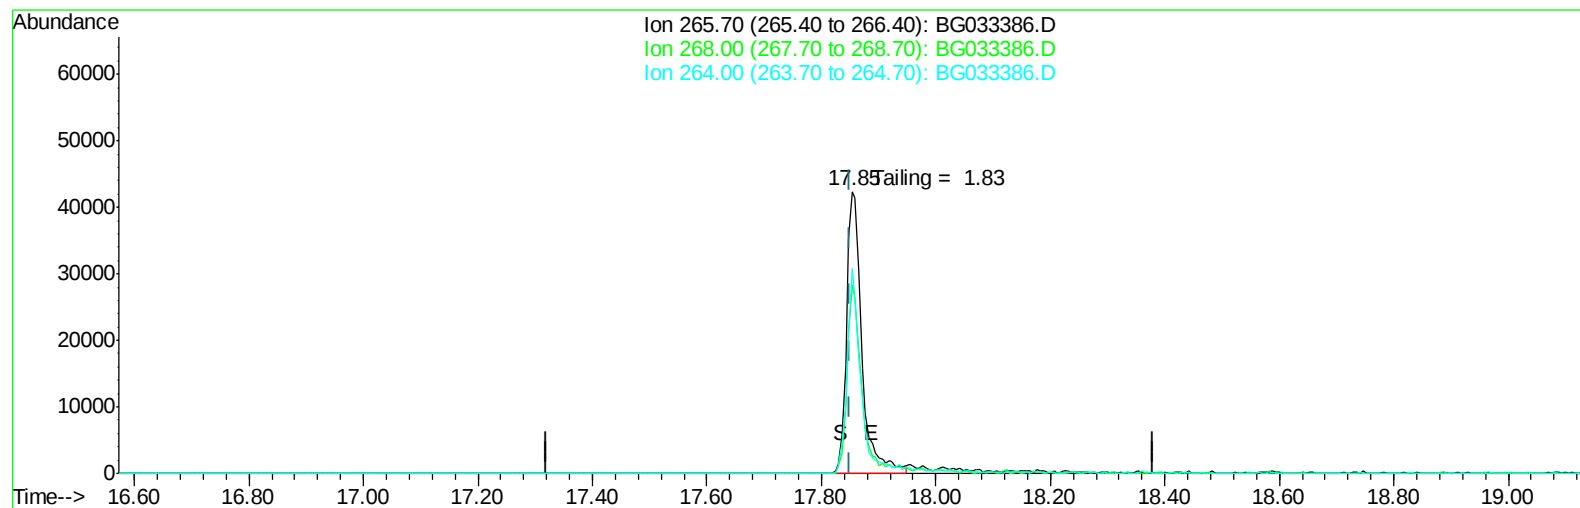

TIC: BG033386.D

(69) Pentachlorophenol (C)




17.854min (+0.003) 154396.91ng

response 78806

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	66.64
264.00	62.00	72.77
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA G\DATA\BG032818\
Data File : BG033386.D
Acq On : 28 Mar 2018 14:31
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 29 13:24:05 2018
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG031918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 28 18:34:58 2018
Response via : Initial Calibration

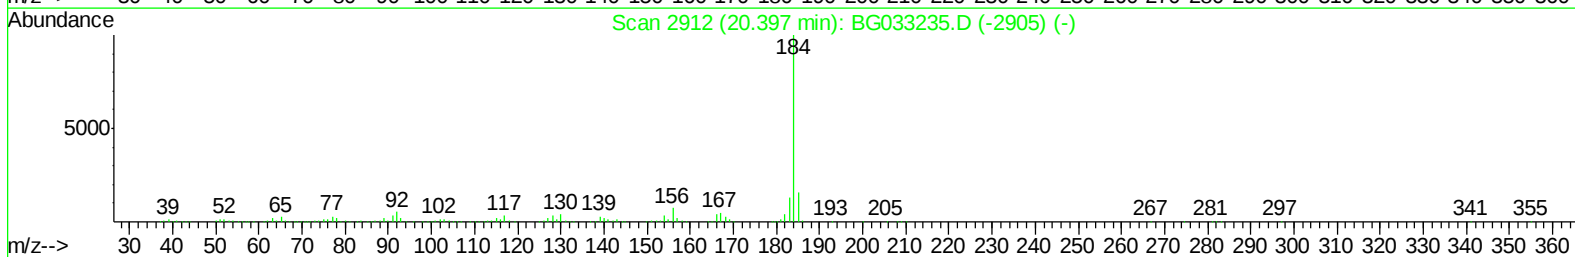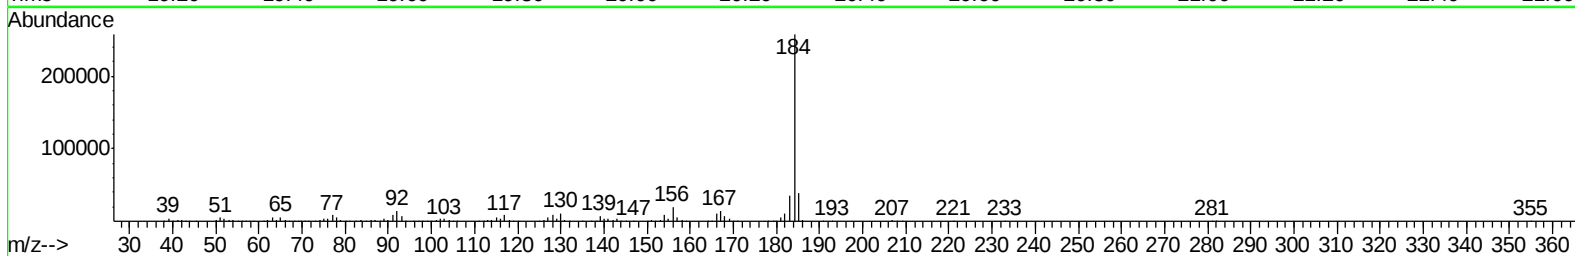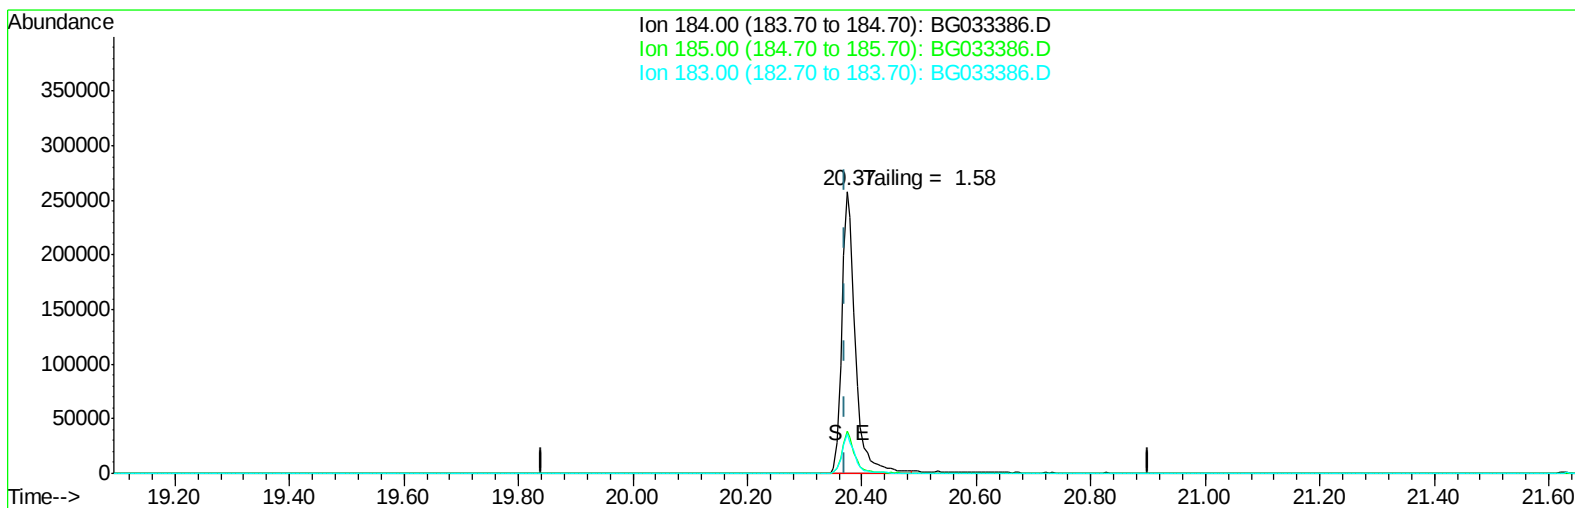

TIC: BG033386.D

(76) Benzidine

20.374min (+0.003) 0.00ng

response 428049

Ion	Exp%	Act%
184.00	100	100
185.00	13.90	14.87
183.00	13.30	13.91
0.00	0.00	0.00