
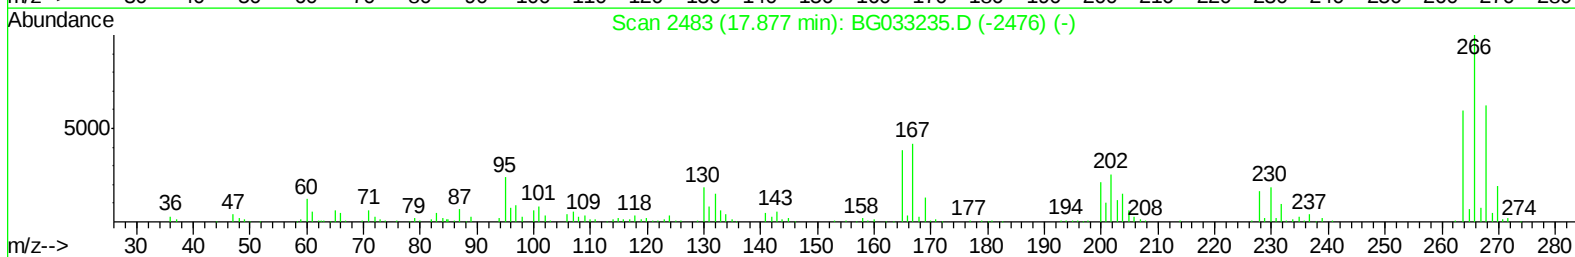
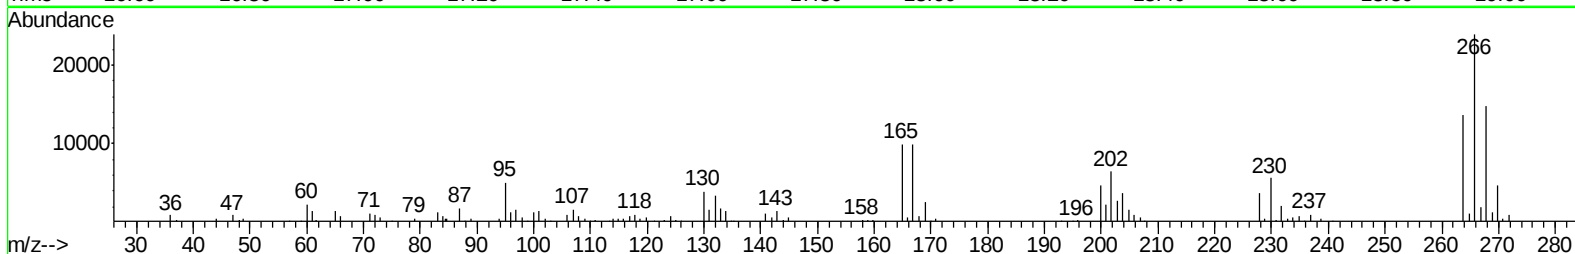


Data Path : Z:\HPCHEM1\BNA G\DATA\BG032818\
Data File : BG033404.D
Acq On : 29 Mar 2018 3:44
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 29 13:29:15 2018
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG031918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 28 18:34:58 2018
Response via : Initial Calibration

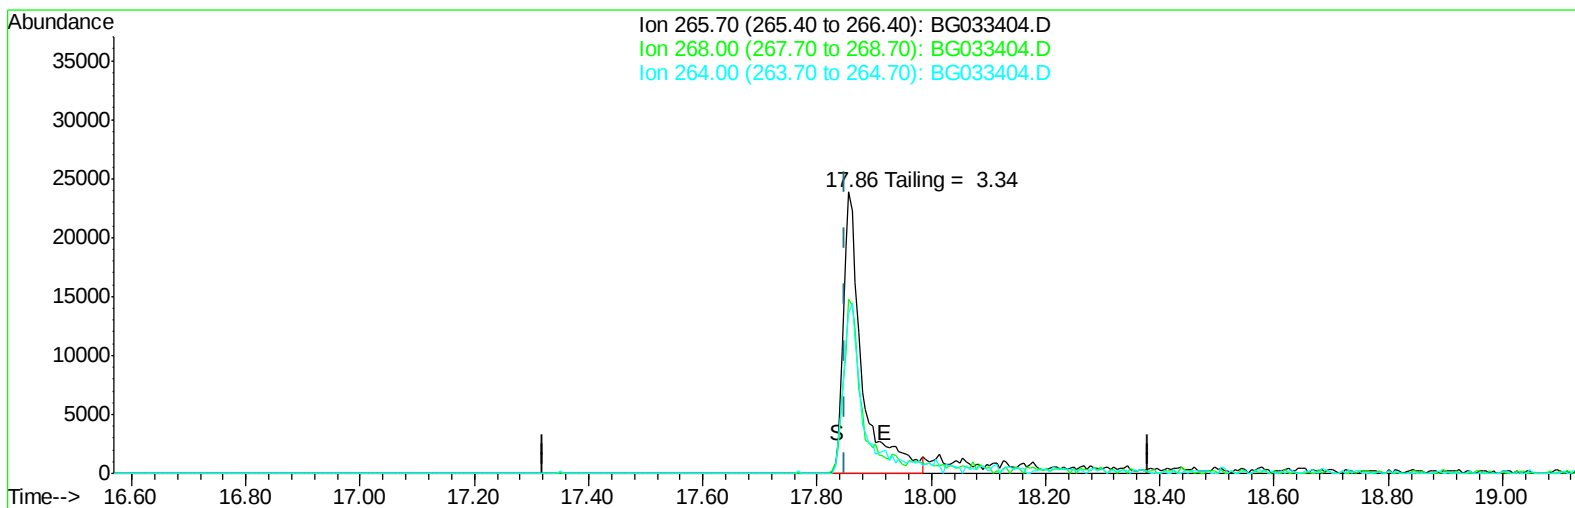

TIC: BG033404.D

(69) Pentachlorophenol (C)




17.855min (+0.005) 103690.48ng

response 54689

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	61.96
264.00	62.00	56.95
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA G\DATA\BG032818\
Data File : BG033404.D
Acq On : 29 Mar 2018 3:44
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 29 13:29:15 2018
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG031918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 28 18:34:58 2018
Response via : Initial Calibration

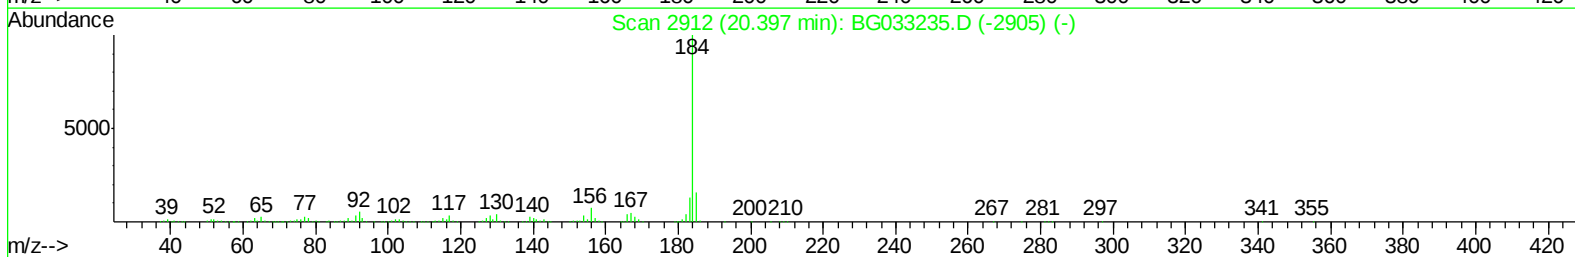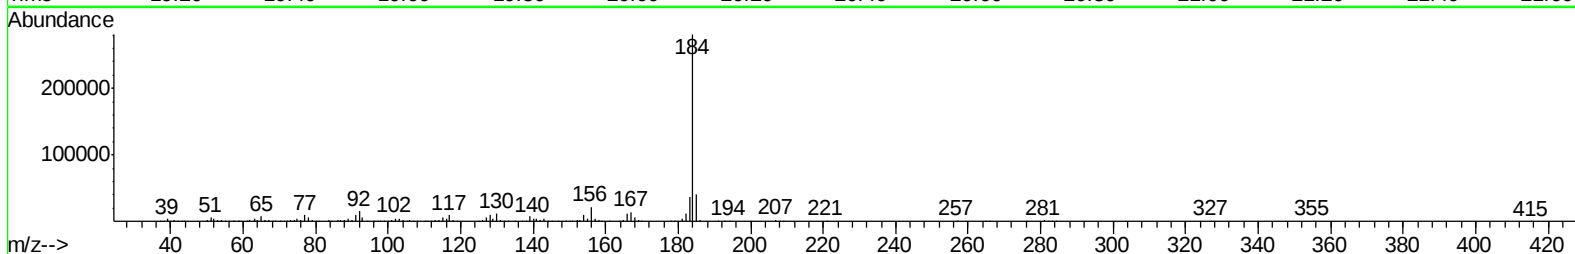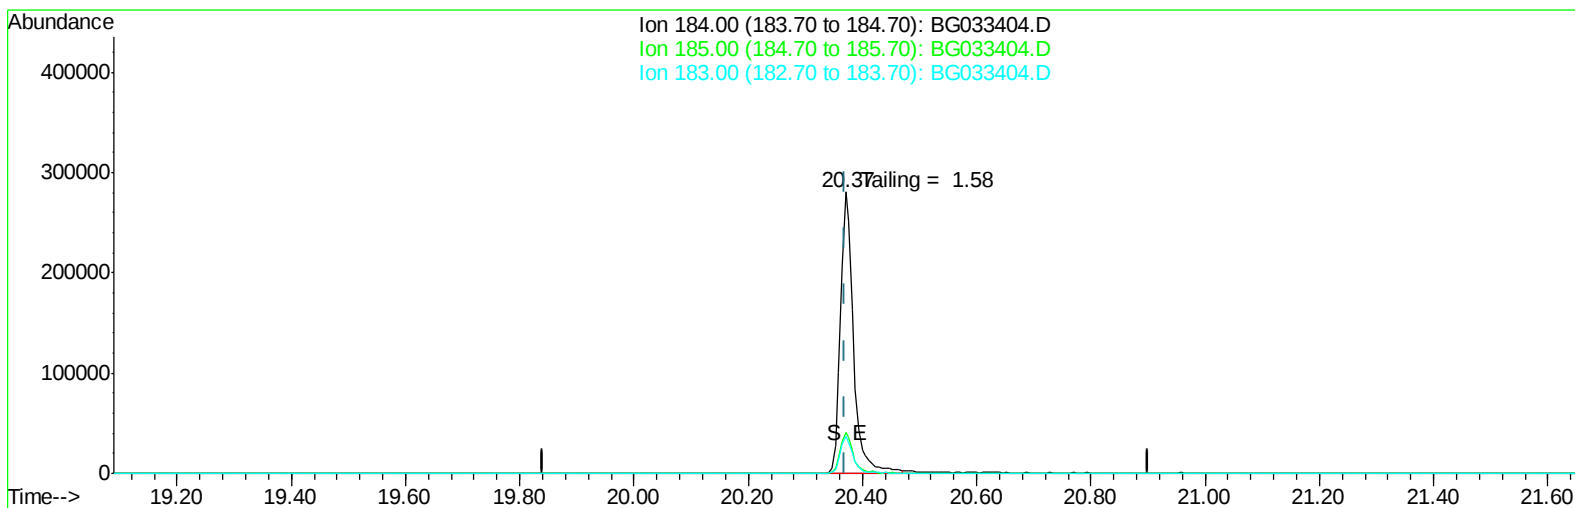

TIC: BG033404.D

(76) Benzidine

20.370min (-0.001) 264723.28ng

response 452271

Ion	Exp%	Act%
184.00	100	100
185.00	13.90	14.72
183.00	13.30	13.39
0.00	0.00	0.00