

Data Path : Z:\HPCHEM1\BNA G\DATA\BG032818\
 Data File : BG033388.D
 Acq On : 28 Mar 2018 16:28
 Operator : SJ/JU
 Sample : J2071-10
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 TP-7-DB

Quant Time: Mar 28 18:38:47 2018
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG031918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Mar 28 18:29:08 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.87	152	42983	20.00	ng	0.00
21) Naphthalene-d8	11.75	136	181470	20.00	ng	0.00
38) Acenaphthene-d10	15.48	164	138442	20.00	ng	0.00
63) Phenanthrene-d10	18.21	188	357736	20.00	ng	0.00
75) Chrysene-d12	22.56	240	367115	20.00	ng	0.00
86) Perylene-d12	26.33	264	387147	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	6.29	112	122544	53.46	ng	0.00
7) Phenol-d6	7.97	99	109296	27.75	ng	0.00
23) Nitrobenzene-d5	10.07	82	292399	74.03	ng	0.00
41) 2,4,6-Tribromophenol	16.96	330	218881	105.71	ng	0.00
44) 2-Fluorobiphenyl	14.11	172	702489	73.25	ng	0.00
78) Terphenyl-d14	20.73	244	1291768	75.25	ng	0.00


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG032818\
Data File : BG033388.D
Acq On : 28 Mar 2018 16:28
Operator : SJ/JU
Sample : J2071-10
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
TP-7-DB

Quant Time: Mar 28 18:38:47 2018
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG031918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 28 18:29:08 2018
Response via : Initial Calibration

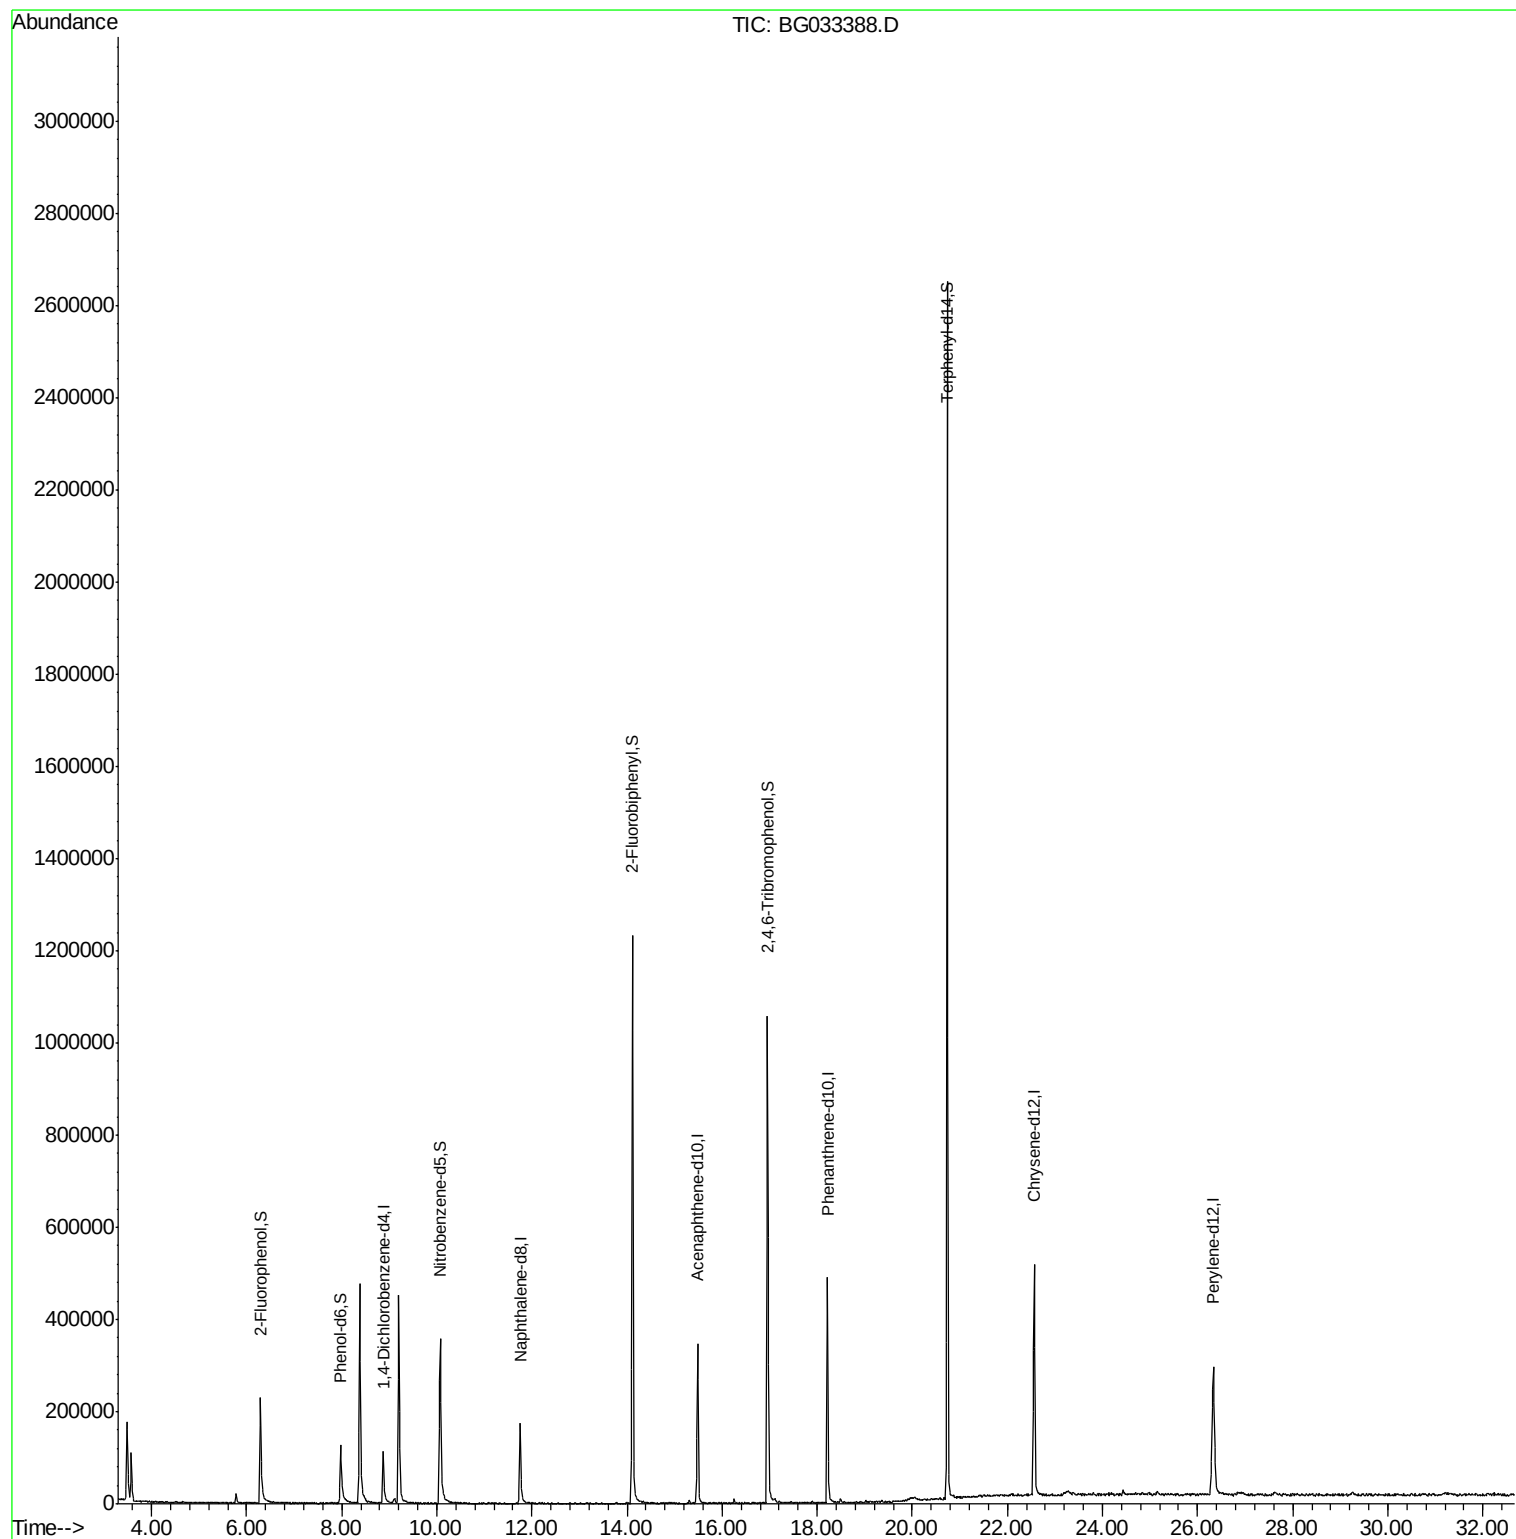

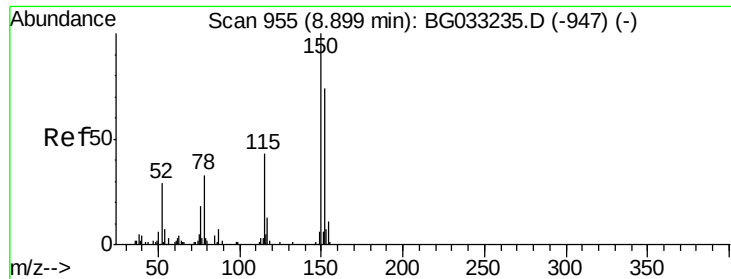


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.87 min Scan# 950
Delta R.T. -0.01 min
Lab File: BG033388.D
Acq: 28 Mar 2018 16:28

Instrument :
BNA_G
ClientSampleId :
TP-7-DB

Tot Ion	Ratio	Lower	Upper
152	100		
150	156.2	126.6	189.8
115	59.1	53.0	79.4

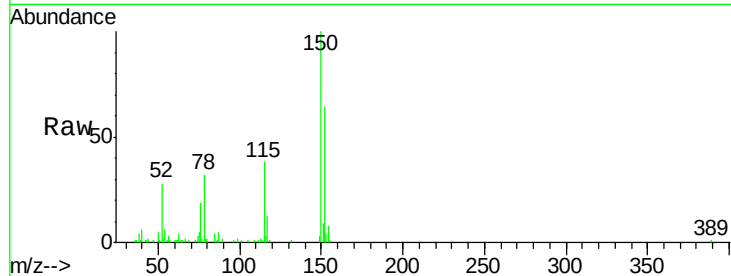


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

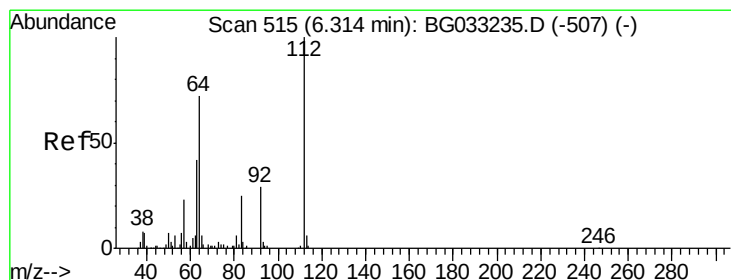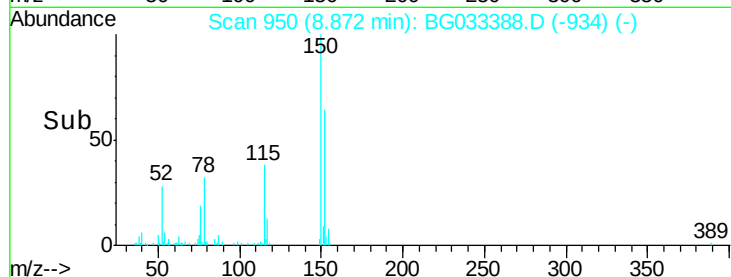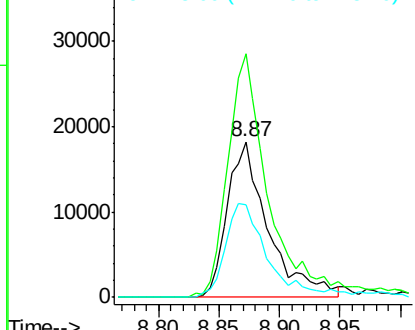



#5


2-Fluorophenol
Concen: 53.459 ng
RT: 6.29 min Scan# 511
Delta R.T. -0.00 min
Lab File: BG033388.D
Acq: 28 Mar 2018 16:28

Tgt Ion	Ratio	Lower	Upper
112	100		
64	75.0	56.3	84.5
63	41.9	30.1	45.1

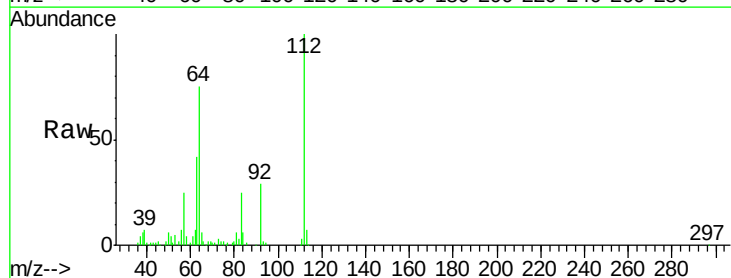

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BG
Ion 63.00 (62.70 to 63.70): BG

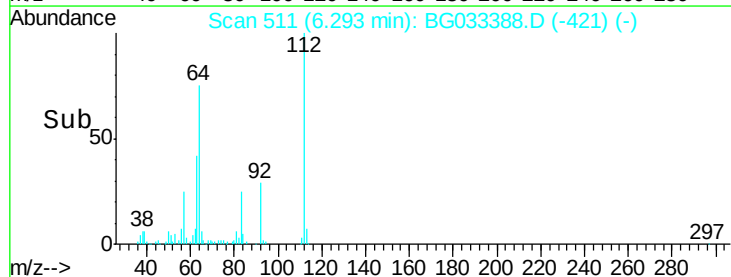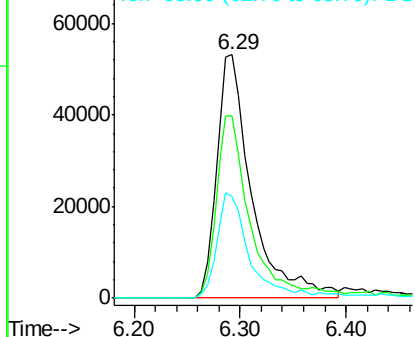

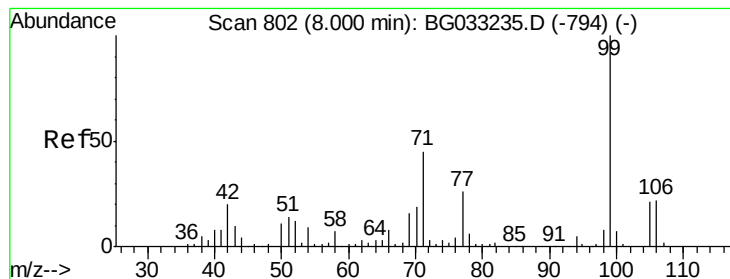

#7

Phenol-d6

Concen: 27.750 ng

RT: 7.97 min Scan# 797

Delta R.T. -0.01 min

Lab File: BG033388.D

Acq: 28 Mar 2018 16:28

Instrument :

BNA_G

ClientSampled :

TP-7-DB


Tot Ion: 99 Resp: 109296

Ion Ratio Lower Upper




99 100

42 18.3 14.1 21.1

71 39.3 26.1 39.1#

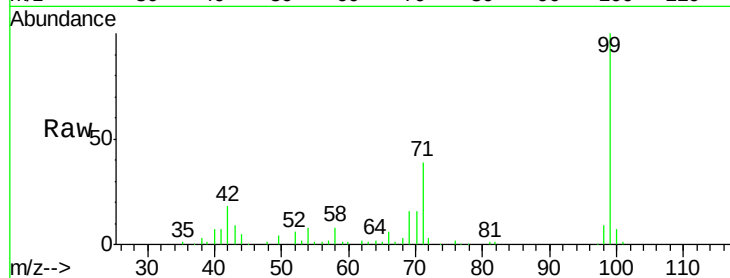

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

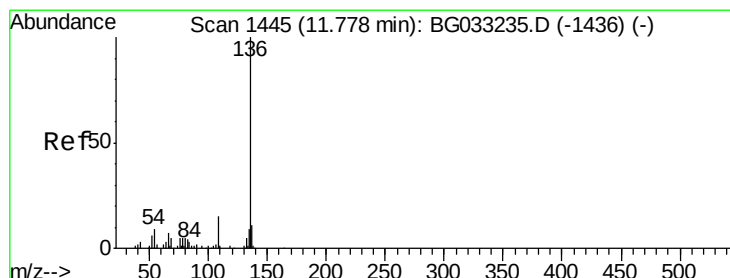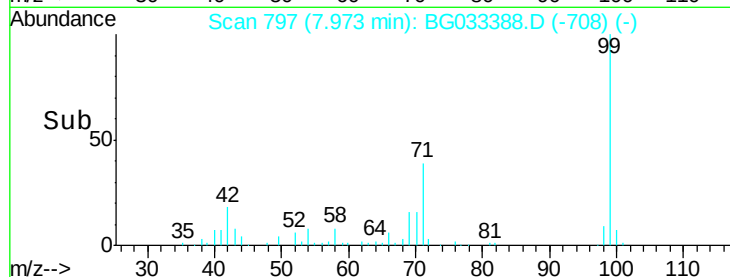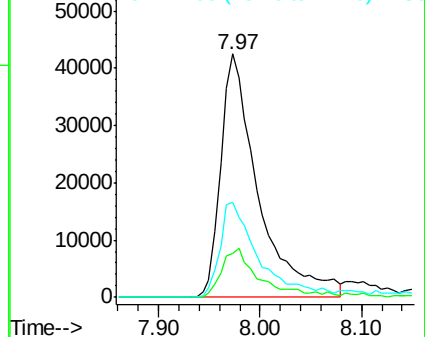

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 11.75 min Scan# 1440

Delta R.T. -0.01 min

Lab File: BG033388.D

Acq: 28 Mar 2018 16:28

Tgt Ion: 136 Resp: 181470


Ion Ratio Lower Upper

136 100



137 9.4 9.2 13.8


54 10.3 10.3 15.5#

68 3.9 4.5 6.7#

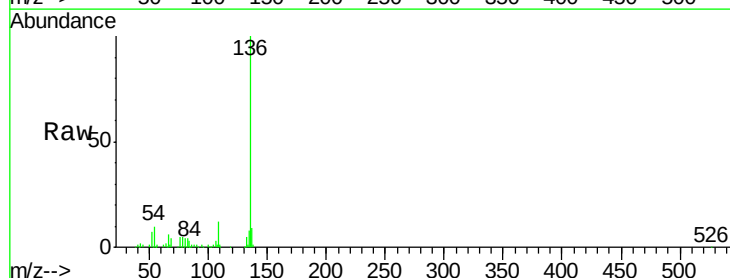

Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC



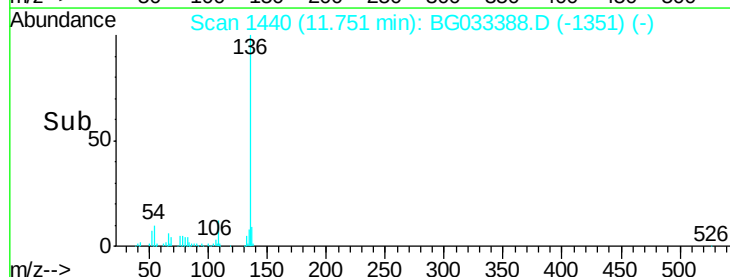
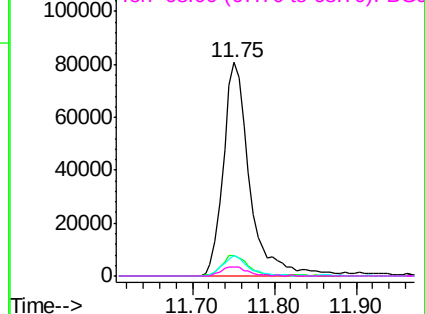


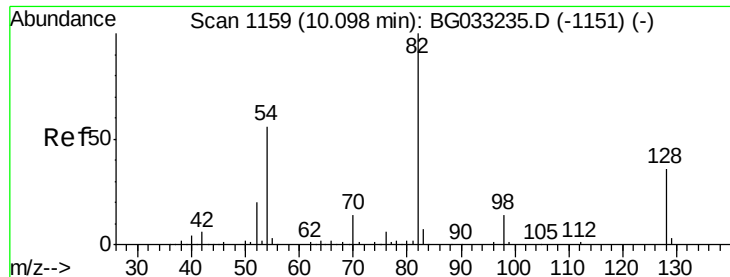

#23
 Nitrobenzene-d5
 Concen: 74.029 ng
 RT: 10.07 min Scan# 1154
 Delta R.T. -0.01 min
 Lab File: BG033388.D
 Acq: 28 Mar 2018 16:28




Instrument :
 BNA_G
 ClientSampleId :
 TP-7-DB


Tot Ion: 82 Resp: 292399
 Ion Ratio Lower Upper
 82 100
 128 40.2 29.7 44.5
 54 56.2 43.1 64.7

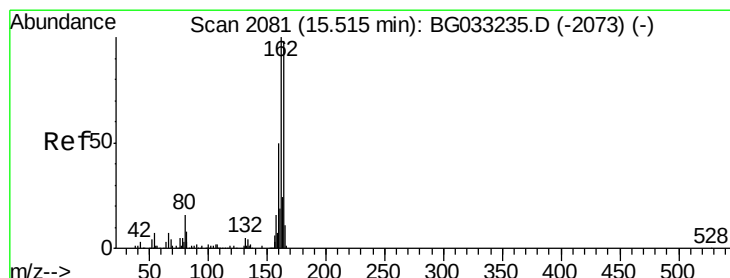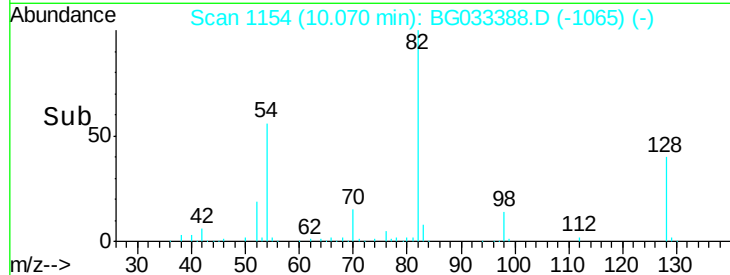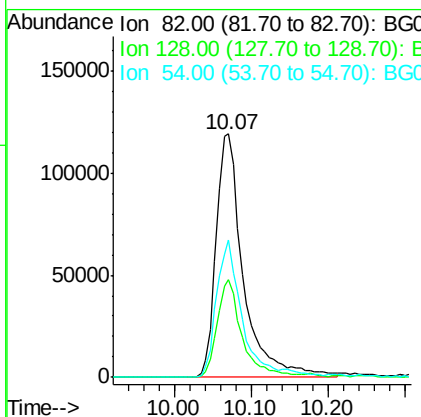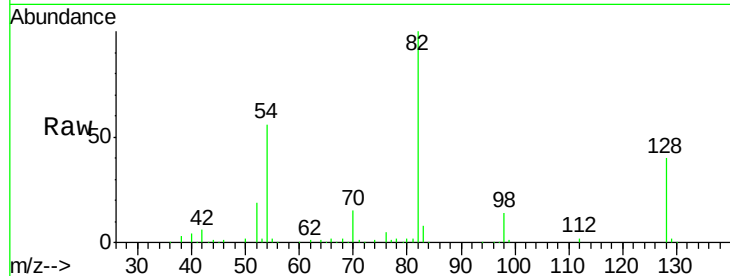

#38
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 15.48 min Scan# 2075
 Delta R.T. -0.01 min
 Lab File: BG033388.D
 Acq: 28 Mar 2018 16:28

Tgt Ion: 164 Resp: 138442
 Ion Ratio Lower Upper
 164 100
 162 95.2 78.8 118.2
 160 41.5 35.4 53.0

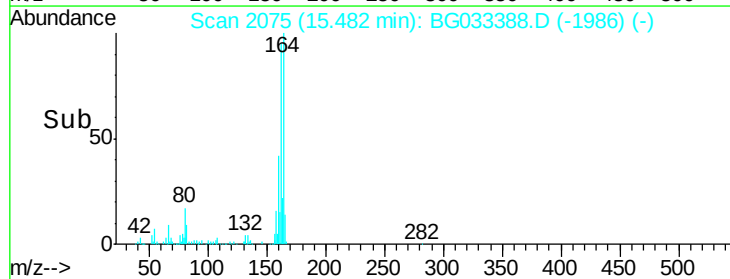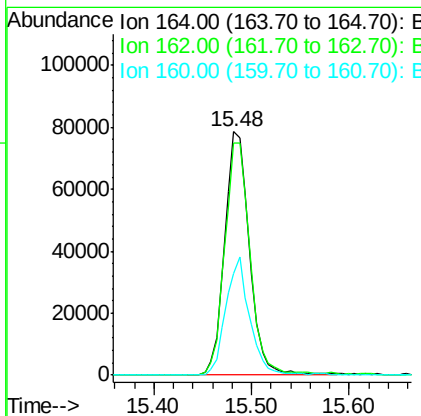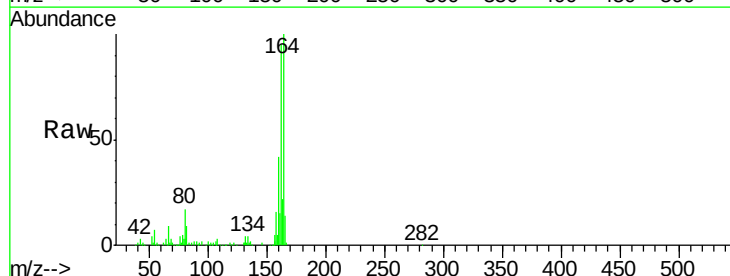


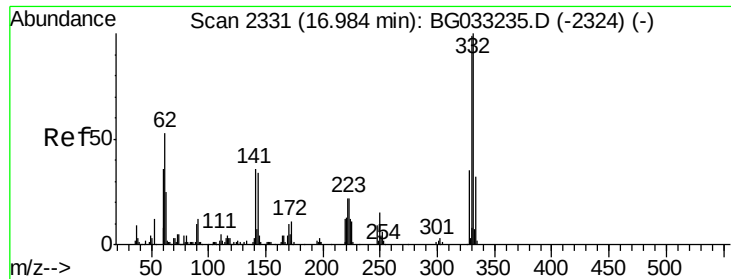




#41
 2,4,6-Tribromophenol
 Concen: 105.711 ng
 RT: 16.96 min Scan# 2326
 Delta R.T. -0.00 min
 Lab File: BG033388.D
 Acq: 28 Mar 2018 16:28

Instrument :
 BNA_G
 ClientSampleId :
 TP-7-DB

Tot Ion	Ratio	Lower	Upper
330	100		
332	98.3	77.0	115.6
141	36.7	25.2	37.8

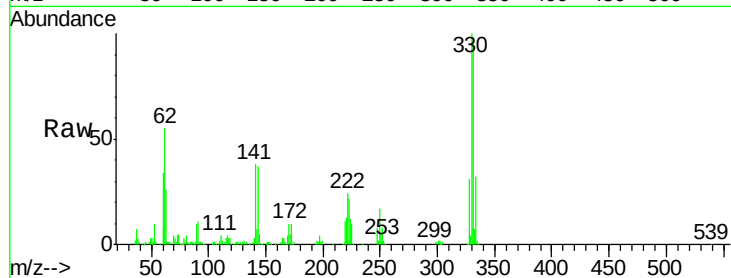


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

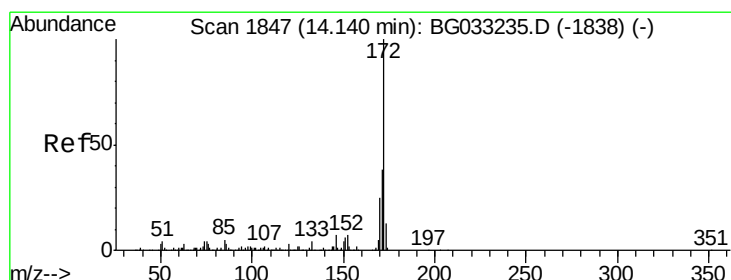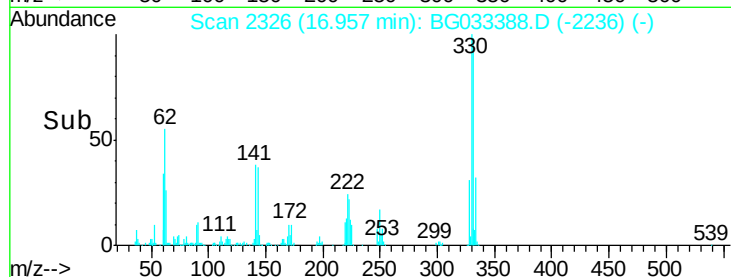
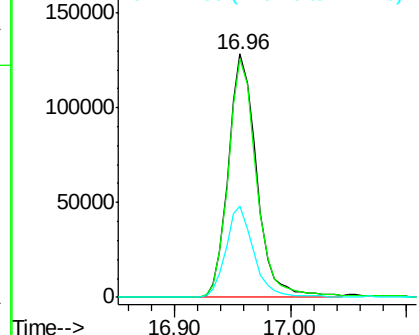



#44
 2-Fluorobiphenyl
 Concen: 73.254 ng
 RT: 14.11 min Scan# 1842
 Delta R.T. -0.00 min
 Lab File: BG033388.D
 Acq: 28 Mar 2018 16:28

Tgt Ion	Ratio	Lower	Upper
172	100		
171	36.5	30.0	45.0
170	24.6	19.5	29.3

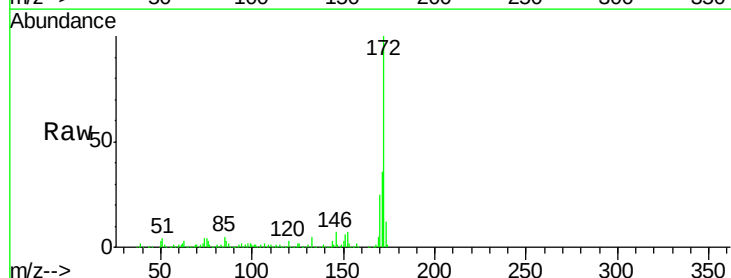

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E



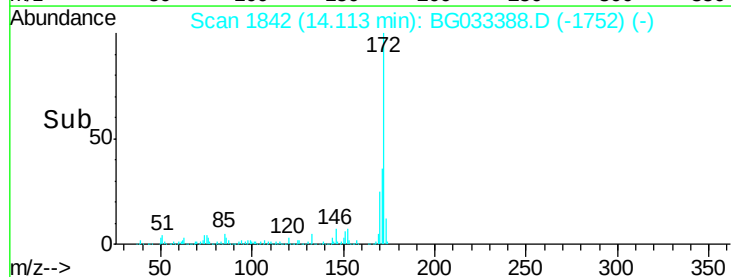
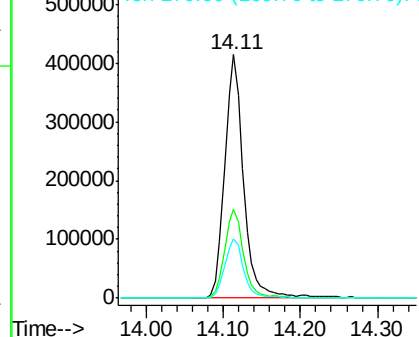


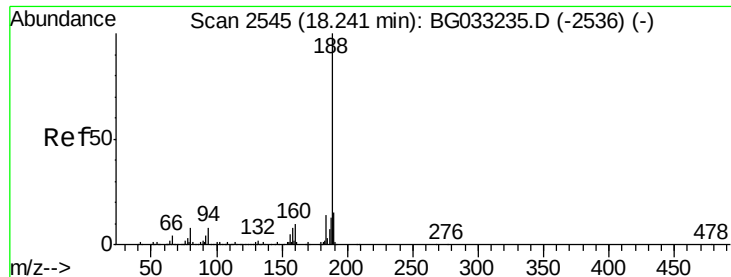

#63
Phenanthrene-d10
Concen: 20.000 ng
RT: 18.21 min Scan# 2540
Delta R.T. -0.00 min
Lab File: BG033388.D
Acq: 28 Mar 2018 16:28




Instrument :
BNA_G
ClientSampleId :
TP-7-DB


Tot Ion:188 Resp: 357736
Ion Ratio Lower Upper
188 100
94 6.4 6.9 10.3#
80 7.4 7.7 11.5#

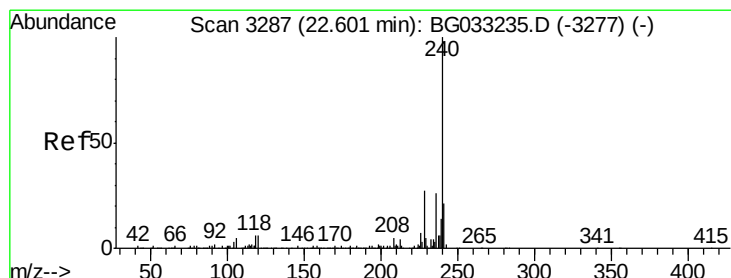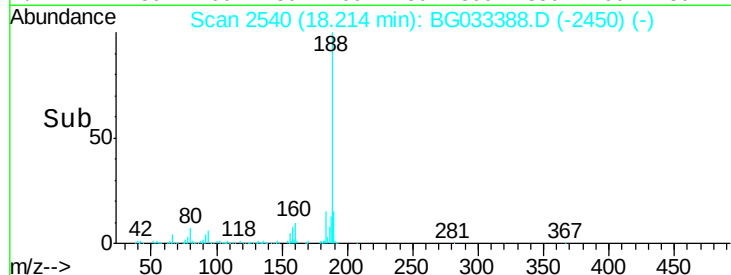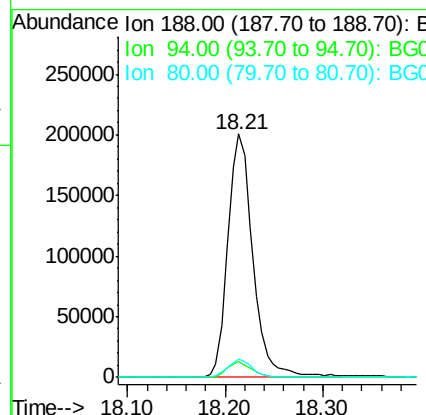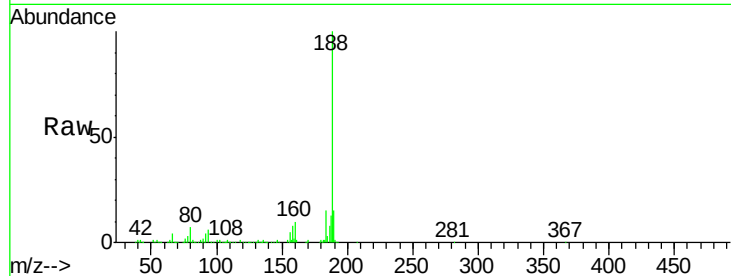

#75
Chrysene-d12
Concen: 20.000 ng
RT: 22.56 min Scan# 3280
Delta R.T. -0.00 min
Lab File: BG033388.D
Acq: 28 Mar 2018 16:28

Tgt Ion:240 Resp: 367115
Ion Ratio Lower Upper
240 100
120 6.0 6.8 10.2#
236 26.3 20.9 31.3

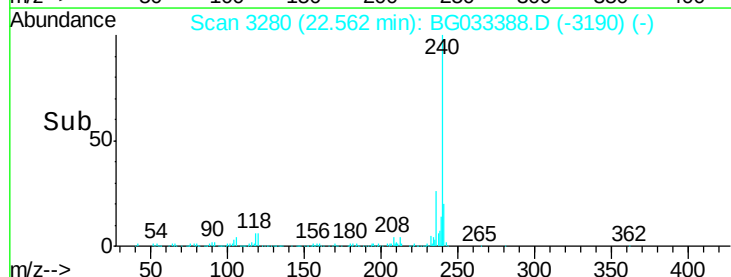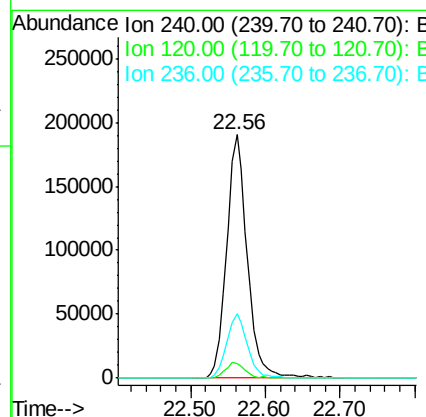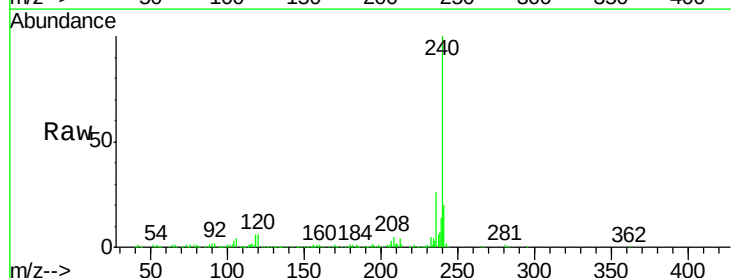

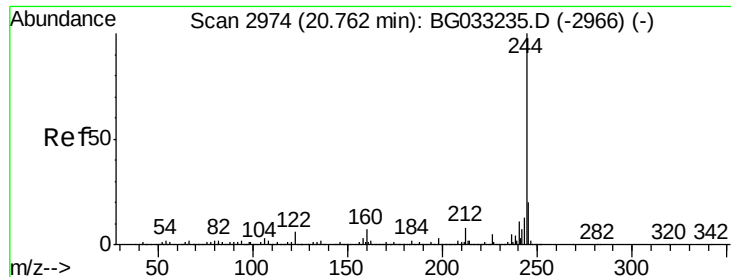

#78

Terphenyl-d14

Concen: 75.251 ng

RT: 20.73 min Scan# 2969

Delta R.T. -0.00 min

Lab File: BG033388.D

Acq: 28 Mar 2018 16:28

Instrument :

BNA_G

ClientSampleId :

TP-7-DB


Tot Ion:244 Resp: 1291768

Ion Ratio Lower Upper

244 100

212 8.4 5.8 8.8




122 7.3 7.0 10.4

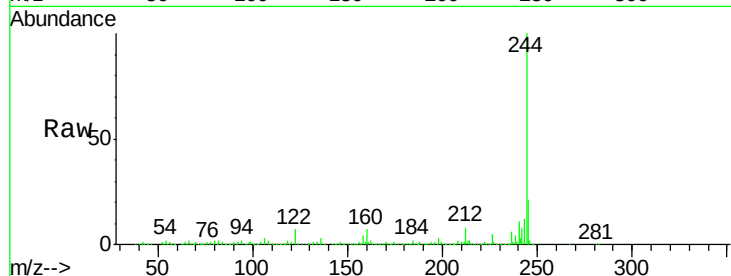

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

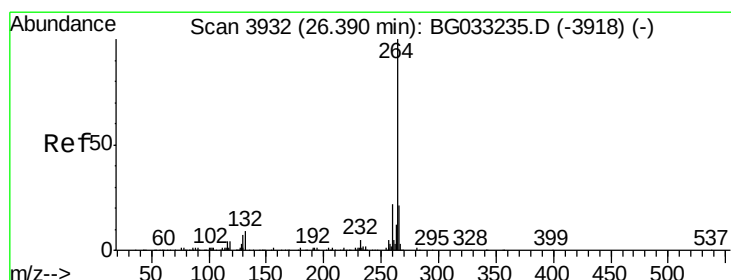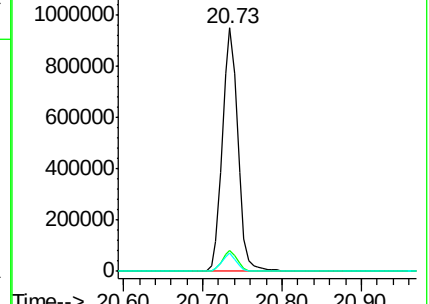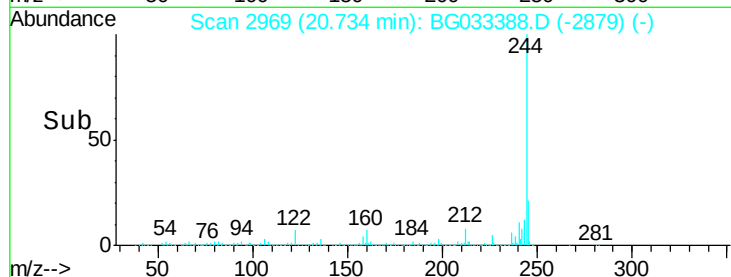

#86

Perylene-d12

Concen: 20.000 ng

RT: 26.33 min Scan# 3921

Delta R.T. -0.01 min

Lab File: BG033388.D

Acq: 28 Mar 2018 16:28


Tgt Ion:264 Resp: 387147

Ion Ratio Lower Upper

264 100

260 24.9 17.4 26.0

265 20.9 17.7 26.5

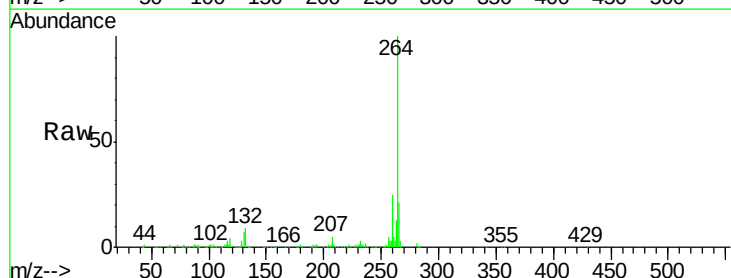

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

