


Data Path : Z:\HPCHEM1\BNA G\DATA\BG032818\
 Data File : BG033386.D
 Acq On : 28 Mar 2018 14:31
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG031918.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Mar 28 18:34:58 2018

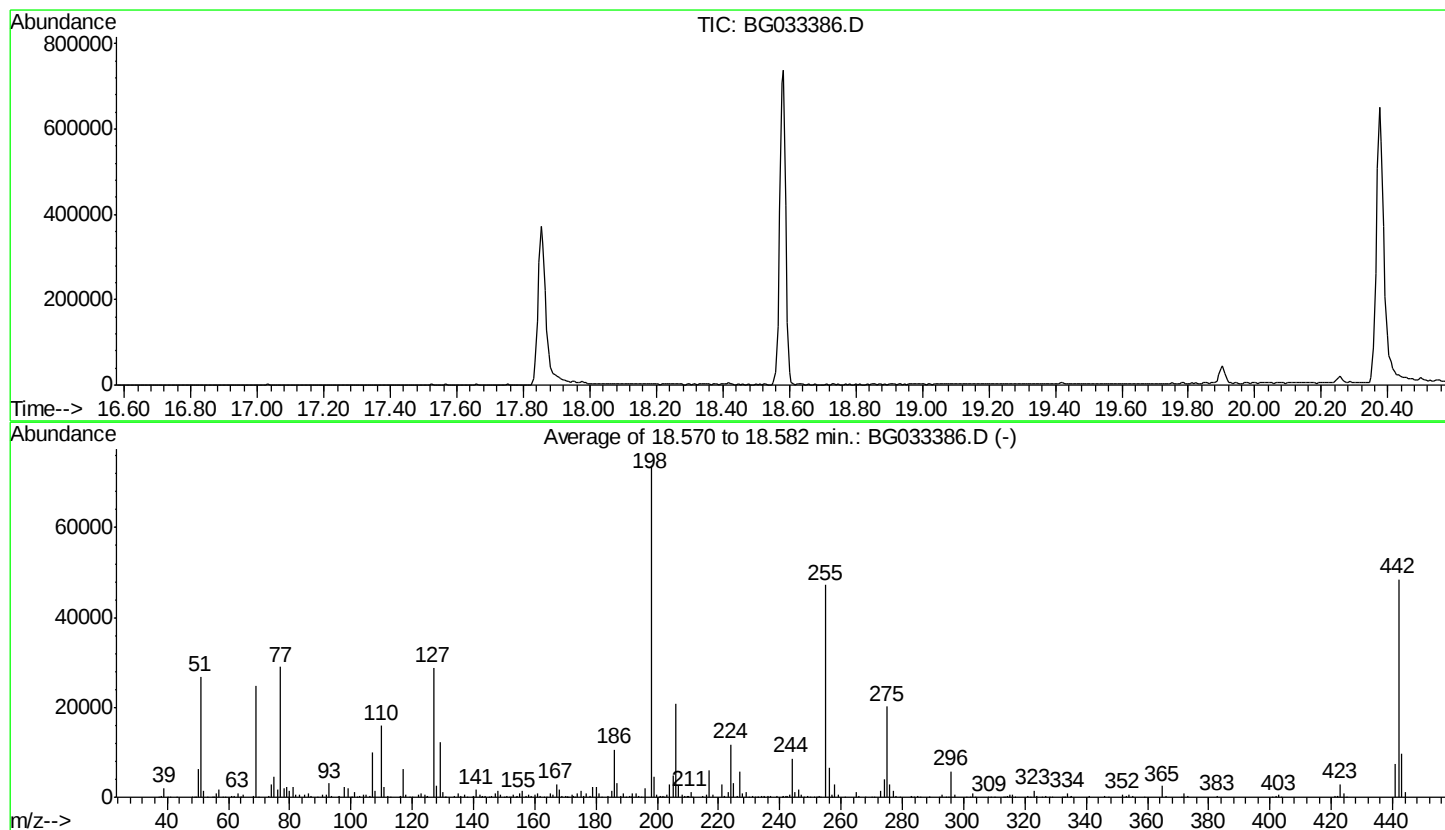

AutoFind: Scans 2601, 2602, 2603; Background Corrected with Scan 2595

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.3	26800	PASS
68	69	0.00	2	1.4	344	PASS
69	198	0.00	100	33.7	24856	PASS
70	69	0.00	2	0.4	97	PASS
127	198	10	80	39.1	28826	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	73802	PASS
199	198	5	9	6.2	4608	PASS
275	198	10	60	27.3	20124	PASS
365	198	1	100	3.4	2545	PASS
441	443	0.01	100	77.9	7540	PASS
442	198	50	100	65.7	48496	PASS
443	442	15	24	20.0	9682	PASS