




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032822\
Data File : BG052893.D
Acq On : 28 Mar 2022 16:05
Operator : CG/JU
Sample : N2082-16
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
EW615

Manual IntegrationsAPPROVED

Quant Time: Mar 29 01:00:04 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Mar 23 13:16:32 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 03/29/2022
Supervised By :mohammad ahmed 03/29/2022

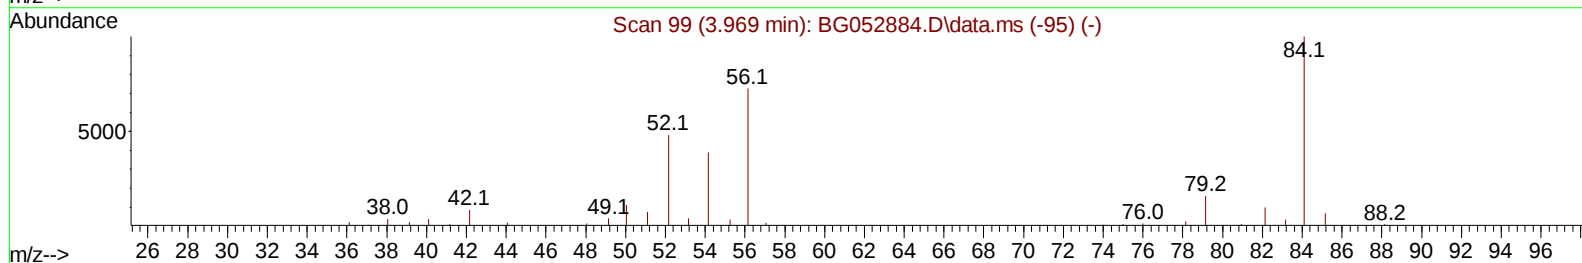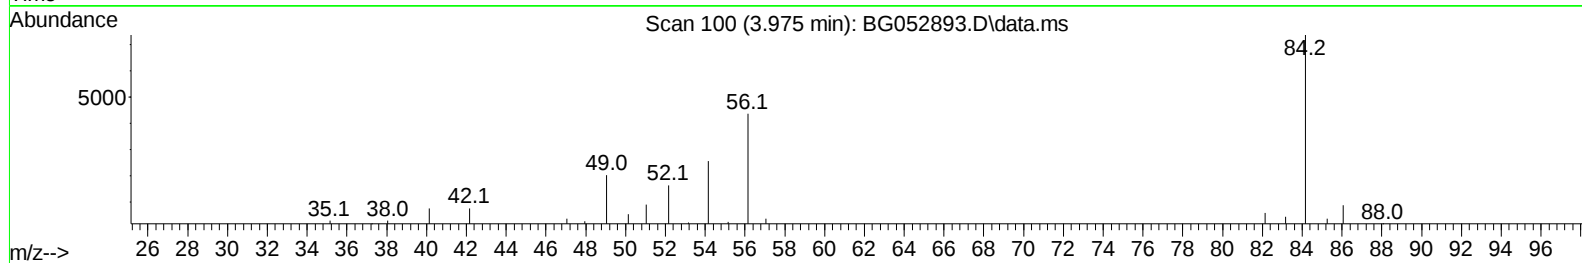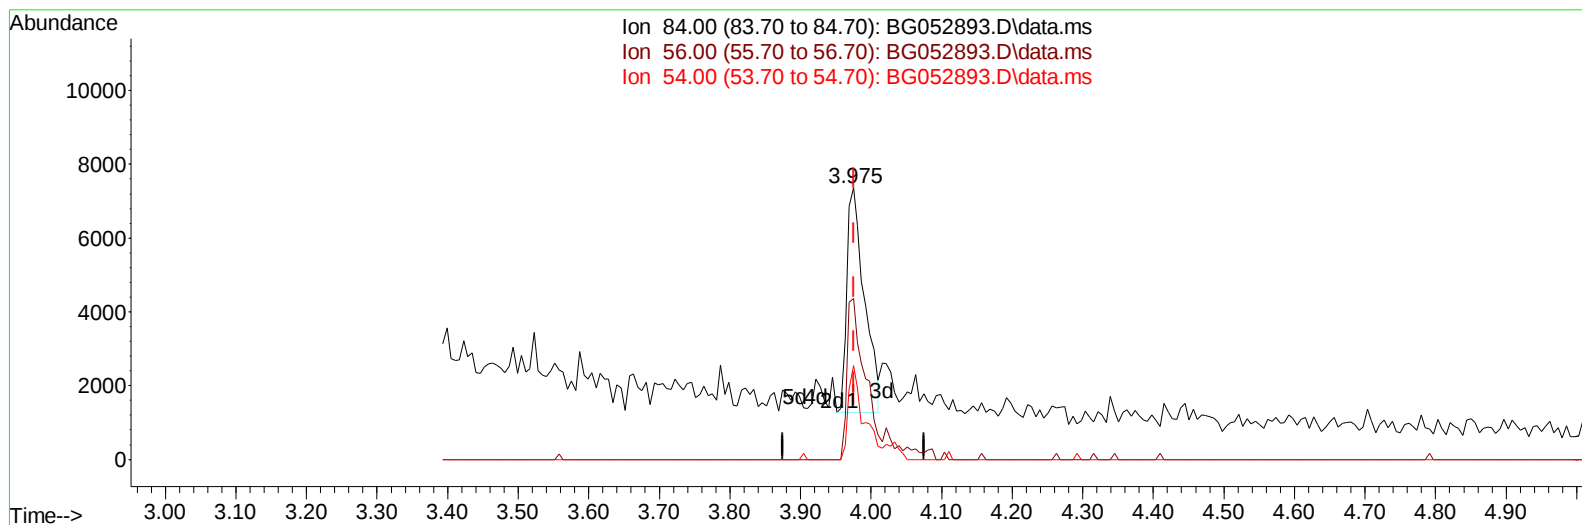

TIC: BG052893.D\data.ms

(4) Pyridine-d5 (S)

3.975min (-0.001) 5.81 ng/u1

response 10569

Ion	Exp%	Act%
84.00	100.00	100.00
56.00	65.20	59.21
54.00	28.70	34.67#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032822\
 Data File : BG052893.D
 Acq On : 28 Mar 2022 16:05
 Operator : CG/JU
 Sample : N2082-16
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 EW615

Manual IntegrationsAPPROVED

Quant Time: Mar 29 01:00:04 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Mar 23 13:16:32 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 03/29/2022
 Supervised By :mohammad ahmed 03/29/2022

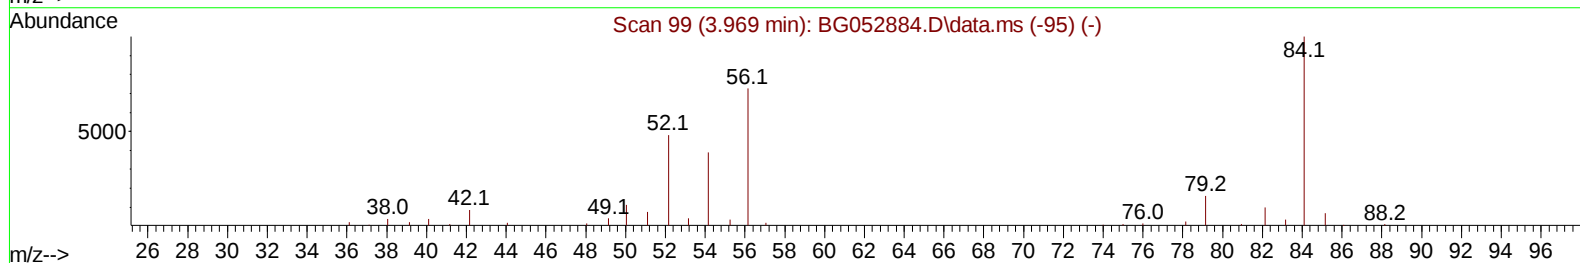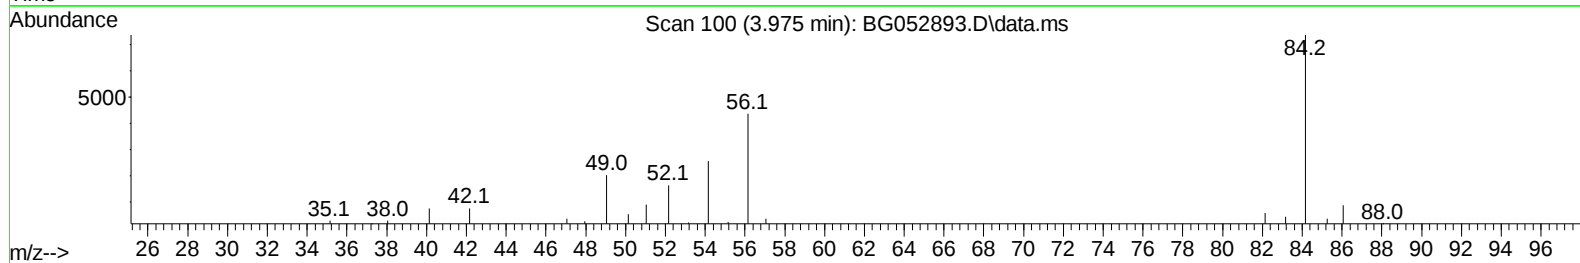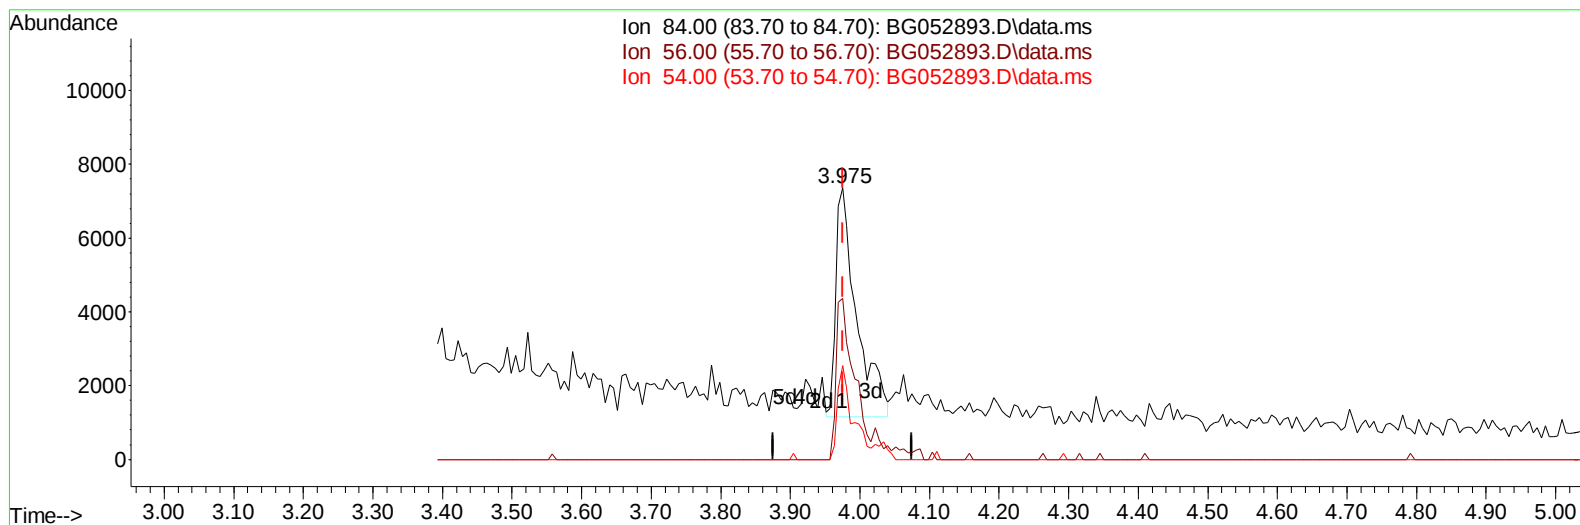

TIC: BG052893.D\data.ms

(4) Pyridine-d5 (S)

3.975min (-0.001) 7.06 ng/ul m

response 12837

Ion	Exp%	Act%
84.00	100.00	100.00
56.00	65.20	59.21
54.00	28.70	34.67#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032822\
 Data File : BG052893.D
 Acq On : 28 Mar 2022 16:05
 Operator : CG/JU
 Sample : N2082-16
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 EW615

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 03/29/2022
 Supervised By :mohammad ahmed 03/29/2022

Quant Time: Mar 29 01:00:04 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Mar 23 13:16:32 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.134	152	25718	20.000	ng/ul	-0.01
20) Naphthalene-d8	10.948	136	119940	20.000	ng/ul	-0.01
38) Acenaphthene-d10	14.754	164	97186	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.498	188	216100	20.000	ng/ul	0.00
79) Chrysene-d12	21.786	240	249231	20.000	ng/ul	# 0.00
88) Perylene-d12	25.099	264	260247	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.546	96	2379	3.267	ng/uL	0.00
4) Pyridine-d5	3.975	84	12837m	7.062	ng/ul	0.00
7) Phenol-d5	7.282	99	16755	7.274	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.452	67	46895	33.334	ng/ul	0.00
11) 2-Chlorophenol-d4	7.664	132	38317	24.498	ng/ul	-0.01
15) 4-Methylphenol-d8	8.833	113	30723	18.413	ng/ul	0.00
21) Nitrobenzene-d5	9.297	128	28371	32.861	ng/ul	0.00
24) 2-Nitrophenol-d4	10.020	143	29627	32.534	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.560	165	56303	28.420	ng/ul	0.00
31) 4-Chloroaniline-d4	11.071	131	72328	27.623	ng/ul	0.00
46) Dimethylphthalate-d6	14.155	166	239198	32.037	ng/ul	0.00
49) Acenaphthylene-d8	14.449	160	276794	30.509	ng/ul	0.00
54) 4-Nitrophenol-d4	14.931	143	8167	6.506	ng/ul	0.00
60) Fluorene-d10	15.747	176	214576	32.731	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.847	200	34148	31.051	ng/ul	-0.01
73) Anthracene-d10	17.598	188	359950	35.770	ng/ul	0.00
81) Pyrene-d10	19.883	212	426204	30.569	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.870	264	488140	36.301	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032822\
Data File : BG052893.D
Acq On : 28 Mar 2022 16:05
Operator : CG/JU
Sample : N2082-16
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
EW615

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 03/29/2022
Supervised By :mohammad ahmed 03/29/2022

Quant Time: Mar 29 01:00:04 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Mar 23 13:16:32 2022
Response via : Initial Calibration

