




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032822\
Data File : BG052894.D
Acq On : 28 Mar 2022 16:44
Operator : CG/JU
Sample : N2082-13
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
EW605

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 03/29/2022
Supervised By :mohammad ahmed 03/29/2022

Quant Time: Mar 29 01:03:29 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Mar 23 13:16:32 2022
Response via : Initial Calibration

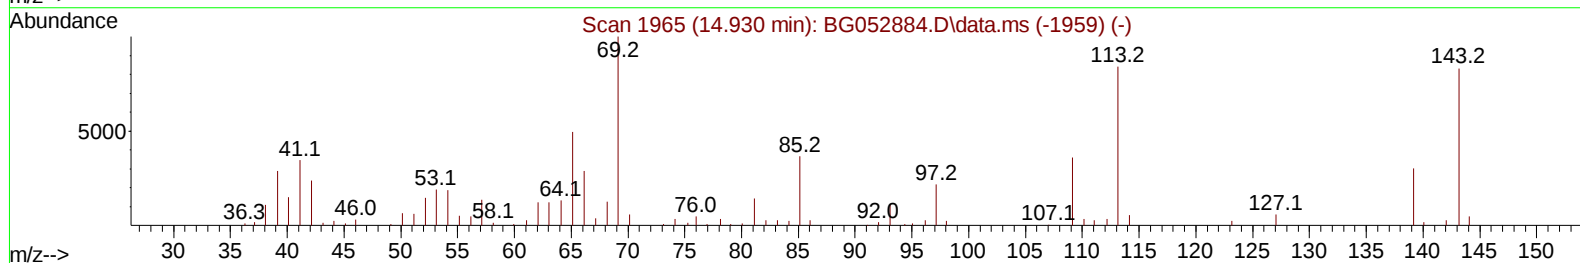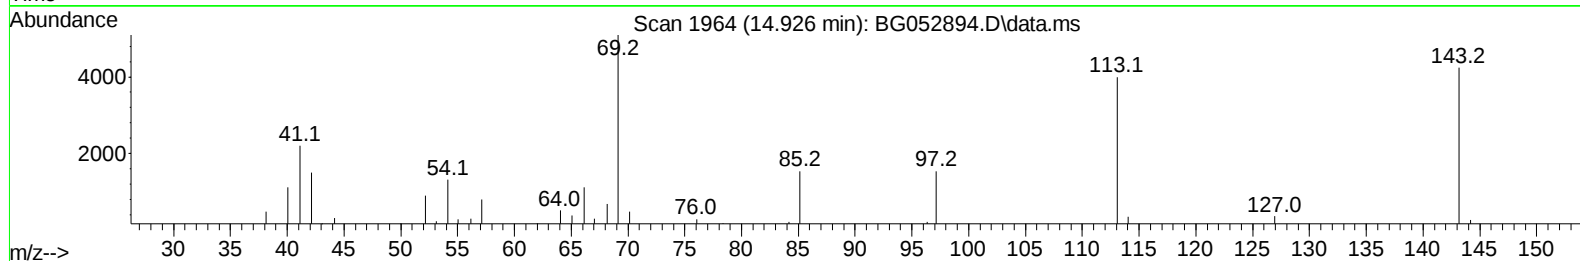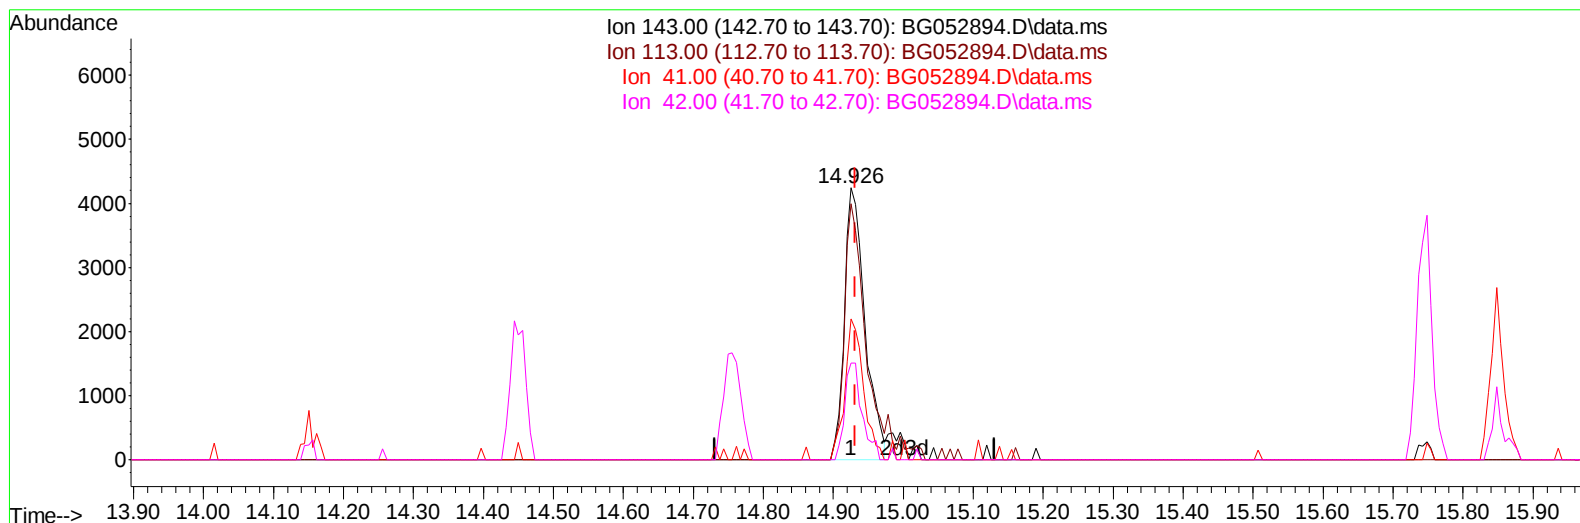

TIC: BG052894.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.926min (-0.005) 7.31 ng/u1

response 8645

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	105.70	94.18
41.00	47.20	51.85
42.00	29.40	35.51#




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032822\
 Data File : BG052894.D
 Acq On : 28 Mar 2022 16:44
 Operator : CG/JU
 Sample : N2082-13
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 EW605

Manual IntegrationsAPPROVED

Quant Time: Mar 29 01:03:29 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Mar 23 13:16:32 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 03/29/2022
 Supervised By :mohammad ahmed 03/29/2022

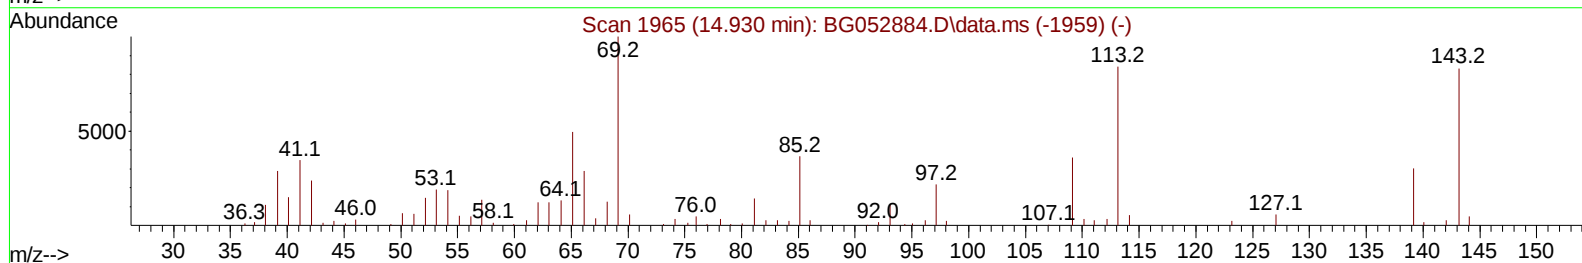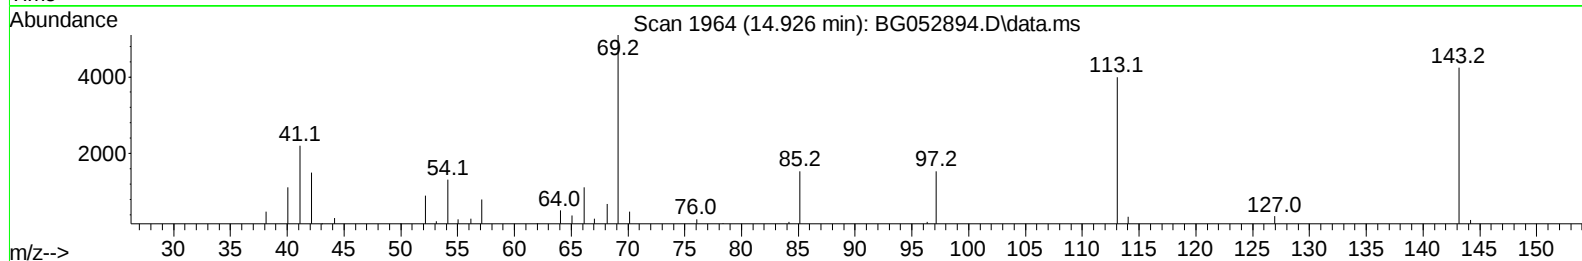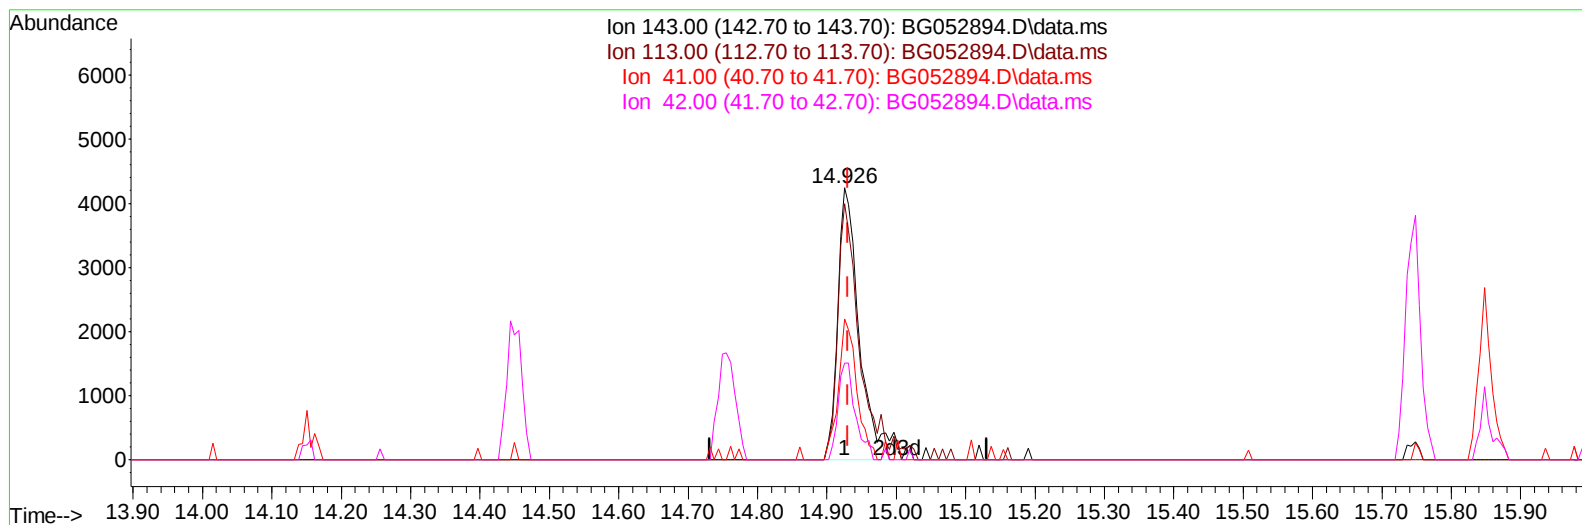

TIC: BG052894.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.926min (-0.005) 7.64 ng/ul m

response 9031

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	105.70	94.18
41.00	47.20	51.85
42.00	29.40	35.51#

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032822\
 Data File : BG052894.D
 Acq On : 28 Mar 2022 16:44
 Operator : CG/JU
 Sample : N2082-13
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 EW605

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 03/29/2022
 Supervised By :mohammad ahmed 03/29/2022

Quant Time: Mar 29 01:03:29 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Mar 23 13:16:32 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.135	152	24757	20.000	ng/ul	-0.01
20) Naphthalene-d8	10.949	136	108478	20.000	ng/ul	-0.01
38) Acenaphthene-d10	14.755	164	91513	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.499	188	226452	20.000	ng/ul	0.00
79) Chrysene-d12	21.787	240	242542	20.000	ng/ul	# 0.00
88) Perylene-d12	25.100	264	236702	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.547	96	2695	3.845	ng/uL	0.00
4) Pyridine-d5	3.970	84	14791	8.453	ng/ul	0.00
7) Phenol-d5	7.283	99	18936	8.540	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.453	67	41547	30.679	ng/ul	0.00
11) 2-Chlorophenol-d4	7.665	132	36595	24.306	ng/ul	-0.01
15) 4-Methylphenol-d8	8.828	113	33052	20.577	ng/ul	0.00
21) Nitrobenzene-d5	9.292	128	24886	31.870	ng/ul	0.00
24) 2-Nitrophenol-d4	10.021	143	27246	33.081	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.561	165	49751	27.766	ng/ul	0.00
31) 4-Chloroaniline-d4	11.072	131	66646	28.143	ng/ul	0.00
46) Dimethylphthalate-d6	14.150	166	220408	31.351	ng/ul	-0.01
49) Acenaphthylene-d8	14.450	160	251611	29.452	ng/ul	0.00
54) 4-Nitrophenol-d4	14.926	143	9031m	7.640	ng/ul	0.00
60) Fluorene-d10	15.748	176	196368	31.810	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.848	200	39848	34.578	ng/ul	-0.01
73) Anthracene-d10	17.598	188	369180	35.010	ng/ul	0.00
81) Pyrene-d10	19.884	212	460300	33.925	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.871	264	443325	36.248	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032822\
Data File : BG052894.D
Acq On : 28 Mar 2022 16:44
Operator : CG/JU
Sample : N2082-13
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
EW605

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 03/29/2022
Supervised By :mohammad ahmed 03/29/2022

Quant Time: Mar 29 01:03:29 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Mar 23 13:16:32 2022
Response via : Initial Calibration

