




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032822\
Data File : BG052907.D
Acq On : 29 Mar 2022 1:43
Operator : CG/JU
Sample : N2100-10
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0AG2

Manual IntegrationsAPPROVED

Quant Time: Mar 29 02:37:59 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Mar 23 13:16:32 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 03/29/2022
Supervised By :mohammad ahmed 03/29/2022

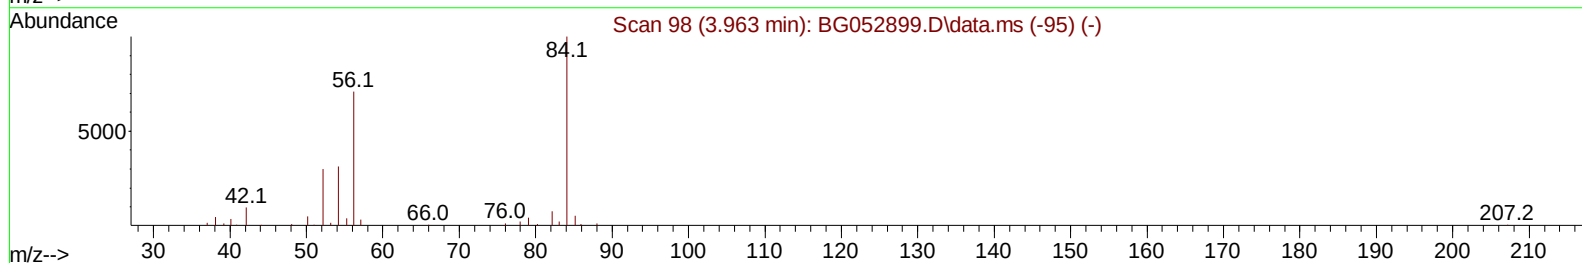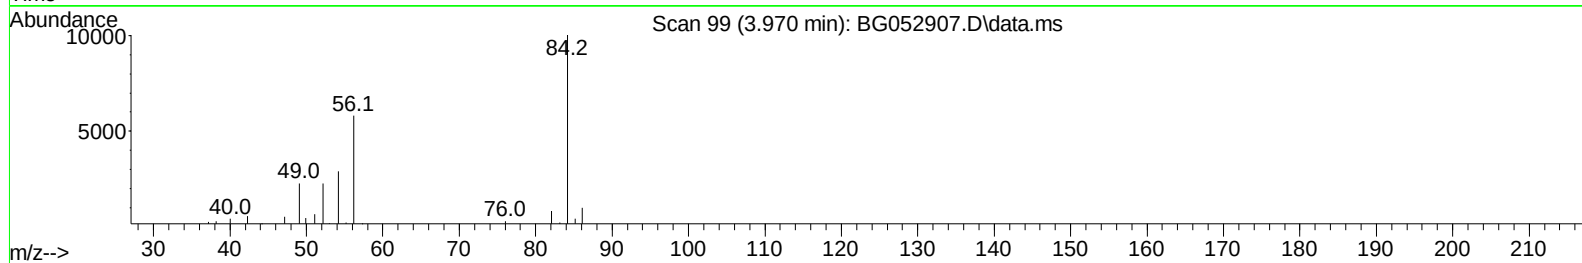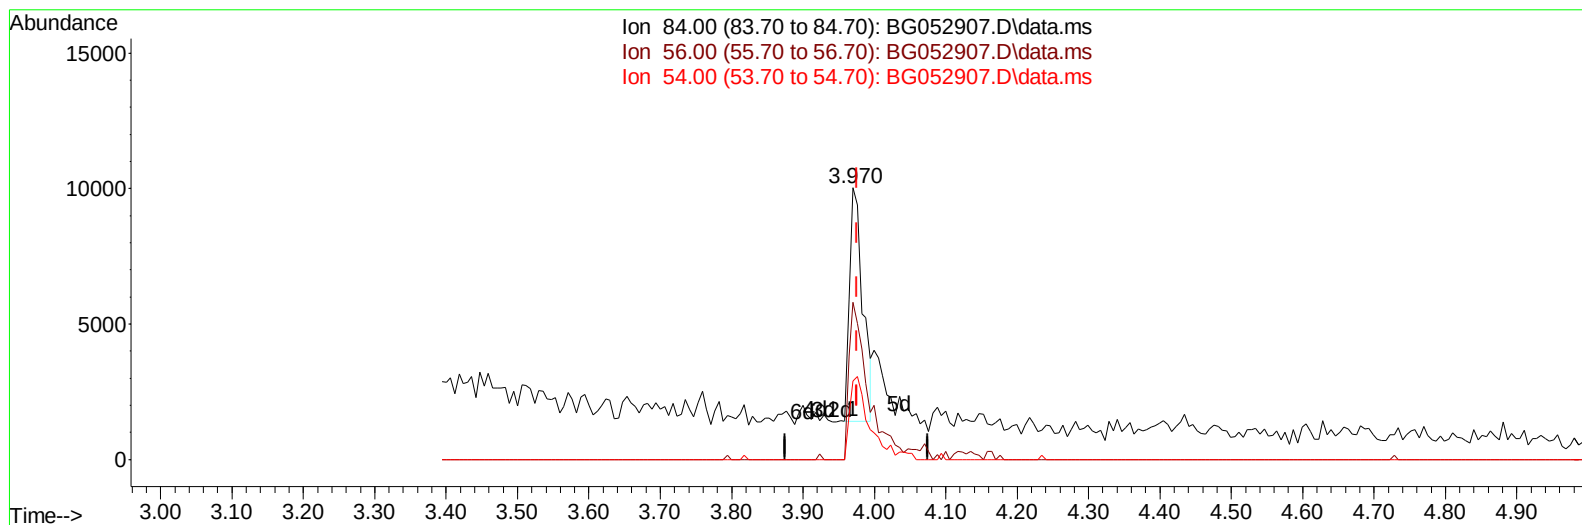

TIC: BG052907.D\data.ms

(4) Pyridine-d5 (S)

3.970min (-0.005) 6.47 ng/u1

response 10999

Ion	Exp%	Act%
84.00	100.00	100.00
56.00	65.20	58.00
54.00	28.70	28.92
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032822\
Data File : BG052907.D
Acq On : 29 Mar 2022 1:43
Operator : CG/JU
Sample : N2100-10
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0AG2

Manual IntegrationsAPPROVED

Quant Time: Mar 29 02:37:59 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Mar 23 13:16:32 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 03/29/2022
Supervised By :mohammad ahmed 03/29/2022

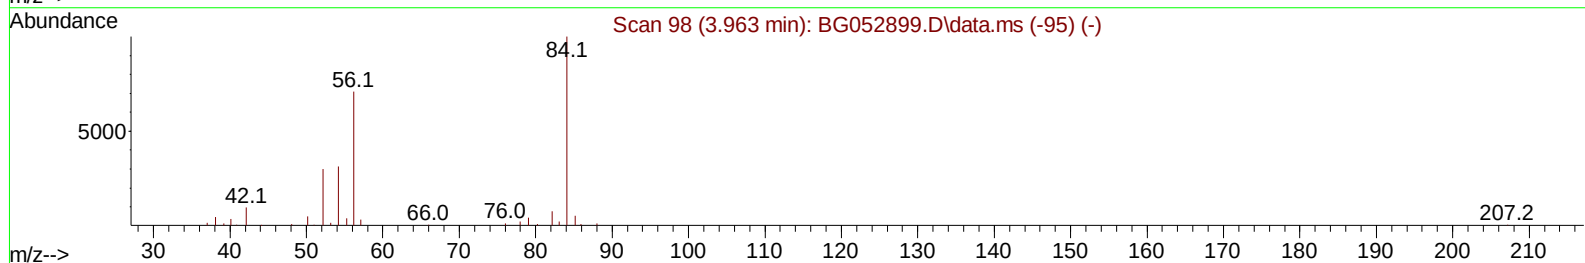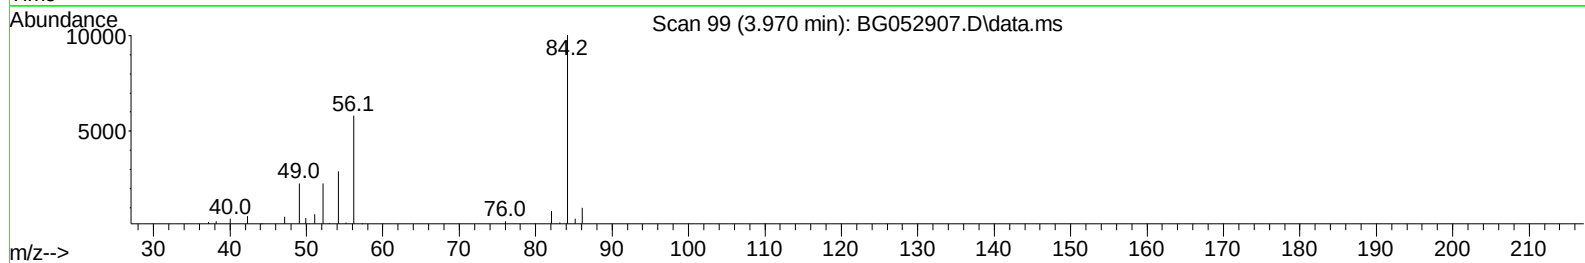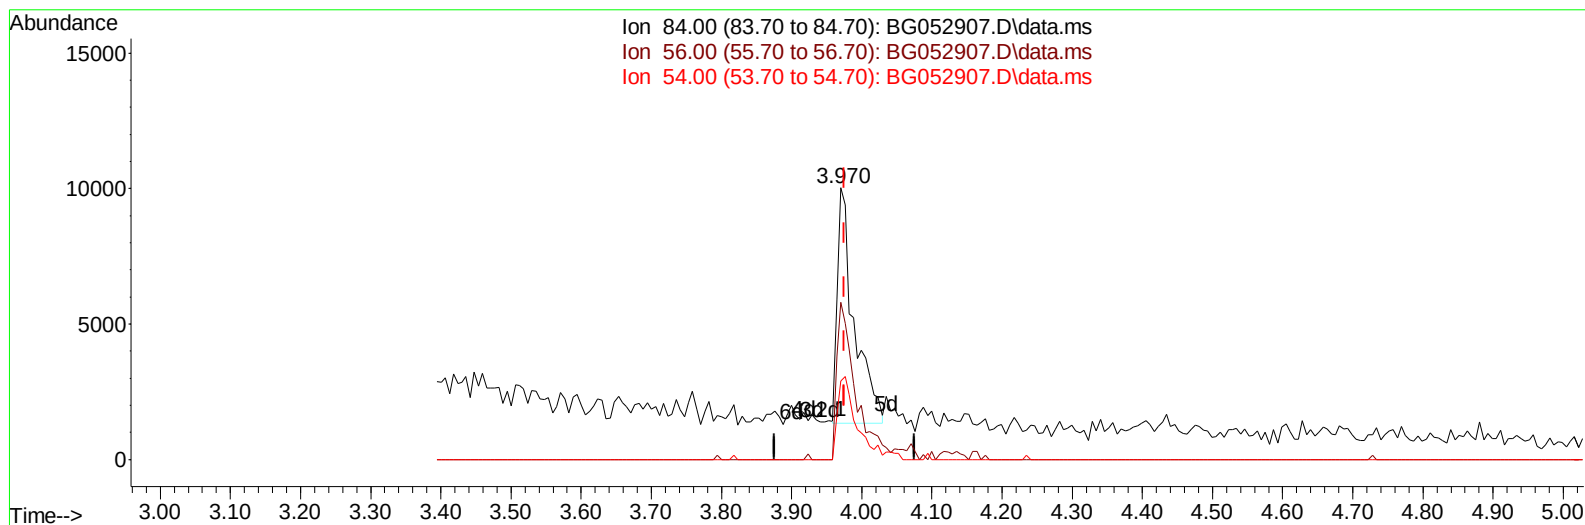

TIC: BG052907.D\data.ms

(4) Pyridine-d5 (S)

3.970min (-0.005) 8.46 ng/ul m

response 14378

Ion	Exp%	Act%
84.00	100.00	100.00
56.00	65.20	58.00
54.00	28.70	28.92
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032822\
 Data File : BG052907.D
 Acq On : 29 Mar 2022 1:43
 Operator : CG/JU
 Sample : N2100-10
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0AG2

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 03/29/2022
 Supervised By :mohammad ahmed 03/29/2022

Quant Time: Mar 29 02:37:59 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Mar 23 13:16:32 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.135	152	24056	20.000	ng/ul	-0.01
20) Naphthalene-d8	10.949	136	113289	20.000	ng/ul	-0.01
38) Acenaphthene-d10	14.756	164	95005	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.499	188	233604	20.000	ng/ul	0.00
79) Chrysene-d12	21.782	240	257725	20.000	ng/ul	#-0.01
88) Perylene-d12	25.095	264	258044	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.547	96	2823	4.145	ng/uL	0.00
4) Pyridine-d5	3.970	84	14378m	8.457	ng/ul	0.00
7) Phenol-d5	7.284	99	16697	7.750	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.454	67	47469	36.073	ng/ul	0.00
11) 2-Chlorophenol-d4	7.665	132	38064	26.018	ng/ul	-0.01
15) 4-Methylphenol-d8	8.828	113	29878	19.143	ng/ul	0.00
21) Nitrobenzene-d5	9.293	128	29165	35.763	ng/ul	0.00
24) 2-Nitrophenol-d4	10.021	143	32426	37.698	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.561	165	54732	29.249	ng/ul	0.00
31) 4-Chloroaniline-d4	11.073	131	68525	27.707	ng/ul	0.00
46) Dimethylphthalate-d6	14.151	166	244318	33.474	ng/ul	-0.01
49) Acenaphthylene-d8	14.450	160	272417	30.716	ng/ul	0.00
54) 4-Nitrophenol-d4	14.926	143	7733	6.302	ng/ul	0.00
60) Fluorene-d10	15.743	176	221051	34.493	ng/ul	-0.01
65) 4,6-Dinitro-2-methylph...	15.848	200	38671	32.529	ng/ul	-0.01
73) Anthracene-d10	17.599	188	392873	36.116	ng/ul	0.00
81) Pyrene-d10	19.878	212	480596	33.334	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.866	264	490541	36.791	ng/ul	-0.01

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032822\
Data File : BG052907.D
Acq On : 29 Mar 2022 1:43
Operator : CG/JU
Sample : N2100-10
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0AG2

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 03/29/2022
Supervised By :mohammad ahmed 03/29/2022

Quant Time: Mar 29 02:37:59 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Mar 23 13:16:32 2022
Response via : Initial Calibration

