




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032822\
Data File : BG052911.D
Acq On : 29 Mar 2022 4:16
Operator : CG/JU
Sample : N2097-08
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0AD7

Manual IntegrationsAPPROVED

Quant Time: Mar 29 05:02:34 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Mar 23 13:16:32 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 03/29/2022
Supervised By :mohammad ahmed 03/29/2022

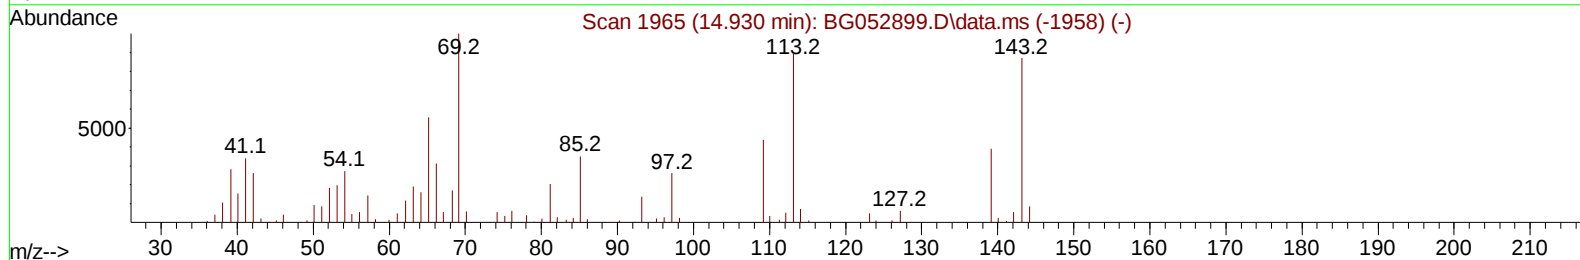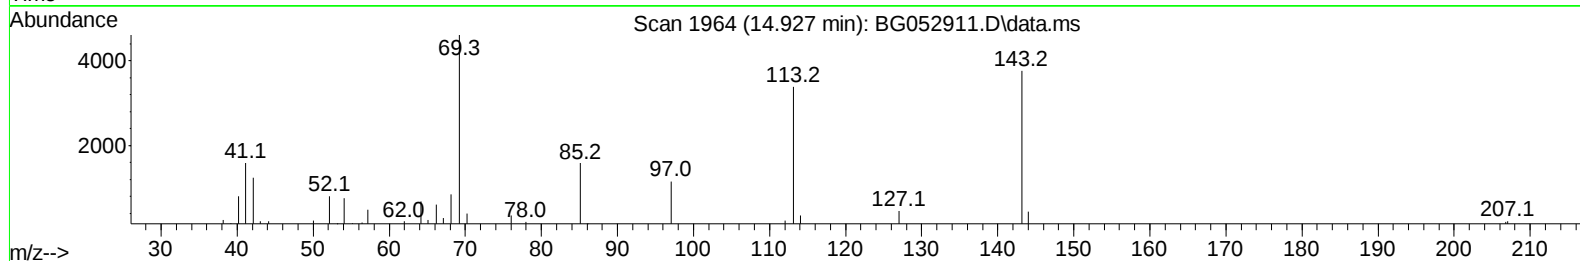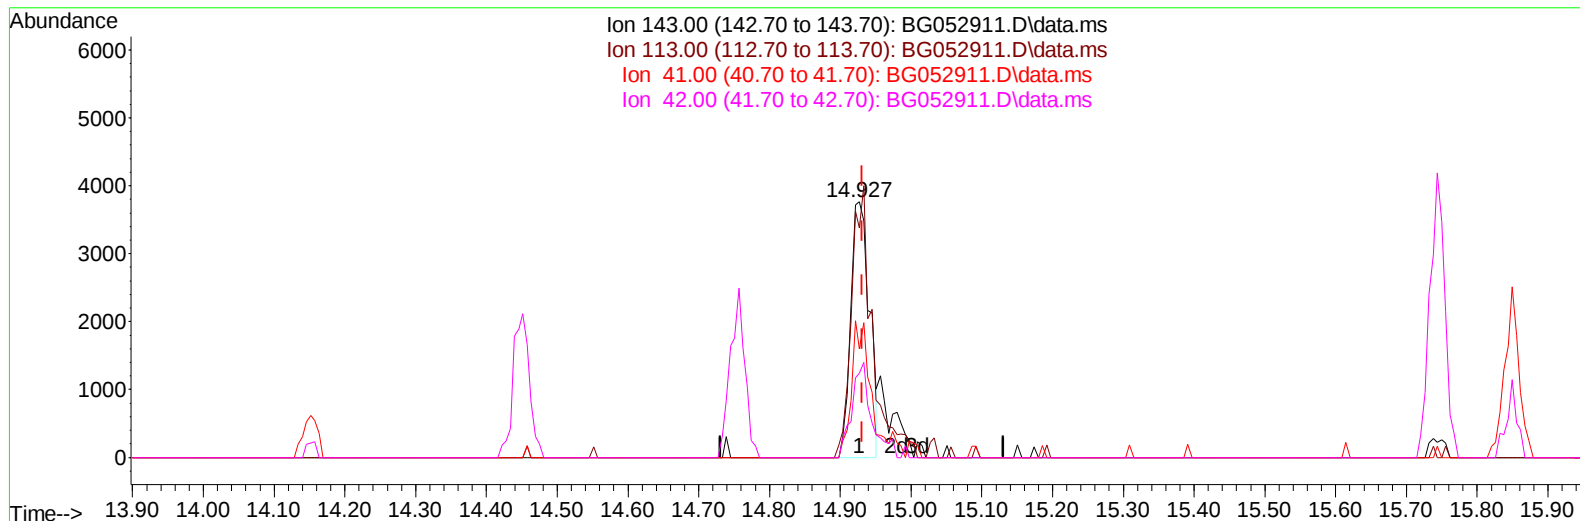

TIC: BG052911.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.927min (-0.004) 4.91 ng/u1

response 6958

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	105.70	89.73
41.00	47.20	42.31
42.00	29.40	33.02

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032822\
 Data File : BG052911.D
 Acq On : 29 Mar 2022 4:16
 Operator : CG/JU
 Sample : N2097-08
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0AD7

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 03/29/2022
 Supervised By :mohammad ahmed 03/29/2022

Quant Time: Mar 29 05:02:34 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Mar 23 13:16:32 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.136	152	29419	20.000	ng/ul	0.00
20) Naphthalene-d8	10.950	136	131819	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.757	164	109739	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.500	188	268664	20.000	ng/ul	0.00
79) Chrysene-d12	21.783	240	283472	20.000	ng/ul	# 0.00
88) Perylene-d12	25.096	264	274598	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.554	96	2555	3.068	ng/uL	0.00
4) Pyridine-d5	0.000	84	0d	0.000	ng/ul	
7) Phenol-d5	7.279	99	16965	6.439	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.449	67	47006	29.209	ng/ul	0.00
11) 2-Chlorophenol-d4	7.666	132	39356	21.997	ng/ul	0.00
15) 4-Methylphenol-d8	8.824	113	29880	15.655	ng/ul	0.00
21) Nitrobenzene-d5	9.288	128	28128	29.643	ng/ul	0.00
24) 2-Nitrophenol-d4	10.022	143	30683	30.657	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.557	165	55445	25.465	ng/ul	0.00
31) 4-Chloroaniline-d4	11.074	131	48119	16.721	ng/ul	0.00
46) Dimethylphthalate-d6	14.152	166	255055	30.253	ng/ul	0.00
49) Acenaphthylene-d8	14.451	160	278824	27.217	ng/ul	0.00
54) 4-Nitrophenol-d4	14.927	143	8645m	6.099	ng/ul	0.00
60) Fluorene-d10	15.744	176	229060	30.944	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.849	200	43732	31.986	ng/ul	0.00
73) Anthracene-d10	17.594	188	426344	34.079	ng/ul	0.00
81) Pyrene-d10	19.879	212	515882	32.531	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.867	264	502597	35.423	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032822\
Data File : BG052911.D
Acq On : 29 Mar 2022 4:16
Operator : CG/JU
Sample : N2097-08
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0AD7

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 03/29/2022
Supervised By :mohammad ahmed 03/29/2022

Quant Time: Mar 29 05:02:34 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Mar 23 13:16:32 2022
Response via : Initial Calibration

