




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032822\
Data File : BG052922.D
Acq On : 29 Mar 2022 11:57
Operator : CG/JU
Sample : N2097-07
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0AD6

Manual IntegrationsAPPROVED

Quant Time: Mar 30 01:08:41 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Mar 23 13:16:32 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 03/30/2022
Supervised By :Yogesh Patel 04/02/2022

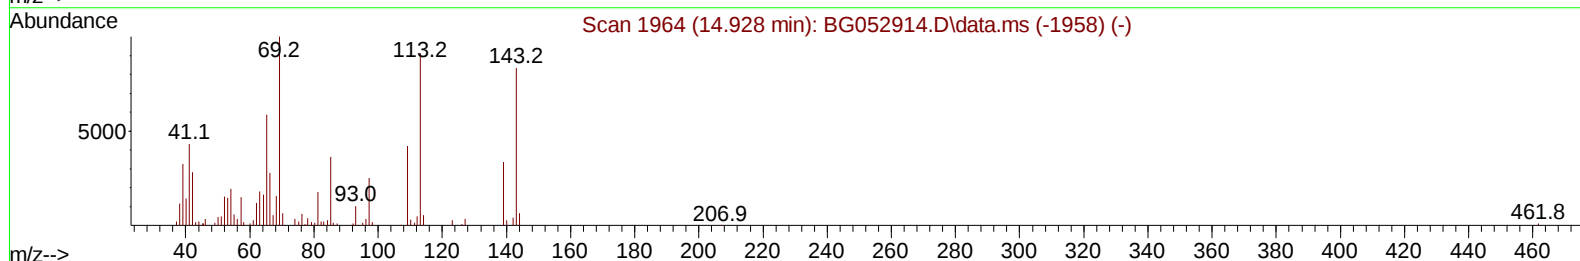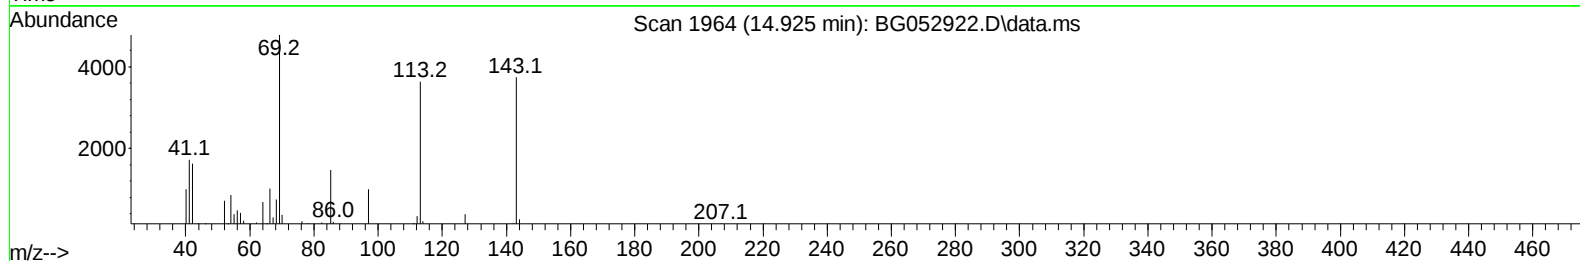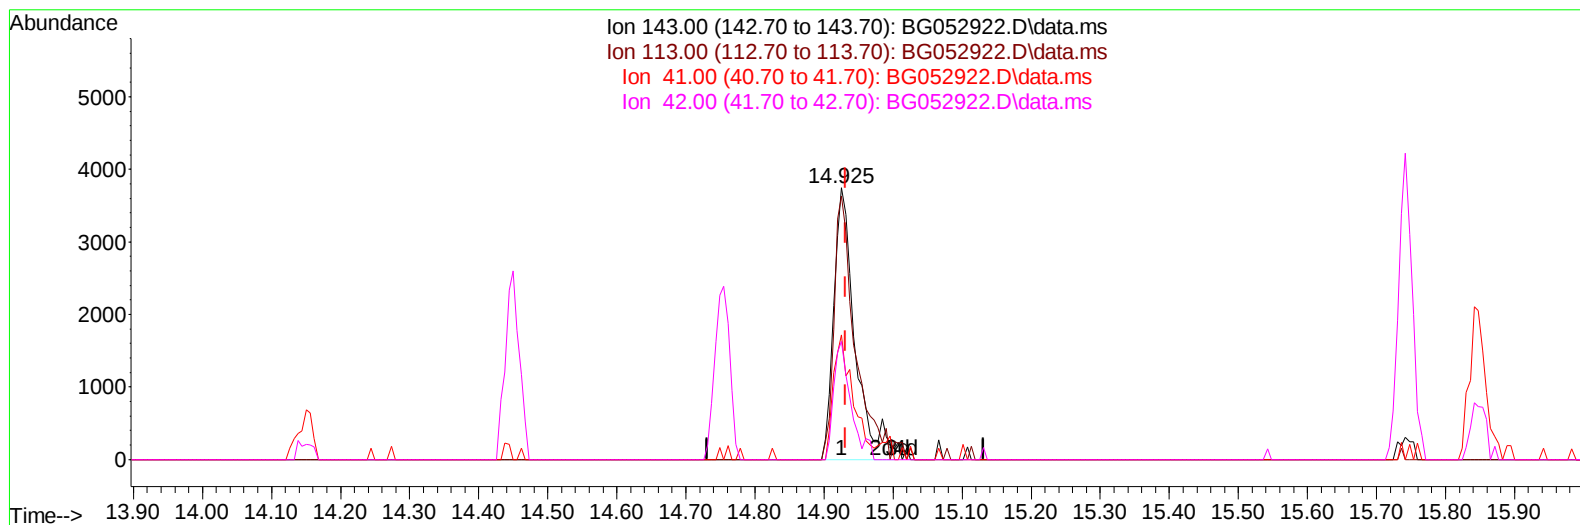

TIC: BG052922.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.925min (-0.006) 6.43 ng/ul m

response 8002

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	105.70	97.06
41.00	47.20	45.85
42.00	29.40	43.52#

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032822\
 Data File : BG052922.D
 Acq On : 29 Mar 2022 11:57
 Operator : CG/JU
 Sample : N2097-07
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0AD6

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 03/30/2022
 Supervised By :Yogesh Patel 04/02/2022

Quant Time: Mar 30 01:08:41 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Mar 23 13:16:32 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.140	152	25967	20.000	ng/ul	0.00
20) Naphthalene-d8	10.948	136	118350	20.000	ng/ul	-0.01
38) Acenaphthene-d10	14.755	164	96280	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.498	188	240942	20.000	ng/ul	0.00
79) Chrysene-d12	21.781	240	260163	20.000	ng/ul	-0.01
88) Perylene-d12	25.094	264	258352	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.547	96	2653	3.609	ng/uL	0.00
4) Pyridine-d5	3.970	84	13289	7.241	ng/ul	0.00
7) Phenol-d5	7.277	99	16948	7.287	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.447	67	45801	32.244	ng/ul	-0.01
11) 2-Chlorophenol-d4	7.665	132	38643	24.470	ng/ul	-0.01
15) 4-Methylphenol-d8	8.828	113	30211	17.932	ng/ul	0.00
21) Nitrobenzene-d5	9.292	128	26861	31.530	ng/ul	0.00
24) 2-Nitrophenol-d4	10.020	143	29018	32.293	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.561	165	52677	26.947	ng/ul	0.00
31) 4-Chloroaniline-d4	11.072	131	71482	27.667	ng/ul	0.00
46) Dimethylphthalate-d6	14.150	166	239820	32.423	ng/ul	-0.01
49) Acenaphthylene-d8	14.450	160	265553	29.545	ng/ul	0.00
54) 4-Nitrophenol-d4	14.925	143	8002m	6.434	ng/ul	0.00
60) Fluorene-d10	15.742	176	216584	33.348	ng/ul	-0.01
65) 4,6-Dinitro-2-methylph...	15.848	200	38761	31.612	ng/ul	-0.01
73) Anthracene-d10	17.598	188	383687	34.198	ng/ul	0.00
81) Pyrene-d10	19.878	212	480172	32.992	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.865	264	476042	35.661	ng/ul	-0.01

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032822\
Data File : BG052922.D
Acq On : 29 Mar 2022 11:57
Operator : CG/JU
Sample : N2097-07
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0AD6

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 03/30/2022
Supervised By :Yogesh Patel 04/02/2022

Quant Time: Mar 30 01:08:41 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Mar 23 13:16:32 2022
Response via : Initial Calibration

