




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032822\
Data File : BG052938.D
Acq On : 29 Mar 2022 22:13
Operator : CG/JU
Sample : N2097-14
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0AE3

Manual IntegrationsAPPROVED

Quant Time: Mar 30 01:11:29 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Mar 23 13:16:32 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 03/30/2022
Supervised By :Yogesh Patel 04/02/2022

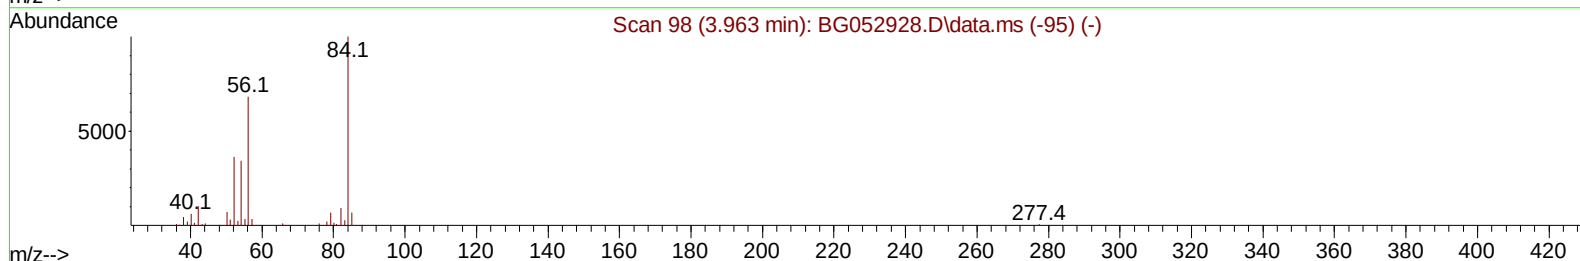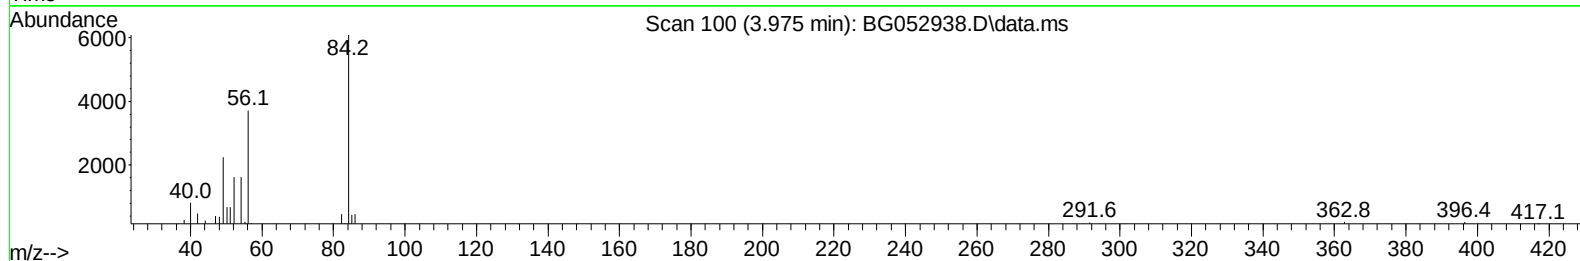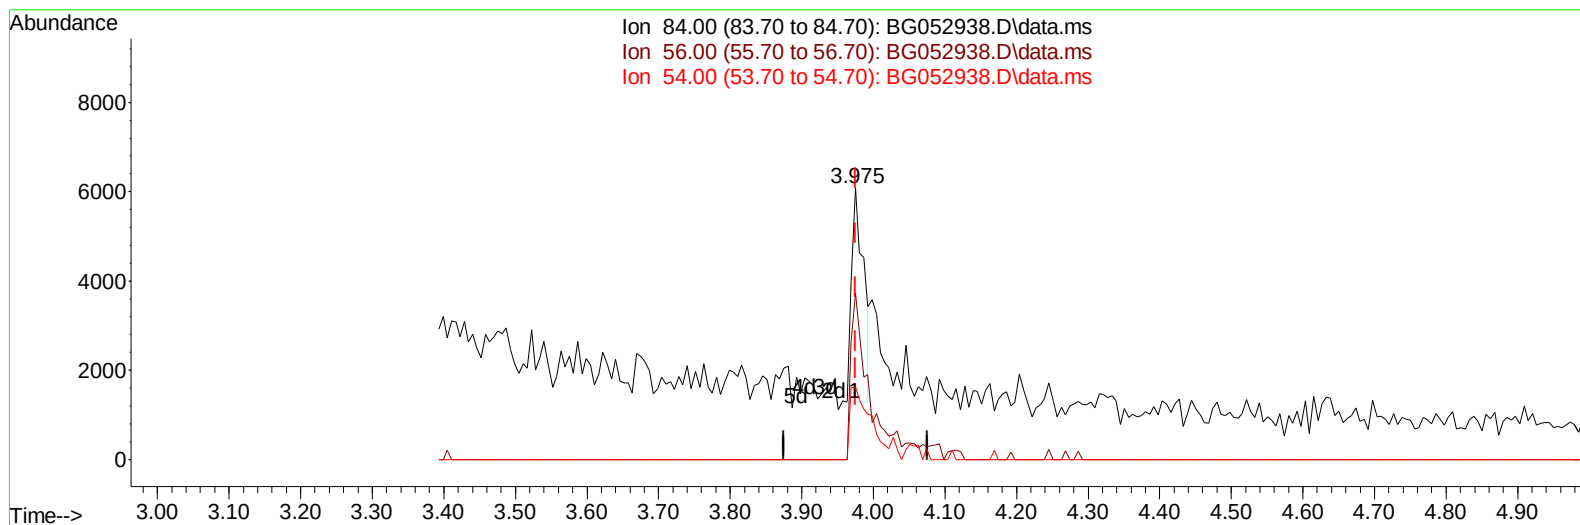

TIC: BG052938.D\data.ms

(4) Pyridine-d5 (S)

3.975min (-0.001) 3.29 ng/uI

response	5709	
Ion	Exp%	Act%
84.00	100.00	100.00
56.00	65.20	61.13
54.00	28.70	26.81
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032822\
Data File : BG052938.D
Acq On : 29 Mar 2022 22:13
Operator : CG/JU
Sample : N2097-14
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0AE3

Manual IntegrationsAPPROVED

Quant Time: Mar 30 01:11:29 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Mar 23 13:16:32 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 03/30/2022
Supervised By :Yogesh Patel 04/02/2022

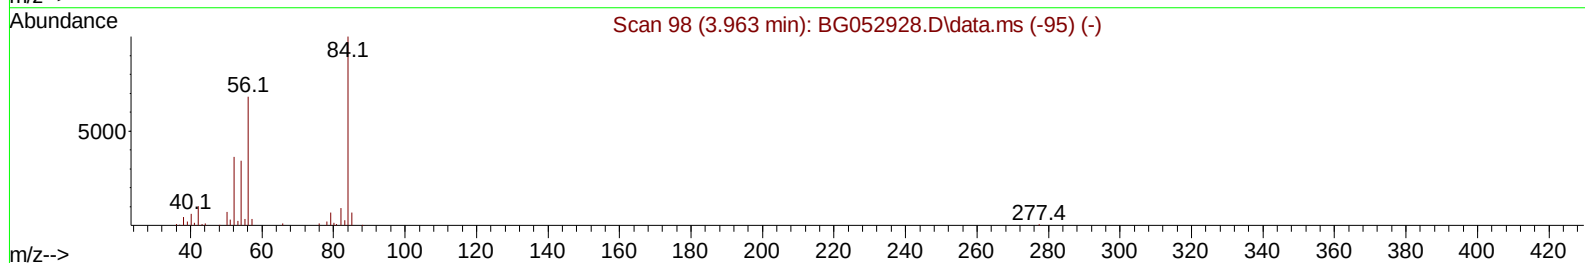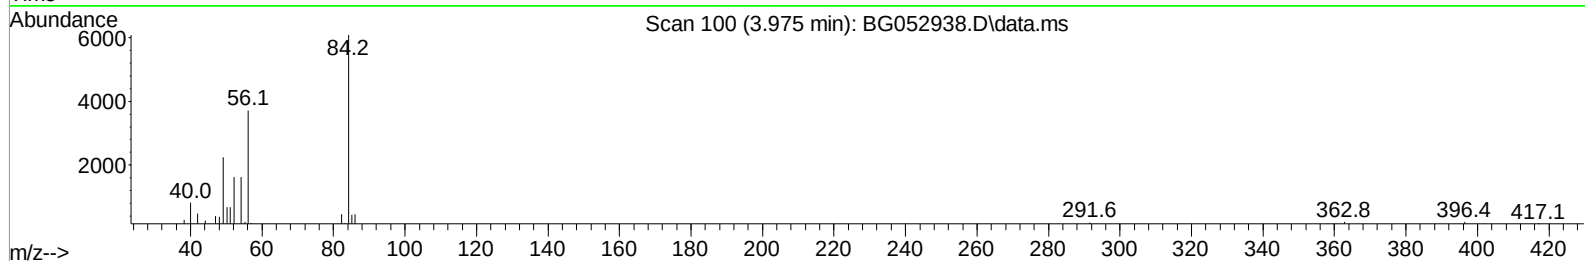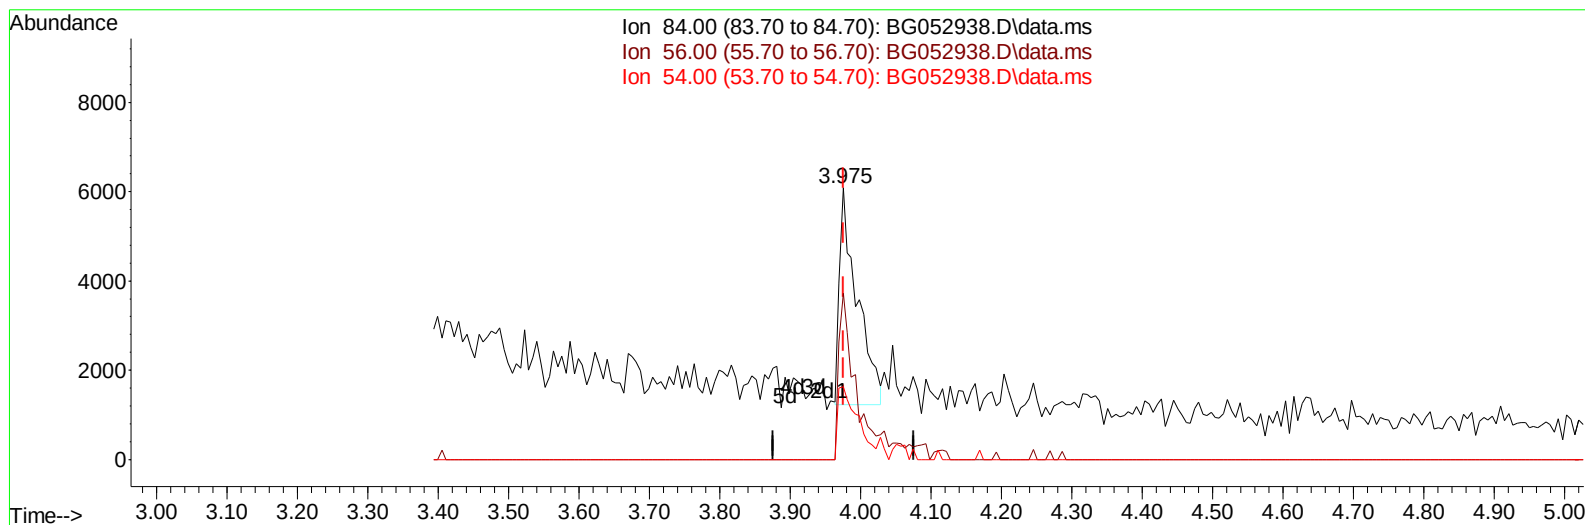

TIC: BG052938.D\data.ms

(4) Pyridine-d5 (S)

3.975min (-0.001) 4.91 ng/ul m

response 8515

Ion	Exp%	Act%
84.00	100.00	100.00
56.00	65.20	61.13
54.00	28.70	26.81
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032822\
 Data File : BG052938.D
 Acq On : 29 Mar 2022 22:13
 Operator : CG/JU
 Sample : N2097-14
 Misc :
 ALS Vial : 57 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0AE3

Manual IntegrationsAPPROVED

Quant Time: Mar 30 01:11:29 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Mar 23 13:16:32 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 03/30/2022
 Supervised By :Yogesh Patel 04/02/2022

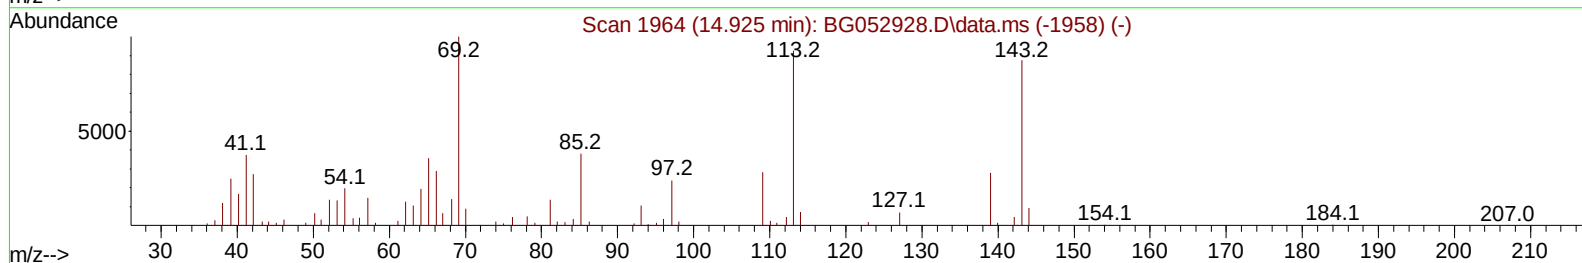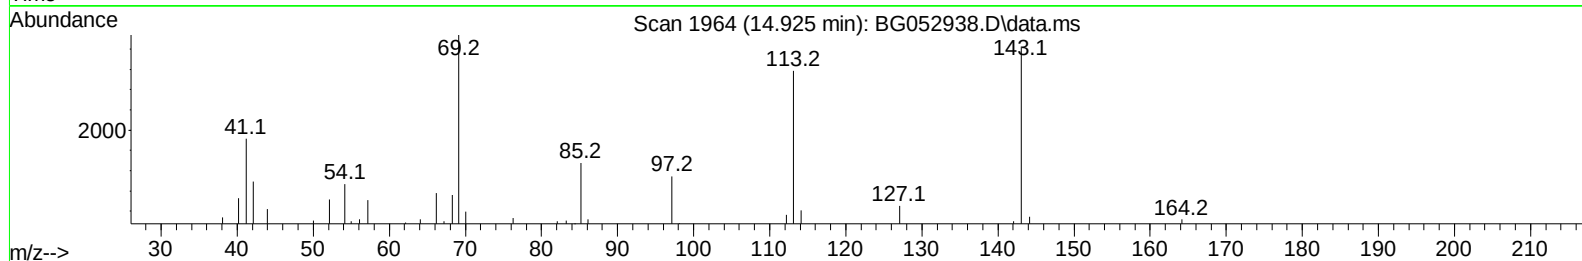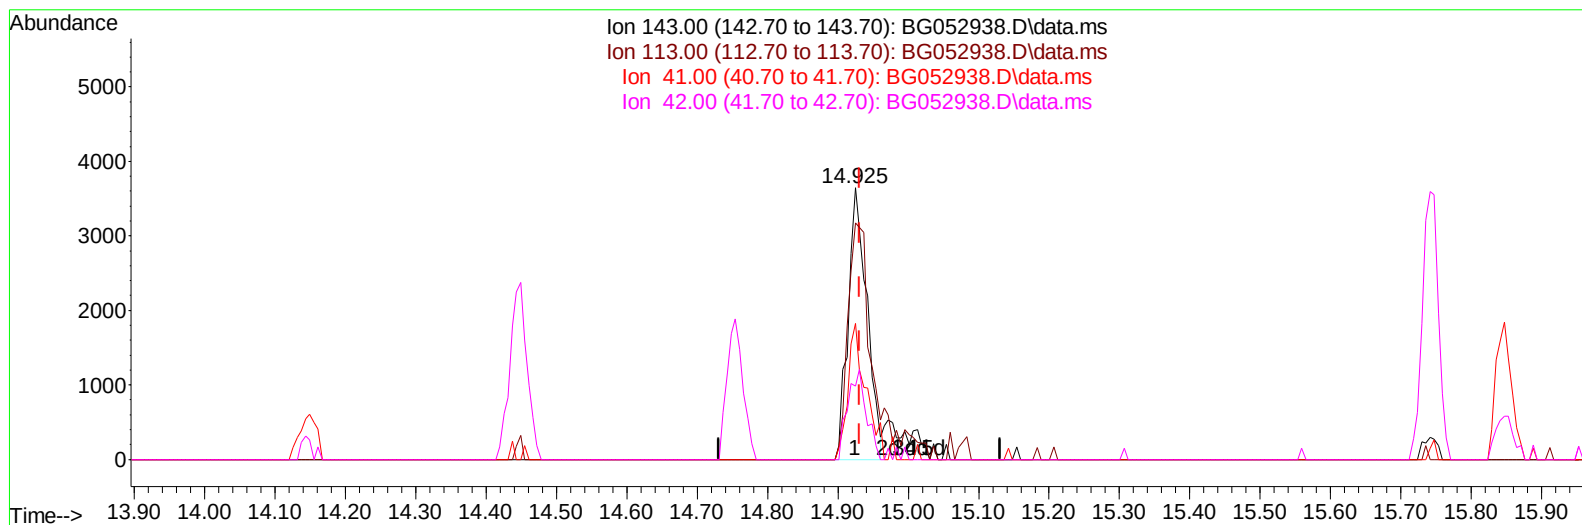

TIC: BG052938.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.925min (-0.006) 5.68 ng/ul

response 6720

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	105.70	87.10
41.00	47.20	50.12
42.00	29.40	27.12




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032822\
Data File : BG052938.D
Acq On : 29 Mar 2022 22:13
Operator : CG/JU
Sample : N2097-14
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0AE3

Manual IntegrationsAPPROVED

Quant Time: Mar 30 01:11:29 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Mar 23 13:16:32 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 03/30/2022
Supervised By :Yogesh Patel 04/02/2022

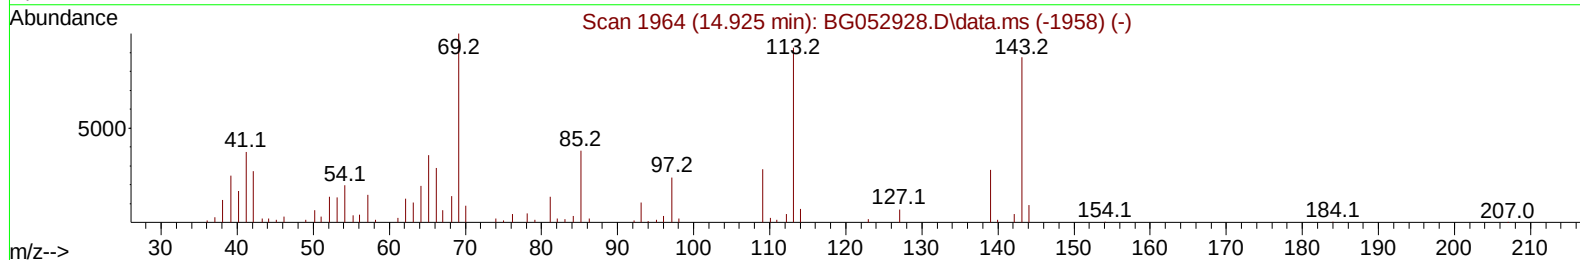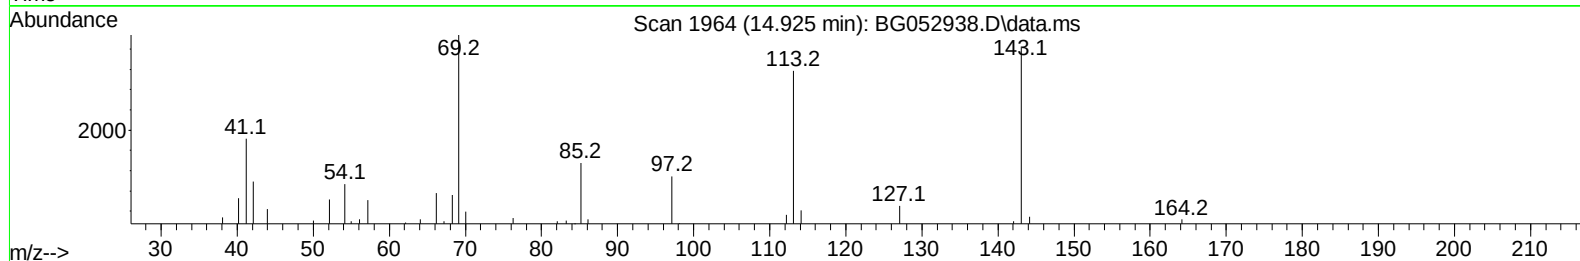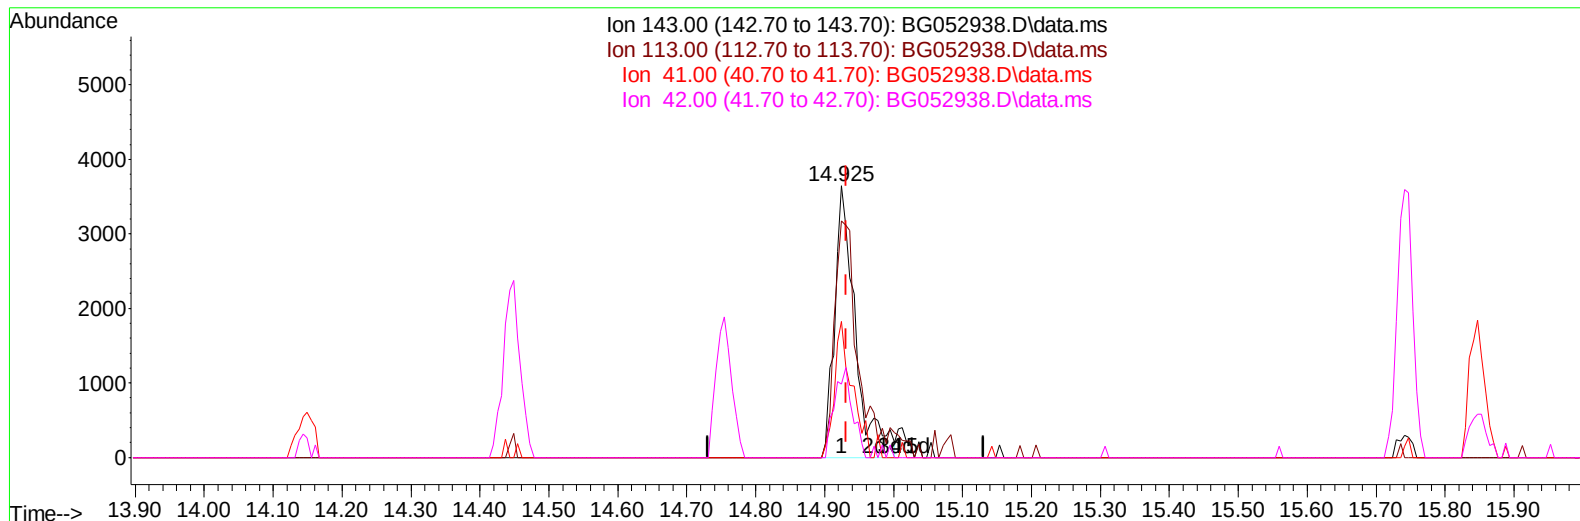

TIC: BG052938.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.925min (-0.006) 6.47 ng/ul m

response 7651

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	105.70	87.10
41.00	47.20	50.12
42.00	29.40	27.12

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032822\
 Data File : BG052938.D
 Acq On : 29 Mar 2022 22:13
 Operator : CG/JU
 Sample : N2097-14
 Misc :
 ALS Vial : 57 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0AE3

Manual IntegrationsAPPROVED

Quant Time: Mar 30 01:11:29 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Mar 23 13:16:32 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 03/30/2022
 Supervised By :Yogesh Patel 04/02/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.134	152	24539	20.000	ng/ul	-0.01
20) Naphthalene-d8	10.948	136	108383	20.000	ng/ul	-0.01
38) Acenaphthene-d10	14.754	164	91598	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.498	188	215610	20.000	ng/ul	0.00
79) Chrysene-d12	21.780	240	241602	20.000	ng/ul	-0.01
88) Perylene-d12	25.087	264	237234	20.000	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.546	96	2961	4.262	ng/uL	0.00
4) Pyridine-d5	3.975	84	8515m	4.910	ng/ul	0.00
7) Phenol-d5	7.276	99	17035	7.751	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.447	67	47683	35.522	ng/ul	-0.01
11) 2-Chlorophenol-d4	7.664	132	40165	26.914	ng/ul	-0.01
15) 4-Methylphenol-d8	8.827	113	32265	20.266	ng/ul	0.00
21) Nitrobenzene-d5	9.291	128	29970	38.414	ng/ul	0.00
24) 2-Nitrophenol-d4	10.014	143	31612	38.415	ng/ul	-0.01
28) 2,4-Dichlorophenol-d3	10.554	165	55608	31.062	ng/ul	-0.01
31) 4-Chloroaniline-d4	11.071	131	69388	29.326	ng/ul	0.00
46) Dimethylphthalate-d6	14.149	166	246521	35.032	ng/ul	-0.01
49) Acenaphthylene-d8	14.449	160	272461	31.863	ng/ul	0.00
54) 4-Nitrophenol-d4	14.925	143	7651m	6.467	ng/ul	0.00
60) Fluorene-d10	15.741	176	218465	35.357	ng/ul	-0.01
65) 4,6-Dinitro-2-methylph...	15.847	200	36695	33.443	ng/ul	-0.01
73) Anthracene-d10	17.598	188	375283	37.378	ng/ul	0.00
81) Pyrene-d10	19.877	212	469601	34.745	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.864	264	467037	38.101	ng/ul	-0.01

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032822\
Data File : BG052938.D
Acq On : 29 Mar 2022 22:13
Operator : CG/JU
Sample : N2097-14
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0AE3

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 03/30/2022
Supervised By :Yogesh Patel 04/02/2022

Quant Time: Mar 30 01:11:29 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Mar 23 13:16:32 2022
Response via : Initial Calibration

