

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032822\
 Data File : BG052893.D
 Acq On : 28 Mar 2022 16:05
 Operator : CG/JU
 Sample : N2082-16
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 EW615

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
 Title : SVOA CALIBRATION

Signal : TIC: BG052893.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.558	25	29	32	rVB6	5626	8276	0.66%	0.083%
2	3.787	66	68	71	rVB	3774	3299	0.26%	0.033%
3	3.816	71	73	78	rBV4	1874	3204	0.26%	0.032%
4	3.975	96	100	107	rBV2	18275	32025	2.56%	0.320%
5	4.092	118	120	121	rVB2	2348	1454	0.12%	0.015%
6	4.151	128	130	132	rBV3	1759	1513	0.12%	0.015%
7	4.304	154	156	161	rBV5	2029	2743	0.22%	0.027%
8	4.368	164	167	172	rVB4	2198	2484	0.20%	0.025%
9	4.445	179	180	183	rBV2	1951	1744	0.14%	0.017%
10	4.697	221	223	228	rVB5	1263	1619	0.13%	0.016%
11	5.097	290	291	295	rVB3	1305	1478	0.12%	0.015%
12	5.485	354	357	360	rBV2	1407	2154	0.17%	0.022%
13	5.614	378	379	382	rVB	1829	1347	0.11%	0.013%
14	5.949	432	436	439	rVB3	974	1570	0.13%	0.016%
15	6.148	465	470	473	rVV4	1486	1809	0.14%	0.018%
16	6.753	571	573	577	rBV3	1345	2077	0.17%	0.021%
17	7.206	647	650	653	rBV3	1115	1554	0.12%	0.016%
18	7.282	657	663	670	rVB	32744	57898	4.62%	0.578%
19	7.452	685	692	700	rBV	89811	156667	12.51%	1.564%
20	7.664	722	728	737	rVB	91537	157835	12.61%	1.576%
21	7.758	741	744	745	rBV3	1204	1513	0.12%	0.015%
22	8.081	794	799	801	rBV3	985	1459	0.12%	0.015%
23	8.134	802	808	817	rVB	92935	165967	13.25%	1.657%
24	8.833	919	927	934	rBV	82294	148102	11.83%	1.479%
25	9.291	998	1005	1015	rVB	123853	231212	18.47%	2.309%
26	9.409	1021	1025	1026	rBV2	1470	1640	0.13%	0.016%
27	9.420	1026	1027	1030	rVV3	1625	1413	0.11%	0.014%
28	9.456	1030	1033	1037	rVB4	2220	3065	0.24%	0.031%
29	9.585	1054	1055	1060	rVB3	1210	1382	0.11%	0.014%
30	9.785	1086	1089	1092	rVB2	987	1421	0.11%	0.014%
31	10.020	1122	1129	1140	rVV	105833	186563	14.90%	1.863%
32	10.560	1214	1221	1229	rBV2	156761	276102	22.05%	2.757%
33	10.948	1280	1287	1295	rBV	147238	265963	21.24%	2.656%
34	11.071	1300	1308	1317	rBV2	138464	263487	21.04%	2.631%
35	12.522	1552	1555	1559	rVB2	2795	3542	0.28%	0.035%
36	14.149	1825	1832	1840	rBV	357062	535100	42.74%	5.343%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032822\
 Data File : BG052893.D
 Acq On : 28 Mar 2022 16:05
 Operator : CG/JU
 Sample : N2082-16
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 EW615

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
 Title : SVOA CALIBRATION

37	14.449	1876	1883	1891	rVV	386015	609122	48.65%	6.082%
38	14.754	1928	1935	1943	rBV	271532	435211	34.76%	4.346%
39	14.925	1958	1964	1972	rBV4	28121	56396	4.50%	0.563%
40	14.983	1972	1974	1979	rVB4	2742	3950	0.32%	0.039%
41	15.395	2042	2044	2045	rVB2	1812	1271	0.10%	0.013%
42	15.412	2045	2047	2048	rBV	2246	1803	0.14%	0.018%
43	15.430	2048	2050	2053	rVV3	1581	1668	0.13%	0.017%
44	15.547	2067	2070	2074	rBV4	2764	3464	0.28%	0.035%
45	15.630	2080	2084	2088	rBV5	1759	2754	0.22%	0.027%
46	15.747	2097	2104	2111	rBV	518686	807629	64.50%	8.064%
47	15.847	2115	2121	2130	rBV	140394	218790	17.47%	2.185%
48	15.988	2141	2145	2147	rBV3	2913	3205	0.26%	0.032%
49	16.152	2171	2173	2178	rVB6	3561	5278	0.42%	0.053%
50	16.194	2178	2180	2181	rBV2	3184	2427	0.19%	0.024%
51	16.217	2181	2184	2185	rBV3	1637	1563	0.12%	0.016%
52	16.293	2194	2197	2199	rBV3	2339	2705	0.22%	0.027%
53	16.335	2200	2204	2205	rBV4	2088	2318	0.19%	0.023%
54	16.393	2212	2214	2215	rBV2	1989	1682	0.13%	0.017%
55	16.429	2216	2220	2221	rBV4	1992	2789	0.22%	0.028%
56	16.564	2240	2243	2244	rBV2	3619	3241	0.26%	0.032%
57	16.617	2249	2252	2253	rBV3	2198	2391	0.19%	0.024%
58	16.652	2256	2258	2261	rBV4	3950	4995	0.40%	0.050%
59	16.840	2288	2290	2291	rBV2	3454	2610	0.21%	0.026%
60	16.857	2291	2293	2296	rVB3	5643	5835	0.47%	0.058%
61	16.893	2297	2299	2300	rBV2	4428	2676	0.21%	0.027%
62	17.498	2396	2402	2410	rBV	343289	564466	45.08%	5.636%
63	17.598	2413	2419	2425	rVV2	587273	923373	73.74%	9.220%
64	19.883	2802	2808	2815	rVB	745481	1098378	87.72%	10.967%
65	20.834	2968	2970	2974	rVB5	12635	13733	1.10%	0.137%
66	21.786	3126	3132	3140	rBV	385296	649274	51.85%	6.483%
67	22.714	3288	3290	3292	rVB3	6086	4171	0.33%	0.042%
68	23.078	3351	3352	3354	rVB	5942	4089	0.33%	0.041%
69	23.102	3354	3356	3357	rBV2	4530	3771	0.30%	0.038%
70	23.284	3385	3387	3388	rBV2	5086	4229	0.34%	0.042%
71	23.907	3491	3493	3495	rVB3	4987	2614	0.21%	0.026%
72	24.012	3510	3511	3512	rBV	4116	1575	0.13%	0.016%
73	24.077	3519	3522	3524	rBV4	4288	5280	0.42%	0.053%
74	24.870	3646	3657	3671	rVB2	427652	1252124	100.00%	12.503%
75	25.099	3685	3696	3707	rBV	232838	704028	56.23%	7.030%
76	26.104	3865	3867	3871	rBV5	4907	5099	0.41%	0.051%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032822\
Data File : BG052893.D
Acq On : 28 Mar 2022 16:05
Operator : CG/JU
Sample : N2082-16
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
EW615

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
Title : SVOA CALIBRATION

77	26.321	3898	3904	3906	rBV6	10264	20308	1.62%	0.203%
78	26.574	3945	3947	3949	rBV3	4073	4367	0.35%	0.044%
79	27.702	4135	4139	4141	rBV4	8651	13504	1.08%	0.135%
80	27.890	4169	4171	4172	rBV2	4015	2536	0.20%	0.025%
81	29.423	4428	4432	4434	rBV5	6780	9078	0.73%	0.091%
82	29.869	4506	4508	4509	rBV	3649	2420	0.19%	0.024%
83	30.063	4539	4541	4542	rBV2	4102	2986	0.24%	0.030%
84	30.645	4639	4640	4644	rBV4	4681	4608	0.37%	0.046%
85	31.449	4775	4777	4778	rBV2	4513	2497	0.20%	0.025%




Sum of corrected areas: 10014962

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032822\
Data File : BG052893.D
Acq On : 28 Mar 2022 16:05
Operator : CG/JU
Sample : N2082-16
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
EW615

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

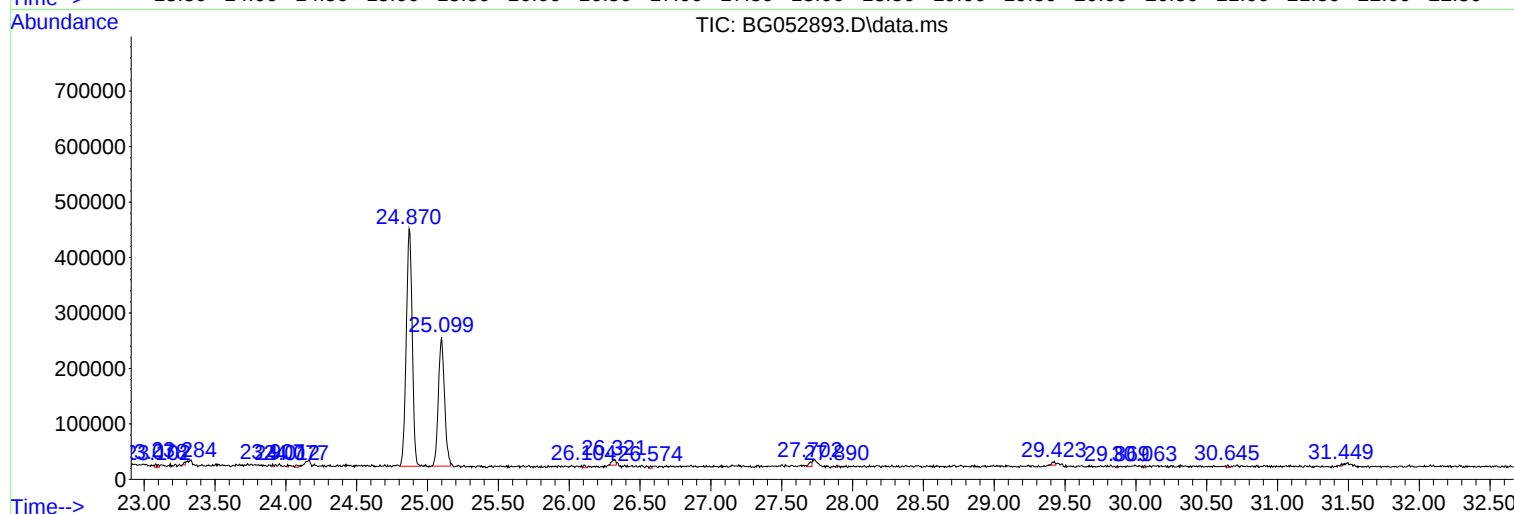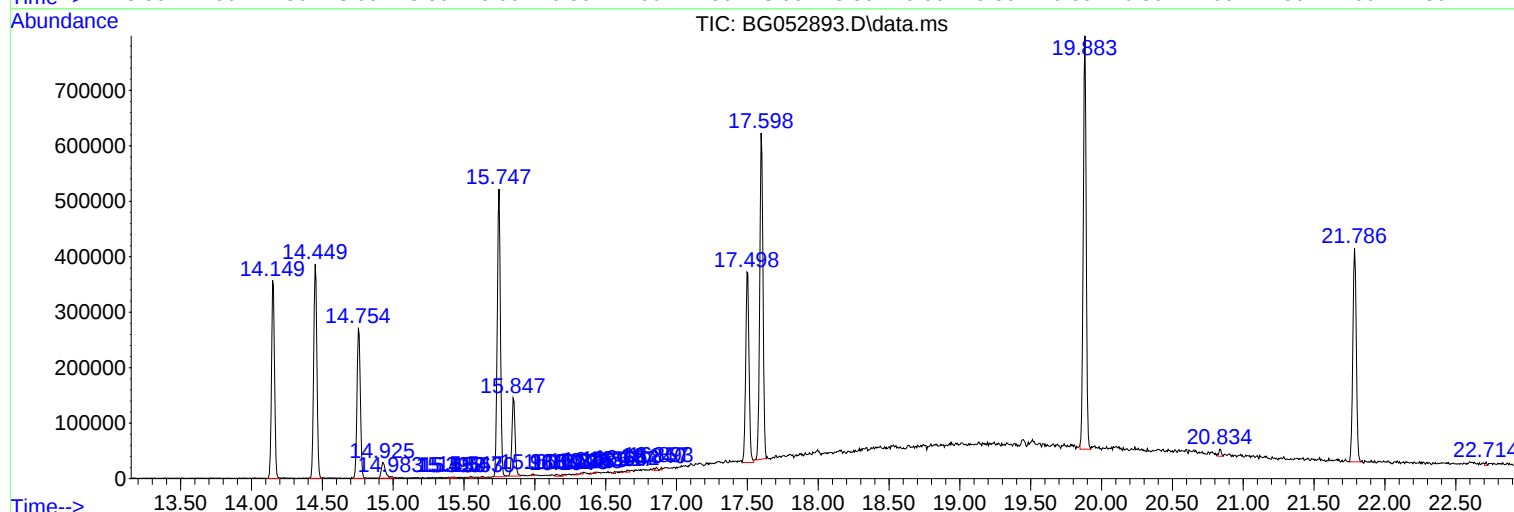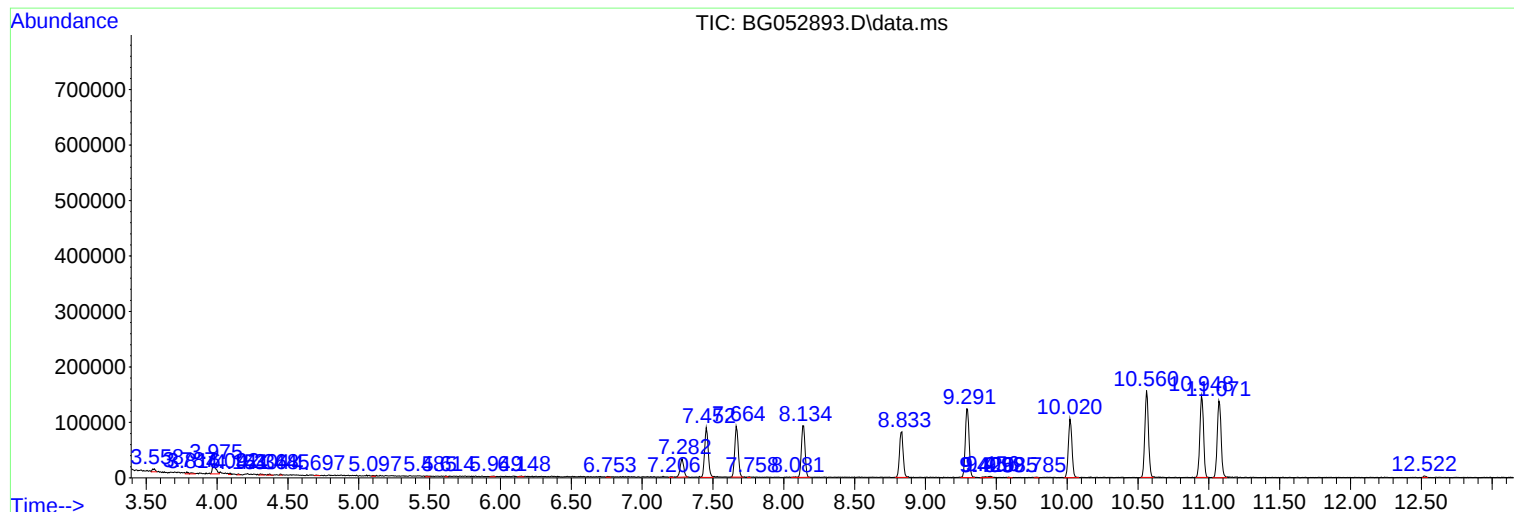

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032822\
Data File : BG052893.D
Acq On : 28 Mar 2022 16:05
Operator : CG/JU
Sample : N2082-16
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
EW615

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032822\
Data File : BG052893.D
Acq On : 28 Mar 2022 16:05
Operator : CG/JU
Sample : N2082-16
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
EW615

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------