

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032822\
 Data File : BG052900.D
 Acq On : 28 Mar 2022 21:14
 Operator : CG/JU
 Sample : PB143650BL
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK650

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
 Title : SVOA CALIBRATION

Signal : TIC: BG052900.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.552	24	28	30	rBV3	5890	6299	0.56%	0.063%
2	3.816	71	73	75	rVB2	1929	1414	0.13%	0.014%
3	3.869	80	82	86	rVB4	2101	2286	0.21%	0.023%
4	3.904	86	88	91	rBV4	1575	1514	0.14%	0.015%
5	3.963	95	98	112	rBV	77365	137949	12.37%	1.370%
6	4.304	154	156	157	rBV2	2114	1450	0.13%	0.014%
7	4.321	157	159	161	rVB3	1936	1328	0.12%	0.013%
8	4.533	193	195	199	rVB2	1483	1648	0.15%	0.016%
9	4.691	220	222	226	rVB3	2166	2243	0.20%	0.022%
10	5.197	305	308	313	rVB2	1930	2040	0.18%	0.020%
11	5.279	320	322	325	rVB4	1604	1356	0.12%	0.013%
12	5.390	339	341	344	rVB3	1565	1836	0.16%	0.018%
13	5.426	344	347	348	rBV2	1461	1655	0.15%	0.016%
14	5.731	396	399	401	rVB4	1237	1239	0.11%	0.012%
15	5.778	406	407	410	rBV3	1230	1376	0.12%	0.014%
16	7.118	632	635	638	rVB3	975	1236	0.11%	0.012%
17	7.159	638	642	646	rBV4	820	1270	0.11%	0.013%
18	7.212	650	651	655	rVB3	1398	1321	0.12%	0.013%
19	7.282	655	663	673	rBV	113273	199368	17.88%	1.980%
20	7.452	684	692	700	rBV	80071	137205	12.31%	1.363%
21	7.511	700	702	705	rVB3	1264	1398	0.13%	0.014%
22	7.664	720	728	734	rVV2	102914	177818	15.95%	1.766%
23	7.905	765	769	771	rBV3	1091	1551	0.14%	0.015%
24	8.134	802	808	816	rVB	86375	155946	13.99%	1.549%
25	8.827	920	926	934	rBV	136398	242066	21.71%	2.404%
26	9.291	997	1005	1016	rBV2	110120	203352	18.24%	2.020%
27	10.019	1122	1129	1137	rVB	94053	167106	14.99%	1.660%
28	10.560	1214	1221	1232	rBV	144128	259375	23.26%	2.576%
29	10.948	1279	1287	1295	rBV2	137958	252646	22.66%	2.510%
30	11.071	1301	1308	1318	rBV2	150124	269309	24.15%	2.675%
31	11.153	1320	1322	1327	rVB2	929	1333	0.12%	0.013%
32	12.357	1526	1527	1531	rBV2	909	1244	0.11%	0.012%
33	12.522	1549	1555	1563	rVB3	2726	4956	0.44%	0.049%
34	13.215	1671	1673	1678	rVB2	927	1265	0.11%	0.013%
35	14.149	1826	1832	1838	rBV	345718	502188	45.04%	4.988%
36	14.449	1876	1883	1890	rBV	331345	540097	48.44%	5.365%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032822\
 Data File : BG052900.D
 Acq On : 28 Mar 2022 21:14
 Operator : CG/JU
 Sample : PB143650BL
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK650

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
 Title : SVOA CALIBRATION

37	14.754	1928	1935	1943	rBV	266925	416908	37.39%	4.141%
38	14.925	1956	1964	1976	rBV2	151268	269706	24.19%	2.679%
39	15.071	1986	1989	1991	rBV2	1285	1191	0.11%	0.012%
40	15.353	2032	2037	2040	rVB2	1005	1345	0.12%	0.013%
41	15.747	2097	2104	2113	rBV	468798	734353	65.86%	7.294%
42	15.847	2115	2121	2131	rVV	139084	218161	19.57%	2.167%
43	15.917	2131	2133	2138	rVB3	1791	2103	0.19%	0.021%
44	15.988	2138	2145	2149	rBV5	4197	7187	0.64%	0.071%
45	16.528	2234	2237	2240	rVV3	1337	1484	0.13%	0.015%
46	17.286	2361	2366	2373	rBV3	1678	3745	0.34%	0.037%
47	17.498	2396	2402	2411	rBV	371067	560369	50.26%	5.566%
48	17.597	2411	2419	2426	rBV	594749	891371	79.95%	8.854%
49	17.868	2461	2465	2467	rBV3	1367	1721	0.15%	0.017%
50	18.056	2495	2497	2500	rVB2	1177	1215	0.11%	0.012%
51	18.144	2509	2512	2516	rBV2	945	1304	0.12%	0.013%
52	18.414	2555	2558	2560	rBV2	1124	1210	0.11%	0.012%
53	18.684	2601	2604	2605	rBV2	1908	1315	0.12%	0.013%
54	18.714	2608	2609	2612	rBV2	1724	1261	0.11%	0.013%
55	18.784	2620	2621	2624	rVB2	2042	1204	0.11%	0.012%
56	19.019	2659	2661	2664	rVB2	1269	1234	0.11%	0.012%
57	19.113	2673	2677	2680	rBV3	1194	1630	0.15%	0.016%
58	19.166	2683	2686	2687	rBV2	1324	1409	0.13%	0.014%
59	19.395	2721	2725	2726	rVB3	1370	1288	0.12%	0.013%
60	19.419	2726	2729	2730	rBV2	1098	1337	0.12%	0.013%
61	19.442	2730	2733	2739	rVV4	7930	11850	1.06%	0.118%
62	19.518	2742	2746	2749	rVB2	7467	10122	0.91%	0.101%
63	19.789	2791	2792	2794	rVB	1791	1251	0.11%	0.012%
64	19.877	2797	2807	2817	rVV	746085	1114977	100.00%	11.075%
65	19.977	2821	2824	2825	rBV3	1568	1631	0.15%	0.016%
66	20.217	2860	2865	2866	rBV4	2773	3656	0.33%	0.036%
67	20.417	2897	2899	2901	rBV3	2353	2252	0.20%	0.022%
68	20.494	2910	2912	2914	rBV2	2095	1650	0.15%	0.016%
69	20.517	2914	2916	2917	rBV2	2212	2060	0.18%	0.020%
70	20.535	2917	2919	2921	rVV3	2128	1731	0.16%	0.017%
71	20.728	2950	2952	2953	rBV2	2997	2499	0.22%	0.025%
72	20.775	2958	2960	2962	rVV2	2837	2436	0.22%	0.024%
73	21.005	2997	2999	3002	rBV3	3021	3424	0.31%	0.034%
74	21.093	3012	3014	3017	rBV4	2689	2866	0.26%	0.028%
75	21.686	3113	3115	3117	rBV3	3439	1585	0.14%	0.016%
76	21.786	3125	3132	3140	rBV	380993	659725	59.17%	6.553%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032822\
 Data File : BG052900.D
 Acq On : 28 Mar 2022 21:14
 Operator : CG/JU
 Sample : PB143650BL
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK650

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
 Title : SVOA CALIBRATION

77	22.579	3265	3267	3269	rBV3	3386	2303	0.21%	0.023%
78	22.790	3302	3303	3305	rBV2	3595	2850	0.26%	0.028%
79	22.931	3325	3327	3330	rBV3	4893	5310	0.48%	0.053%
80	23.619	3443	3444	3446	rBV2	5316	4284	0.38%	0.043%
81	24.153	3533	3535	3537	rBV3	4507	3533	0.32%	0.035%
82	24.864	3645	3656	3671	rBV2	383833	1106407	99.23%	10.990%
83	25.017	3679	3682	3683	rBV3	4232	4609	0.41%	0.046%
84	25.099	3685	3696	3710	rVB2	217531	662023	59.38%	6.576%
85	26.579	3946	3948	3951	rVB4	4183	3396	0.30%	0.034%
86	26.609	3951	3953	3955	rBV2	4271	3443	0.31%	0.034%
87	27.602	4121	4122	4123	rVB	5023	1771	0.16%	0.018%
88	28.165	4216	4218	4219	rBV	3455	1928	0.17%	0.019%
89	28.647	4298	4300	4302	rBV3	3640	3293	0.30%	0.033%
90	29.287	4407	4409	4410	rBV2	2858	1607	0.14%	0.016%
91	29.352	4418	4420	4421	rBV2	3391	2376	0.21%	0.024%
92	29.752	4486	4488	4491	rBV4	3296	3057	0.27%	0.030%
93	29.787	4493	4494	4496	rBV2	3513	2590	0.23%	0.026%
94	30.151	4555	4556	4557	rBV	4446	1880	0.17%	0.019%
95	30.204	4563	4565	4566	rBV2	3716	2892	0.26%	0.029%
96	30.245	4570	4572	4573	rBV2	4921	3950	0.35%	0.039%
97	31.085	4713	4715	4717	rBV2	3209	1852	0.17%	0.018%
98	31.150	4724	4726	4727	rBV2	3507	1674	0.15%	0.017%
99	32.043	4876	4878	4880	rBV3	3568	3167	0.28%	0.031%
100	32.148	4894	4896	4897	rBV2	3220	1674	0.15%	0.017%




Sum of corrected areas: 10067318

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032822\
Data File : BG052900.D
Acq On : 28 Mar 2022 21:14
Operator : CG/JU
Sample : PB143650BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK650

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

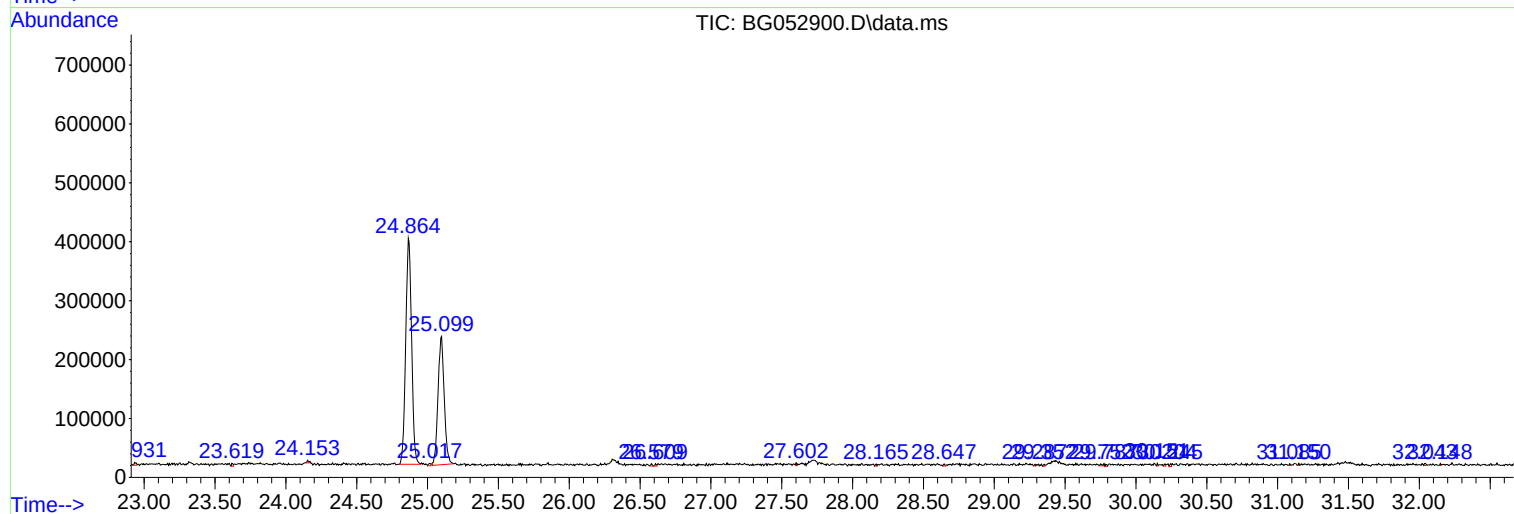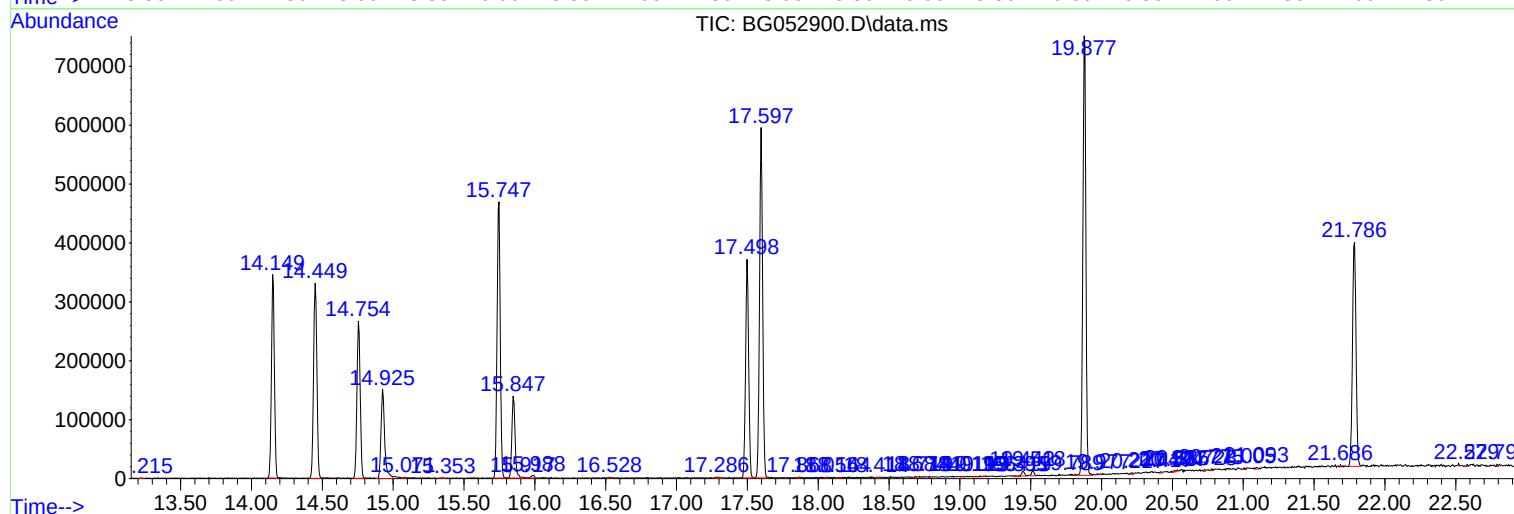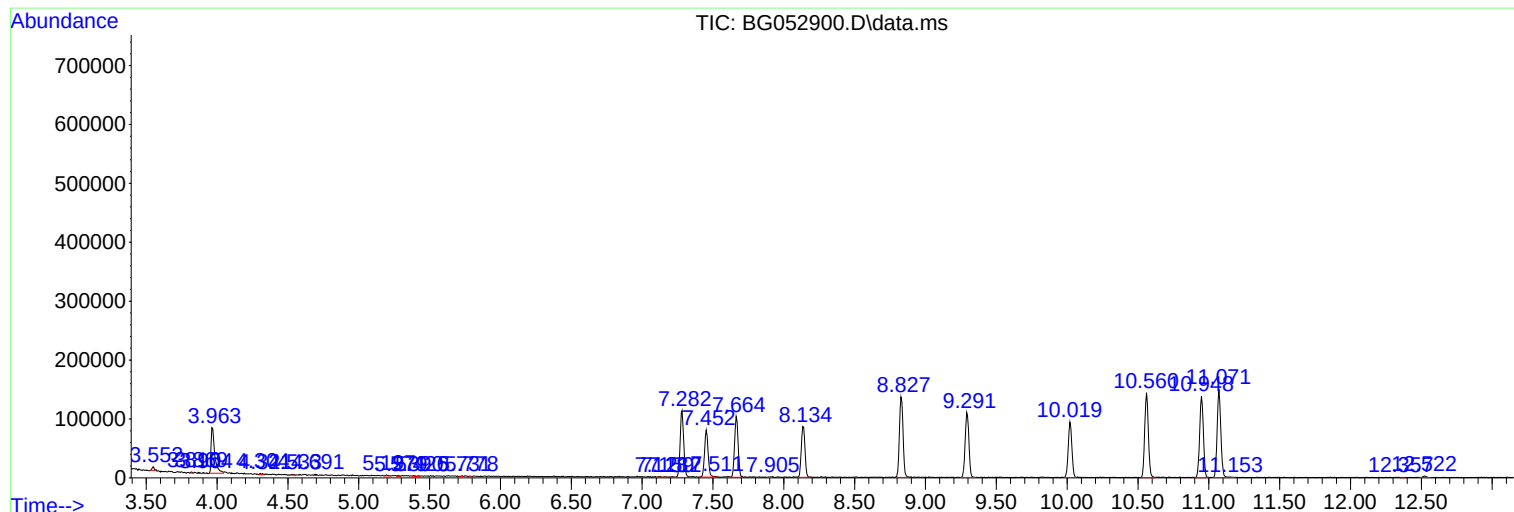

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032822\
Data File : BG052900.D
Acq On : 28 Mar 2022 21:14
Operator : CG/JU
Sample : PB143650BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK650

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032822\
Data File : BG052900.D
Acq On : 28 Mar 2022 21:14
Operator : CG/JU
Sample : PB143650BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK650

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc