

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032822\
 Data File : BG052901.D
 Acq On : 28 Mar 2022 21:52
 Operator : CG/JU
 Sample : PB143652BL
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK652

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
 Title : SVOA CALIBRATION

Signal : TIC: BG052901.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.447	8	10	13	rBV4	2692	3291	0.30%	0.033%
2	3.546	25	27	34	rVB4	7645	10974	1.00%	0.110%
3	3.834	74	76	81	rVB4	1564	1906	0.17%	0.019%
4	3.928	90	92	95	rVB3	2011	1728	0.16%	0.017%
5	3.963	95	98	112	rBV	80805	143496	13.13%	1.442%
6	4.310	152	157	163	rVB4	2701	5745	0.53%	0.058%
7	4.428	174	177	178	rBV2	1888	1468	0.13%	0.015%
8	4.451	178	181	182	rBV3	2053	1483	0.14%	0.015%
9	4.486	186	187	190	rBV2	1371	1499	0.14%	0.015%
10	4.704	223	224	227	rVB3	2410	1620	0.15%	0.016%
11	4.780	234	237	240	rVB3	1771	2307	0.21%	0.023%
12	4.809	240	242	244	rBV2	1485	1445	0.13%	0.015%
13	5.503	356	360	364	rVB3	1186	1992	0.18%	0.020%
14	6.025	444	449	450	rBV2	1516	1564	0.14%	0.016%
15	6.066	454	456	459	rVB2	1435	1371	0.13%	0.014%
16	6.225	481	483	486	rVB3	1310	1548	0.14%	0.016%
17	6.642	551	554	558	rVB3	1293	1874	0.17%	0.019%
18	7.059	624	625	630	rVB3	1278	1530	0.14%	0.015%
19	7.183	645	646	651	rVB3	1014	1357	0.12%	0.014%
20	7.277	656	662	671	rVB	109353	195955	17.93%	1.969%
21	7.365	675	677	680	rBV3	1155	1478	0.14%	0.015%
22	7.453	685	692	699	rBV2	78800	135273	12.38%	1.359%
23	7.664	722	728	735	rBV	103144	175859	16.09%	1.767%
24	8.134	802	808	815	rVB	91647	156173	14.29%	1.569%
25	8.328	836	841	845	rBV4	1391	2654	0.24%	0.027%
26	8.827	917	926	934	rBV3	141405	245000	22.42%	2.462%
27	9.292	997	1005	1013	rBV	110489	197665	18.09%	1.986%
28	10.020	1121	1129	1137	rBV	90848	161982	14.82%	1.628%
29	10.560	1212	1221	1231	rBV	139258	251788	23.04%	2.530%
30	10.948	1279	1287	1296	rVB	141641	253517	23.20%	2.547%
31	11.071	1298	1308	1317	rBV	144958	269345	24.65%	2.706%
32	12.522	1549	1555	1560	rBV3	3198	4515	0.41%	0.045%
33	14.150	1826	1832	1842	rBV	343925	497563	45.54%	4.999%
34	14.449	1876	1883	1891	rVV	322999	525645	48.11%	5.281%
35	14.755	1929	1935	1943	rBV	259397	414215	37.91%	4.162%
36	14.925	1958	1964	1980	rBV	150494	267799	24.51%	2.691%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032822\
 Data File : BG052901.D
 Acq On : 28 Mar 2022 21:52
 Operator : CG/JU
 Sample : PB143652BL
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK652

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
 Title : SVOA CALIBRATION

37	15.101	1992	1994	1998	rBV3	1132	1532	0.14%	0.015%
38	15.542	2064	2069	2071	rBV2	961	1390	0.13%	0.014%
39	15.747	2097	2104	2112	rBV	449870	717295	65.65%	7.207%
40	15.847	2115	2121	2128	rBV	136444	207123	18.96%	2.081%
41	15.982	2140	2144	2147	rVB3	4429	5283	0.48%	0.053%
42	16.529	2234	2237	2240	rBV3	1580	1783	0.16%	0.018%
43	17.445	2388	2393	2395	rVV3	1042	1485	0.14%	0.015%
44	17.498	2395	2402	2409	rVV	376060	559503	51.21%	5.622%
45	17.598	2412	2419	2427	rBV	576424	874916	80.07%	8.791%
46	18.456	2559	2565	2568	rBV5	1611	3086	0.28%	0.031%
47	18.591	2585	2588	2589	rBV	1901	1348	0.12%	0.014%
48	18.632	2592	2595	2599	rVV4	1502	2439	0.22%	0.025%
49	18.673	2599	2602	2605	rVV3	1507	2125	0.19%	0.021%
50	18.720	2607	2610	2612	rVV2	1884	1993	0.18%	0.020%
51	18.749	2612	2615	2618	rVV2	1565	2305	0.21%	0.023%
52	18.790	2618	2622	2623	rVV3	1380	1673	0.15%	0.017%
53	18.984	2653	2655	2658	rBV4	2049	2332	0.21%	0.023%
54	19.055	2665	2667	2669	rBV3	1660	1576	0.14%	0.016%
55	19.166	2683	2686	2688	rBV3	1719	1788	0.16%	0.018%
56	19.395	2724	2725	2728	rBV3	2033	1424	0.13%	0.014%
57	19.442	2730	2733	2738	rBV4	7914	12412	1.14%	0.125%
58	19.519	2742	2746	2751	rBV2	8477	12499	1.14%	0.126%
59	19.642	2765	2767	2770	rBV3	1905	1505	0.14%	0.015%
60	19.666	2770	2771	2774	rVB2	1764	1562	0.14%	0.016%
61	19.719	2777	2780	2783	rVB5	1373	1505	0.14%	0.015%
62	19.807	2793	2795	2797	rVB3	1681	1343	0.12%	0.013%
63	19.883	2801	2808	2816	rVB	736116	1092645	100.00%	10.978%
64	20.095	2842	2844	2845	rBV2	2231	1492	0.14%	0.015%
65	20.147	2851	2853	2855	rVB3	1874	1486	0.14%	0.015%
66	20.212	2862	2864	2866	rBV2	1988	1577	0.14%	0.016%
67	20.294	2876	2878	2880	rBV3	1794	1434	0.13%	0.014%
68	20.324	2881	2883	2885	rVB3	2959	2274	0.21%	0.023%
69	20.353	2885	2888	2889	rBV2	2296	2243	0.21%	0.023%
70	20.447	2902	2904	2909	rBV5	2028	2515	0.23%	0.025%
71	20.529	2915	2918	2919	rBV3	4100	3817	0.35%	0.038%
72	20.547	2919	2921	2923	rBV3	2156	2797	0.26%	0.028%
73	20.747	2953	2955	2957	rVB2	2899	2019	0.18%	0.020%
74	20.829	2967	2969	2973	rVB4	3098	3343	0.31%	0.034%
75	20.888	2977	2979	2983	rBV5	2802	3849	0.35%	0.039%
76	21.170	3025	3027	3028	rBV2	2715	2004	0.18%	0.020%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032822\
 Data File : BG052901.D
 Acq On : 28 Mar 2022 21:52
 Operator : CG/JU
 Sample : PB143652BL
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK652

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
 Title : SVOA CALIBRATION

77	21.199	3030	3032	3034	rBV3	2949	2834	0.26%	0.028%
78	21.781	3125	3131	3139	rBV2	395244	653941	59.85%	6.570%
79	23.096	3354	3355	3357	rBV2	3844	3351	0.31%	0.034%
80	24.447	3583	3585	3587	rVB	4610	3214	0.29%	0.032%
81	24.465	3587	3588	3591	rBV3	4783	4527	0.41%	0.045%
82	24.865	3646	3656	3671	rVB2	369892	1088406	99.61%	10.936%
83	25.094	3685	3695	3710	rVB2	211592	657492	60.17%	6.606%
84	25.252	3720	3722	3725	rBV3	2976	3244	0.30%	0.033%
85	27.203	4052	4054	4056	rBV3	3678	1756	0.16%	0.018%
86	27.379	4082	4084	4085	rBV2	4158	3526	0.32%	0.035%
87	28.994	4357	4359	4360	rBV2	2706	1391	0.13%	0.014%
88	29.012	4360	4362	4364	rBV2	3186	3147	0.29%	0.032%
89	29.094	4374	4376	4379	rBV3	3400	3700	0.34%	0.037%
90	29.341	4416	4418	4420	rBV2	3463	2027	0.19%	0.020%
91	29.629	4465	4467	4469	rBV3	3852	3103	0.28%	0.031%
92	30.404	4597	4599	4601	rVB3	3266	1590	0.15%	0.016%
93	30.598	4631	4632	4634	rBV	4639	4129	0.38%	0.041%
94	31.215	4735	4737	4740	rBV4	3098	2219	0.20%	0.022%
95	31.567	4795	4797	4801	rBV4	2991	2861	0.26%	0.029%
96	31.597	4801	4802	4806	rVB3	4178	3527	0.32%	0.035%
97	31.661	4811	4813	4816	rBV4	3278	3554	0.33%	0.036%
98	31.714	4820	4822	4823	rBV2	2987	1550	0.14%	0.016%
99	32.372	4932	4934	4935	rBV2	3463	2122	0.19%	0.021%
100	32.601	4971	4973	4976	rBV4	4074	4194	0.38%	0.042%




Sum of corrected areas: 9952749

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032822\
Data File : BG052901.D
Acq On : 28 Mar 2022 21:52
Operator : CG/JU
Sample : PB143652BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK652

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

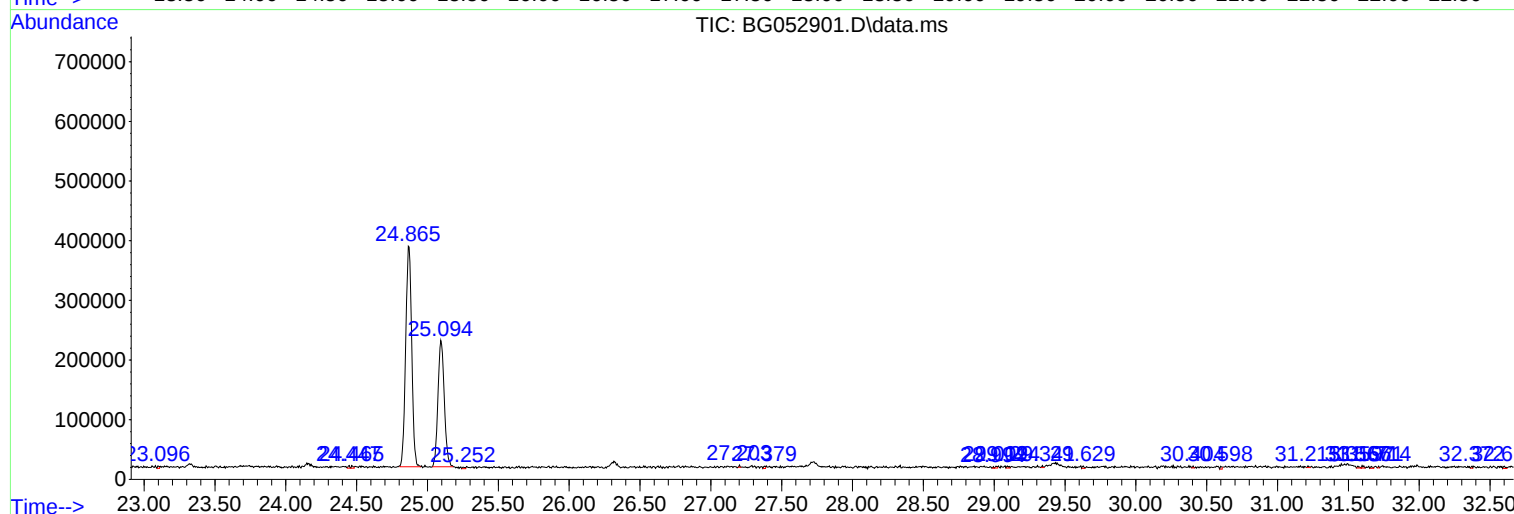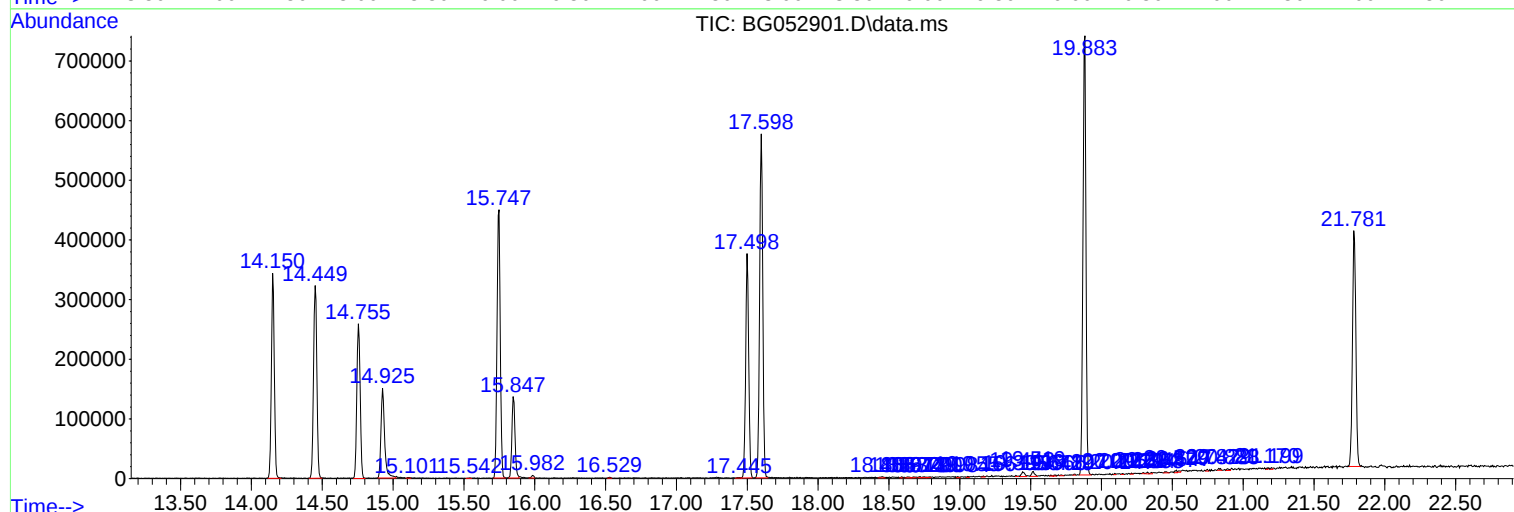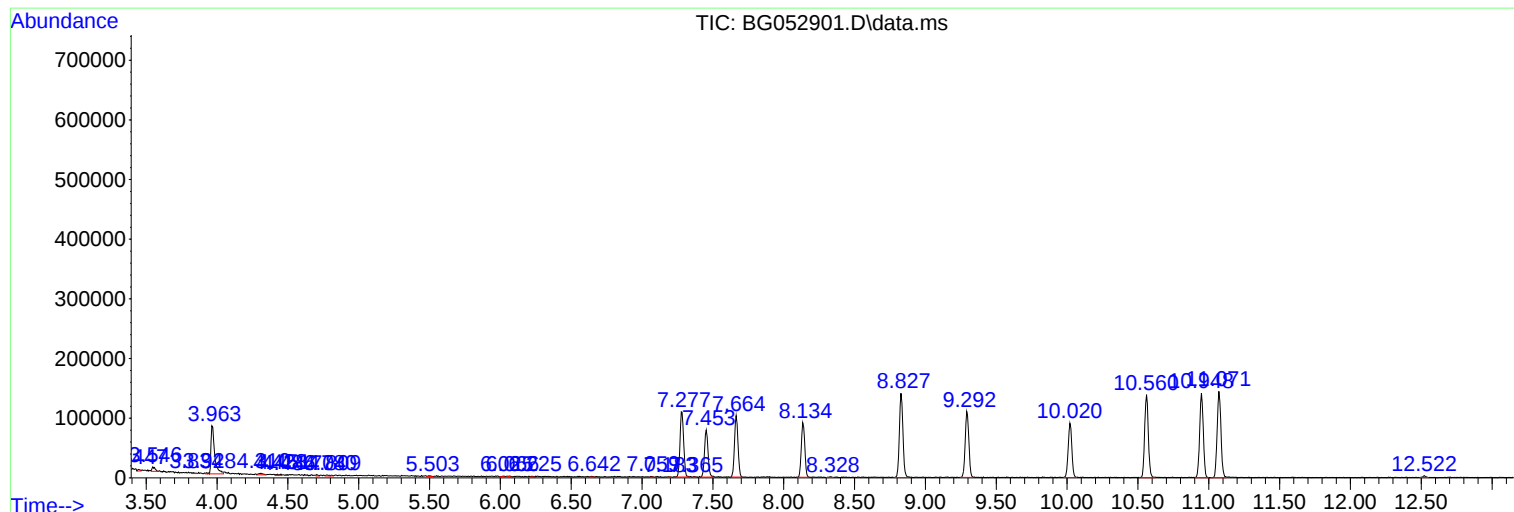

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032822\
Data File : BG052901.D
Acq On : 28 Mar 2022 21:52
Operator : CG/JU
Sample : PB143652BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK652

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032822\
Data File : BG052901.D
Acq On : 28 Mar 2022 21:52
Operator : CG/JU
Sample : PB143652BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK652

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc