

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032822\
 Data File : BG052902.D
 Acq On : 28 Mar 2022 22:31
 Operator : CG/JU
 Sample : N2100-01
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0AF2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
 Title : SVOA CALIBRATION

Signal : TIC: BG052902.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.517	20	22	23	rVB	2634	1327	0.14%	0.015%
2	3.552	26	28	32	rVB4	6497	6719	0.71%	0.078%
3	3.834	75	76	78	rVB2	2207	1552	0.16%	0.018%
4	3.857	78	80	82	rBV2	1473	1818	0.19%	0.021%
5	3.969	97	99	114	rVV	26413	47824	5.04%	0.557%
6	4.080	116	118	119	rVB	2864	1732	0.18%	0.020%
7	4.092	119	120	123	rBV2	2061	1980	0.21%	0.023%
8	4.169	130	133	134	rBV2	2142	1914	0.20%	0.022%
9	4.251	144	147	149	rVB4	1899	2003	0.21%	0.023%
10	4.280	149	152	153	rVV2	1434	1404	0.15%	0.016%
11	4.315	155	158	159	rVV3	2867	2791	0.29%	0.032%
12	4.809	240	242	245	rBV3	1084	1415	0.15%	0.016%
13	5.020	277	278	284	rBV4	1072	1285	0.14%	0.015%
14	5.232	310	314	317	rVB4	1919	1969	0.21%	0.023%
15	5.455	349	352	356	rBV4	1339	1861	0.20%	0.022%
16	5.520	361	363	368	rBV2	1159	1653	0.17%	0.019%
17	5.678	388	390	393	rBV3	1350	1638	0.17%	0.019%
18	6.048	452	453	457	rBV3	1408	1305	0.14%	0.015%
19	6.090	457	460	462	rBV4	1234	1417	0.15%	0.016%
20	6.242	484	486	491	rBV4	1478	1297	0.14%	0.015%
21	6.354	502	505	507	rVB3	927	1254	0.13%	0.015%
22	7.276	657	662	670	rBV2	21261	39304	4.14%	0.458%
23	7.452	686	692	700	rBV	71931	119061	12.54%	1.386%
24	7.664	722	728	737	rBV	69918	117199	12.34%	1.364%
25	8.052	791	794	796	rBV	1623	1488	0.16%	0.017%
26	8.134	801	808	816	rVV	93820	164756	17.35%	1.918%
27	8.827	919	926	933	rBV2	60314	110934	11.68%	1.291%
28	9.291	998	1005	1015	rBV	99238	180365	18.99%	2.100%
29	9.591	1053	1056	1060	rVB2	3133	4090	0.43%	0.048%
30	10.020	1121	1129	1136	rBV2	79014	138805	14.62%	1.616%
31	10.401	1191	1194	1196	rVB2	1353	1360	0.14%	0.016%
32	10.560	1214	1221	1229	rBV	115664	204096	21.49%	2.376%
33	10.742	1247	1252	1254	rBV2	908	1354	0.14%	0.016%
34	10.948	1280	1287	1297	rVB	141296	258675	27.24%	3.011%
35	11.071	1301	1308	1317	rBV	133710	240841	25.36%	2.804%
36	11.253	1334	1339	1341	rBV2	862	1266	0.13%	0.015%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032822\
 Data File : BG052902.D
 Acq On : 28 Mar 2022 22:31
 Operator : CG/JU
 Sample : N2100-01
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0AF2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
 Title : SVOA CALIBRATION

37	12.522	1550	1555	1561	rVB3	2155	3585	0.38%	0.042%
38	14.149	1826	1832	1840	rBV	283816	415058	43.70%	4.832%
39	14.449	1876	1883	1889	rBV	290623	462985	48.75%	5.390%
40	14.754	1927	1935	1943	rBV	269605	425005	44.75%	4.948%
41	14.925	1959	1964	1973	rBV2	22315	41870	4.41%	0.487%
42	15.547	2068	2070	2074	rBV3	1536	1533	0.16%	0.018%
43	15.747	2097	2104	2112	rBV	404871	628117	66.14%	7.312%
44	15.847	2116	2121	2130	rVV	120089	188844	19.88%	2.198%
45	15.988	2140	2145	2148	rBV2	3699	4446	0.47%	0.052%
46	16.816	2281	2286	2289	rBV	699	1286	0.14%	0.015%
47	17.286	2361	2366	2371	rVB2	1786	2641	0.28%	0.031%
48	17.498	2396	2402	2410	rBV	368095	573336	60.37%	6.675%
49	17.597	2412	2419	2429	rVB2	504414	769579	81.03%	8.959%
50	17.768	2444	2448	2452	rVB3	3902	5720	0.60%	0.067%
51	17.832	2456	2459	2461	rVV	1209	1257	0.13%	0.015%
52	17.879	2461	2467	2468	rVB3	979	1789	0.19%	0.021%
53	17.985	2482	2485	2488	rBV2	902	1312	0.14%	0.015%
54	18.449	2562	2564	2567	rVB3	1768	1893	0.20%	0.022%
55	18.808	2622	2625	2627	rVB2	2284	2257	0.24%	0.026%
56	18.843	2627	2631	2632	rBV3	1543	2189	0.23%	0.025%
57	18.937	2645	2647	2652	rBV4	1749	2216	0.23%	0.026%
58	19.007	2657	2659	2661	rBV2	1243	1428	0.15%	0.017%
59	19.448	2729	2734	2738	rVB2	8399	10615	1.12%	0.124%
60	19.513	2741	2745	2750	rBV2	6669	10078	1.06%	0.117%
61	19.642	2766	2767	2770	rBV2	1324	1256	0.13%	0.015%
62	19.789	2789	2792	2794	rBV4	1684	1981	0.21%	0.023%
63	19.877	2799	2807	2815	rVV	657587	949715	100.00%	11.056%
64	19.959	2818	2821	2824	rBV4	2616	2806	0.30%	0.033%
65	19.994	2826	2827	2829	rBV2	1825	1324	0.14%	0.015%
66	20.129	2849	2850	2852	rBV2	1294	1316	0.14%	0.015%
67	20.259	2870	2872	2874	rBV3	2489	2408	0.25%	0.028%
68	20.476	2904	2909	2910	rBV5	3684	5186	0.55%	0.060%
69	20.511	2913	2915	2916	rBV2	2835	2459	0.26%	0.029%
70	20.593	2927	2929	2930	rBV2	3284	2231	0.23%	0.026%
71	20.611	2930	2932	2933	rVB2	2307	1275	0.13%	0.015%
72	20.670	2940	2942	2945	rVB4	2492	2444	0.26%	0.028%
73	20.828	2967	2969	2976	rVB6	3613	6148	0.65%	0.072%
74	20.881	2976	2978	2980	rVB2	2629	1849	0.19%	0.022%
75	21.240	3037	3039	3041	rBV3	3442	2714	0.29%	0.032%
76	21.786	3124	3132	3142	rBV	390510	678063	71.40%	7.894%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032822\
 Data File : BG052902.D
 Acq On : 28 Mar 2022 22:31
 Operator : CG/JU
 Sample : N2100-01
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0AF2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
 Title : SVOA CALIBRATION

77	22.121	3187	3189	3190	rBV2	3214	2578	0.27%	0.030%
78	22.696	3285	3287	3290	rBV4	3707	3443	0.36%	0.040%
79	22.814	3305	3307	3308	rBV2	3474	2398	0.25%	0.028%
80	23.672	3451	3453	3456	rBV2	3367	2826	0.30%	0.033%
81	24.147	3532	3534	3538	rBV4	6155	9904	1.04%	0.115%
82	24.870	3646	3657	3669	rVB	331714	933186	98.26%	10.864%
83	25.099	3684	3696	3712	rBV2	223878	689118	72.56%	8.022%
84	25.704	3797	3799	3803	rVB5	3622	2719	0.29%	0.032%
85	25.751	3806	3807	3808	rVB	3867	1363	0.14%	0.016%
86	25.957	3840	3842	3845	rBV4	3155	3353	0.35%	0.039%
87	26.321	3900	3904	3909	rVB8	6106	11963	1.26%	0.139%
88	26.403	3916	3918	3919	rBV2	2876	2015	0.21%	0.023%
89	26.433	3921	3923	3924	rVV2	3160	1374	0.14%	0.016%
90	27.484	4100	4102	4104	rBV3	2979	1387	0.15%	0.016%
91	27.672	4132	4134	4137	rBV4	3078	3167	0.33%	0.037%
92	28.124	4210	4211	4212	rVB	4646	1638	0.17%	0.019%
93	29.100	4375	4377	4378	rBV2	4569	2785	0.29%	0.032%
94	29.276	4405	4407	4410	rBV4	3732	3200	0.34%	0.037%
95	29.564	4454	4456	4459	rVB4	4753	3406	0.36%	0.040%
96	29.593	4459	4461	4463	rBV3	3536	3221	0.34%	0.037%
97	30.833	4671	4672	4675	rBV3	3684	3705	0.39%	0.043%
98	31.079	4712	4714	4718	rVB4	4061	4596	0.48%	0.054%
99	31.490	4782	4784	4785	rBV2	3447	2975	0.31%	0.035%
100	32.501	4954	4956	4957	rBV2	3034	1605	0.17%	0.019%




Sum of corrected areas: 8589891

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032822\
Data File : BG052902.D
Acq On : 28 Mar 2022 22:31
Operator : CG/JU
Sample : N2100-01
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0AF2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

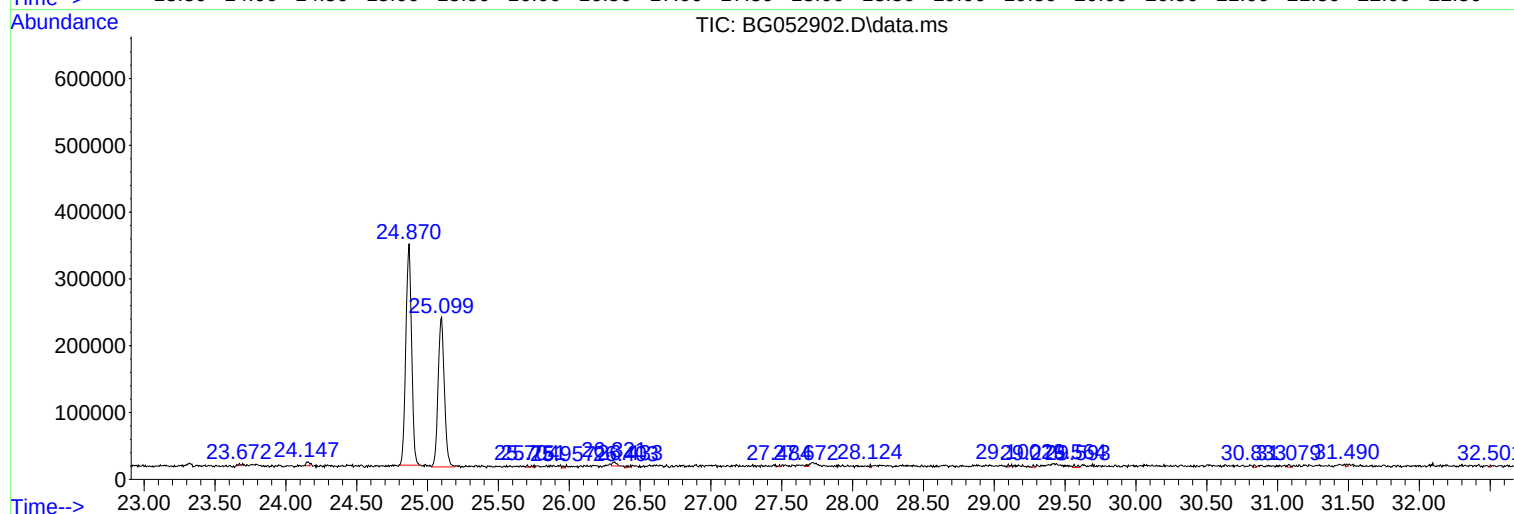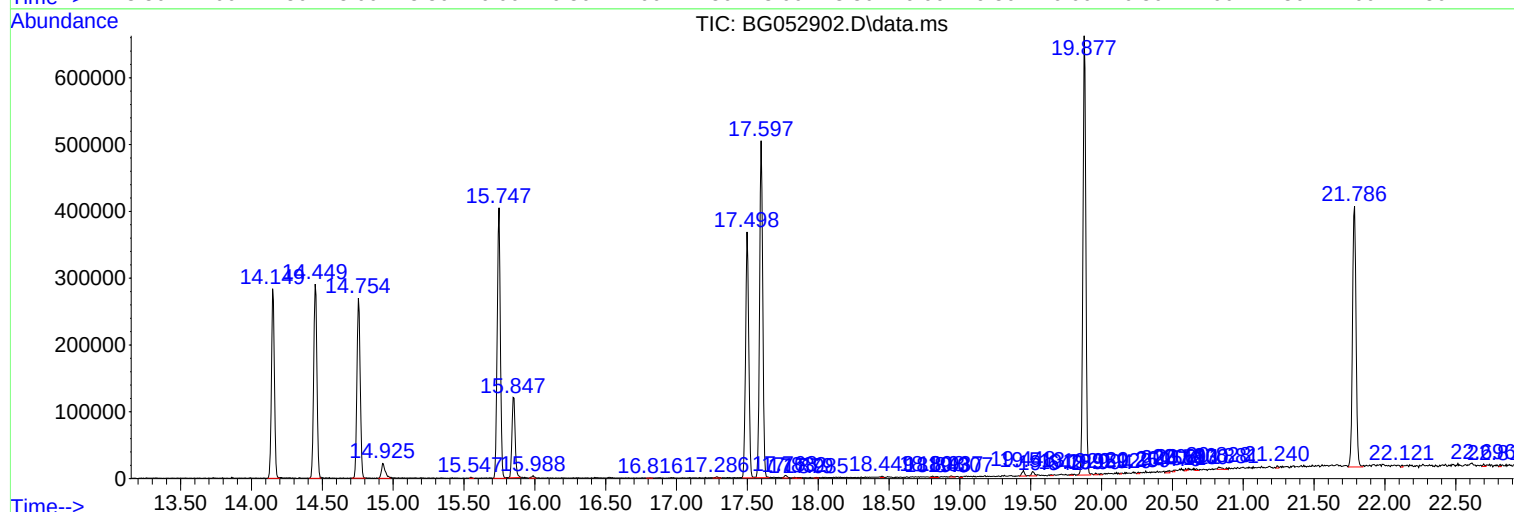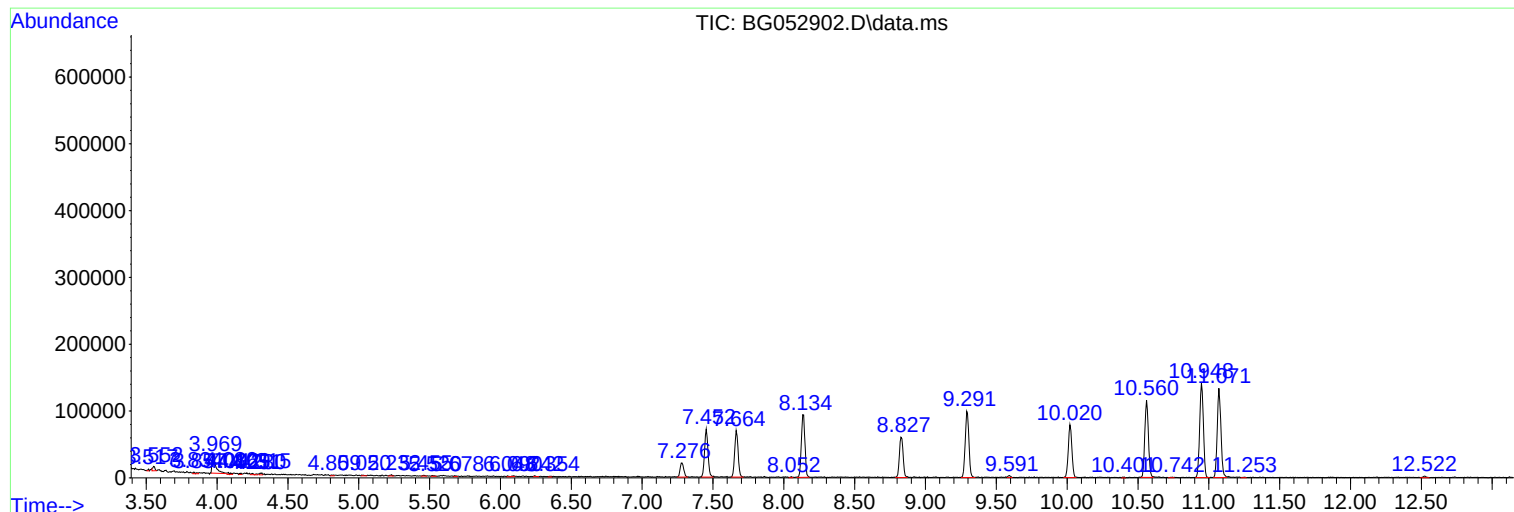

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032822\
Data File : BG052902.D
Acq On : 28 Mar 2022 22:31
Operator : CG/JU
Sample : N2100-01
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0AF2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032822\
Data File : BG052902.D
Acq On : 28 Mar 2022 22:31
Operator : CG/JU
Sample : N2100-01
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0AF2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc