

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032822\
 Data File : BG052908.D
 Acq On : 29 Mar 2022 2:21
 Operator : CG/JU
 Sample : N2100-09
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0AG1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
 Title : SVOA CALIBRATION

Signal : TIC: BG052908.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.549	24	27	32	rVV4	6689	9668	0.75%	0.093%
2	3.778	65	66	70	rBV3	2208	3169	0.25%	0.030%
3	3.908	84	88	90	rBV4	1607	2123	0.17%	0.020%
4	3.978	97	100	108	rBV	18909	36062	2.81%	0.345%
5	4.213	138	140	143	rVV3	1965	2272	0.18%	0.022%
6	4.313	154	157	159	rBV2	2613	2040	0.16%	0.020%
7	6.069	453	456	461	rBV2	1656	2854	0.22%	0.027%
8	6.951	602	606	608	rVB3	1260	1773	0.14%	0.017%
9	7.280	656	662	668	rVB2	27432	47127	3.67%	0.451%
10	7.450	684	691	701	rBV	90687	154471	12.04%	1.480%
11	7.661	721	727	735	rVB	85511	153271	11.95%	1.468%
12	7.926	768	772	775	rBV	1324	2721	0.21%	0.026%
13	8.137	801	808	817	rVB	89303	159024	12.40%	1.523%
14	8.361	842	846	849	rVB	1217	1677	0.13%	0.016%
15	8.830	919	926	933	rBV	81151	140841	10.98%	1.349%
16	9.295	997	1005	1014	rBV	128772	232692	18.14%	2.229%
17	10.017	1122	1128	1137	rVV	100154	181279	14.13%	1.736%
18	10.558	1213	1220	1230	rBV	146726	263095	20.51%	2.520%
19	10.945	1278	1286	1294	rVB	131455	248252	19.36%	2.378%
20	11.074	1300	1308	1319	rBV	137185	264261	20.61%	2.531%
21	11.439	1365	1370	1373	rVB2	882	1516	0.12%	0.015%
22	12.525	1548	1555	1560	rBV3	3218	5728	0.45%	0.055%
23	14.153	1825	1832	1838	rBV	371311	539973	42.10%	5.172%
24	14.452	1874	1883	1891	rBV	373584	596963	46.55%	5.718%
25	14.552	1897	1900	1905	rVB3	1157	1593	0.12%	0.015%
26	14.758	1927	1935	1942	rBV	261694	407163	31.75%	3.900%
27	14.822	1942	1946	1949	rVB	1125	1731	0.13%	0.017%
28	14.928	1958	1964	1973	rBV2	24937	51165	3.99%	0.490%
29	15.680	2088	2092	2094	rBV	1323	1591	0.12%	0.015%
30	15.745	2096	2103	2112	rVV	551888	832184	64.89%	7.971%
31	15.850	2115	2121	2132	rVV	172328	262785	20.49%	2.517%
32	15.985	2139	2144	2147	rBV4	5253	7694	0.60%	0.074%
33	16.426	2212	2219	2224	rBV4	3353	5617	0.44%	0.054%
34	16.485	2226	2229	2232	rVB3	1263	1647	0.13%	0.016%
35	16.526	2232	2236	2239	rBV2	1674	2775	0.22%	0.027%
36	17.495	2392	2401	2410	rBV	349292	551930	43.04%	5.286%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032822\
 Data File : BG052908.D
 Acq On : 29 Mar 2022 2:21
 Operator : CG/JU
 Sample : N2100-09
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0AG1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
 Title : SVOA CALIBRATION

37	17.595	2411	2418	2428	rVV2	647304	1019962	79.53%	9.769%
38	17.695	2433	2435	2439	rVB2	1680	1656	0.13%	0.016%
39	18.153	2511	2513	2517	rVB2	1553	2118	0.17%	0.020%
40	18.435	2560	2561	2566	rBV3	1391	1828	0.14%	0.018%
41	18.934	2643	2646	2648	rBV3	1378	1541	0.12%	0.015%
42	19.017	2658	2660	2663	rVB4	2165	1640	0.13%	0.016%
43	19.281	2703	2705	2709	rVB4	1291	1691	0.13%	0.016%
44	19.446	2729	2733	2737	rVV3	9922	13102	1.02%	0.125%
45	19.510	2740	2744	2749	rVV	9931	13900	1.08%	0.133%
46	19.557	2749	2752	2756	rVB3	1520	2327	0.18%	0.022%
47	19.804	2791	2794	2796	rBV4	2062	2336	0.18%	0.022%
48	19.880	2799	2807	2814	rBV	874671	1258122	98.10%	12.050%
49	20.092	2840	2843	2847	rBV5	5623	6693	0.52%	0.064%
50	20.156	2851	2854	2855	rBV4	2064	2307	0.18%	0.022%
51	20.338	2884	2885	2888	rBV2	2788	2794	0.22%	0.027%
52	20.491	2909	2911	2913	rBV2	2533	2022	0.16%	0.019%
53	20.861	2972	2974	2976	rVB3	2988	1497	0.12%	0.014%
54	20.902	2978	2981	2982	rBV3	3393	2952	0.23%	0.028%
55	21.008	2997	2999	3001	rVB3	2611	1757	0.14%	0.017%
56	21.184	3027	3029	3032	rVB4	3644	3675	0.29%	0.035%
57	21.525	3086	3087	3088	rVB	4351	1532	0.12%	0.015%
58	21.666	3105	3111	3117	rVB	172876	237820	18.54%	2.278%
59	21.784	3124	3131	3138	rBV	380542	637527	49.71%	6.106%
60	22.060	3176	3178	3180	rBV3	4062	3428	0.27%	0.033%
61	22.206	3201	3203	3206	rBV3	3408	2962	0.23%	0.028%
62	23.029	3341	3343	3344	rBV2	2958	1962	0.15%	0.019%
63	23.187	3368	3370	3372	rBV2	3602	3234	0.25%	0.031%
64	23.234	3376	3378	3379	rVB2	3558	2057	0.16%	0.020%
65	23.593	3437	3439	3440	rBV2	4066	2182	0.17%	0.021%
66	23.740	3462	3464	3465	rBV	4095	2419	0.19%	0.023%
67	23.922	3493	3495	3499	rBV4	4084	5025	0.39%	0.048%
68	23.969	3501	3503	3506	rVB3	3662	2711	0.21%	0.026%
69	23.992	3506	3507	3509	rBV2	2933	1727	0.13%	0.017%
70	24.785	3641	3642	3643	rBV	4489	1635	0.13%	0.016%
71	24.868	3643	3656	3669	rBV	448065	1282492	100.00%	12.284%
72	25.003	3677	3679	3680	rBV2	4420	3222	0.25%	0.031%
73	25.097	3684	3695	3708	rVB3	211974	646073	50.38%	6.188%
74	25.291	3727	3728	3731	rBV3	4182	4475	0.35%	0.043%
75	26.283	3895	3897	3898	rBV2	3781	2126	0.17%	0.020%
76	26.583	3946	3948	3951	rBV4	3263	3450	0.27%	0.033%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032822\
 Data File : BG052908.D
 Acq On : 29 Mar 2022 2:21
 Operator : CG/JU
 Sample : N2100-09
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0AG1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
 Title : SVOA CALIBRATION

77	26.830	3988	3990	3991	rVB2	3362	1956	0.15%	0.019%
78	26.953	4009	4011	4012	rBV2	3447	2352	0.18%	0.023%
79	27.070	4029	4031	4035	rBV4	3431	3569	0.28%	0.034%
80	27.582	4116	4118	4119	rBV2	3135	2425	0.19%	0.023%
81	27.723	4141	4142	4144	rVB2	5491	3560	0.28%	0.034%
82	27.963	4181	4183	4184	rBV2	3558	2801	0.22%	0.027%
83	28.104	4205	4207	4209	rBV3	3858	2392	0.19%	0.023%
84	28.157	4214	4216	4217	rVB2	3866	2249	0.18%	0.022%
85	28.175	4217	4219	4220	rBV	4228	2374	0.19%	0.023%
86	28.521	4277	4278	4279	rVB	5667	1998	0.16%	0.019%
87	28.645	4297	4299	4302	rBV3	3303	3587	0.28%	0.034%
88	28.909	4342	4344	4347	rBV4	3493	3163	0.25%	0.030%
89	29.168	4386	4388	4389	rBV	3548	1767	0.14%	0.017%
90	29.467	4438	4439	4441	rBV2	3223	2517	0.20%	0.024%
91	29.667	4471	4473	4474	rBV2	2844	2091	0.16%	0.020%
92	29.961	4521	4523	4526	rBV3	3498	4564	0.36%	0.044%
93	30.871	4676	4678	4679	rBV2	3367	2284	0.18%	0.022%
94	31.188	4730	4732	4735	rBV2	2781	2101	0.16%	0.020%
95	31.388	4764	4766	4769	rVB4	3651	3280	0.26%	0.031%
96	31.934	4857	4859	4860	rBV2	3858	2692	0.21%	0.026%
97	32.070	4880	4882	4886	rBV5	4500	7219	0.56%	0.069%
98	32.099	4886	4887	4889	rVV2	3381	1915	0.15%	0.018%
99	32.169	4898	4899	4902	rVB3	4052	2277	0.18%	0.022%
100	32.616	4973	4975	4977	rVB3	3531	2645	0.21%	0.025%




Sum of corrected areas: 10440484

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032822\
Data File : BG052908.D
Acq On : 29 Mar 2022 2:21
Operator : CG/JU
Sample : N2100-09
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0AG1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

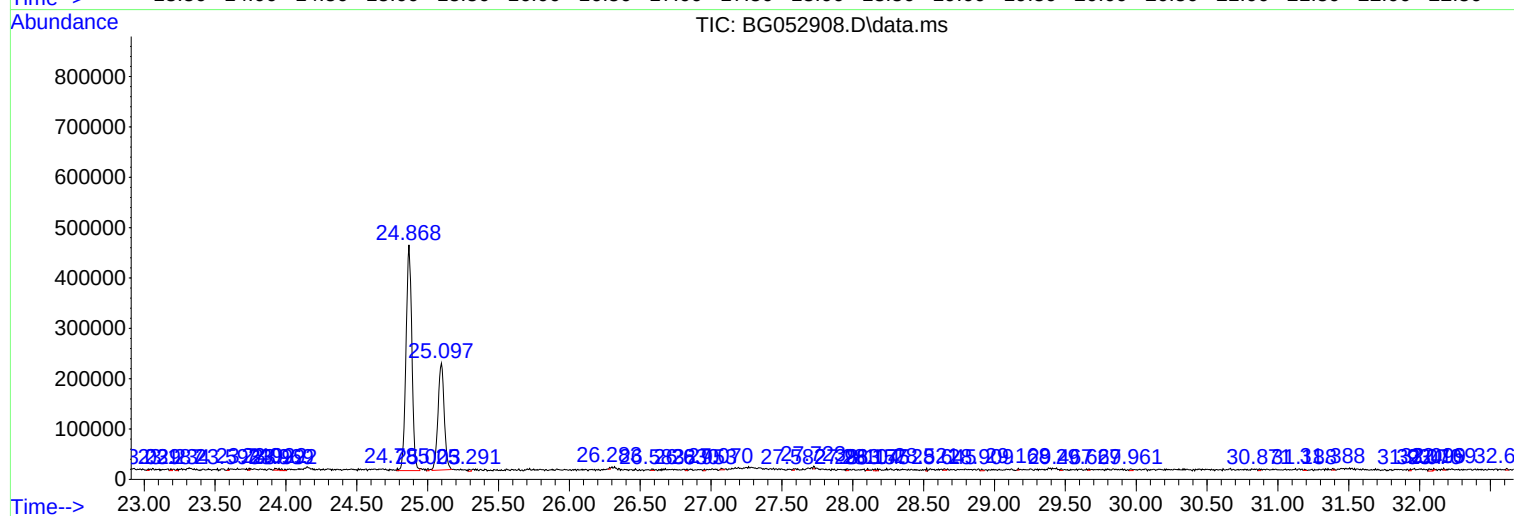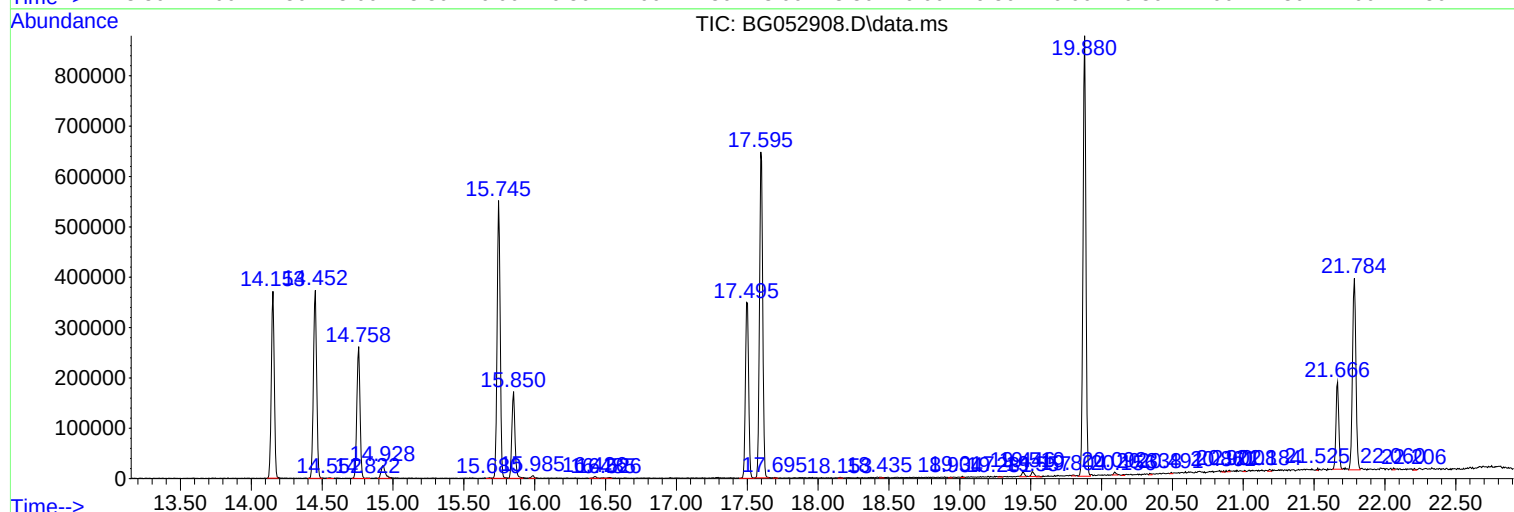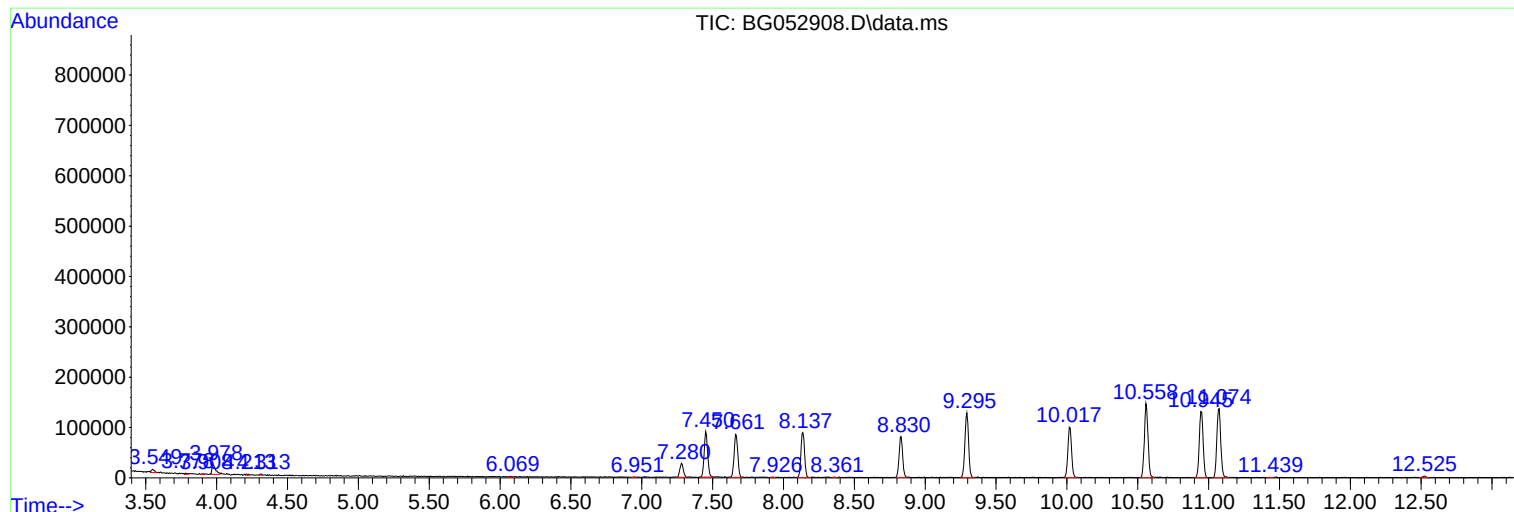

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032822\
Data File : BG052908.D
Acq On : 29 Mar 2022 2:21
Operator : CG/JU
Sample : N2100-09
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0AG1










Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Bis(2-ethylhexyl) phthalate Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
21.666	7.46 ng/ul	237820	Chrysene-d12	21.784

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Bis(2-ethylhexyl) phthalate	390	C24H38O4	000117-81-7	90
2			Phthalic acid, 2-ethylhexyl isoh...	362	C22H34O4	1000308-98-5	86
3			Bis(2-ethylhexyl) phthalate	390	C24H38O4	000117-81-7	78
4			Phthalic acid, decyl 2-ethylhexy...	418	C26H42O4	1000309-00-0	72
5			Phthalic acid, 2-ethylhexyl tetr...	474	C30H50O4	1000309-00-4	72

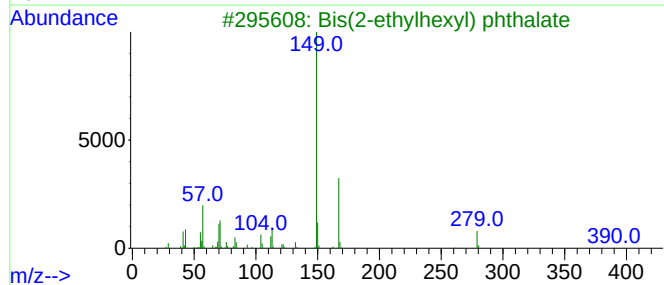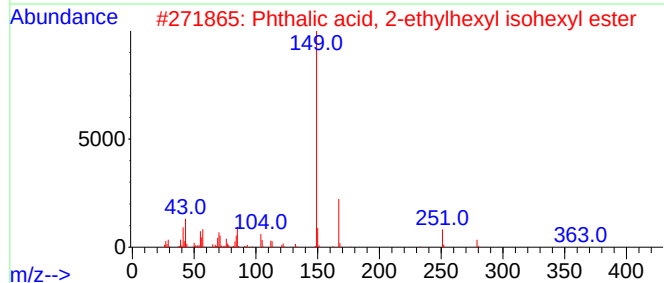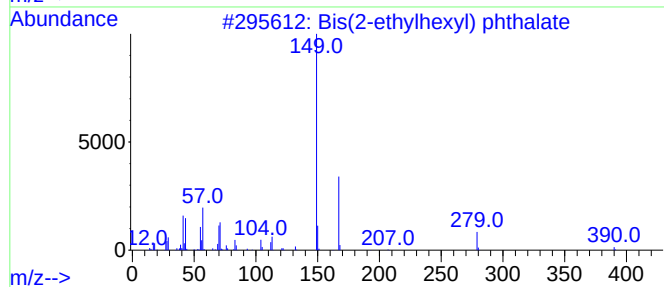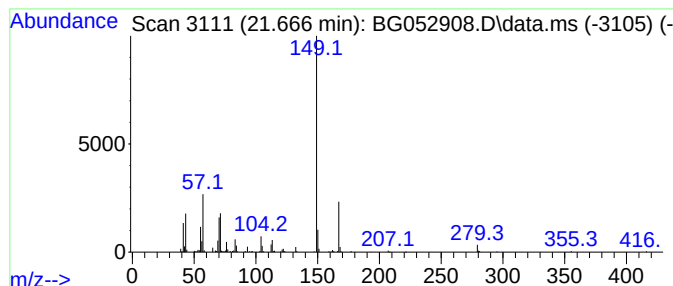

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032822\
Data File : BG052908.D
Acq On : 29 Mar 2022 2:21
Operator : CG/JU
Sample : N2100-09
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0AG1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Bis(2-ethylhexy...	21.666	7.5	ng/u1	237820	5	21.784	637527	20.0