

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032822\
 Data File : BG052932.D
 Acq On : 29 Mar 2022 18:22
 Operator : CG/JU
 Sample : N2097-15
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0AE4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
 Title : SVOA CALIBRATION

Signal : TIC: BG052932.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.546	25	27	32	rVB5	6452	8120	0.74%	0.084%
2	3.975	98	100	109	rBV2	14595	27510	2.51%	0.286%
3	4.845	244	248	253	rVB5	7563	13137	1.20%	0.136%
4	6.848	587	589	593	rBV2	1108	1522	0.14%	0.016%
5	6.965	606	609	612	rBV3	1280	1557	0.14%	0.016%
6	7.106	629	633	634	rBV2	1378	1869	0.17%	0.019%
7	7.277	657	662	671	rBV	26755	47208	4.31%	0.490%
8	7.453	685	692	701	rVB	84842	142979	13.04%	1.484%
9	7.664	721	728	737	rVB	85155	147774	13.48%	1.534%
10	7.758	737	744	747	rBV3	1314	2806	0.26%	0.029%
11	8.134	802	808	816	rBV	91637	157873	14.40%	1.639%
12	8.540	873	877	882	rBV3	911	1875	0.17%	0.019%
13	8.827	919	926	933	rBV2	79768	135507	12.36%	1.406%
14	9.291	998	1005	1013	rBV	119201	212377	19.37%	2.204%
15	9.732	1076	1080	1085	rBV2	1323	2432	0.22%	0.025%
16	10.020	1121	1129	1137	rVB	95784	171013	15.60%	1.775%
17	10.560	1213	1221	1229	rBV	138754	249749	22.78%	2.592%
18	10.948	1279	1287	1295	rBV	134138	252198	23.00%	2.618%
19	11.071	1301	1308	1315	rBV	114005	207359	18.91%	2.152%
20	12.522	1549	1555	1560	rVB2	2830	4445	0.41%	0.046%
21	13.580	1731	1735	1740	rVB2	2779	3607	0.33%	0.037%
22	14.150	1825	1832	1840	rBV	342016	494525	45.10%	5.133%
23	14.449	1876	1883	1893	rVB	344898	546064	49.80%	5.668%
24	14.643	1912	1916	1919	rBV2	1447	1801	0.16%	0.019%
25	14.755	1927	1935	1945	rBV	252520	412235	37.60%	4.279%
26	14.925	1958	1964	1971	rBV3	25358	46814	4.27%	0.486%
27	15.548	2068	2070	2074	rVB2	2865	2888	0.26%	0.030%
28	15.742	2097	2103	2112	rVB	488585	742886	67.76%	7.710%
29	15.847	2115	2121	2129	rBV	151146	234395	21.38%	2.433%
30	15.988	2139	2145	2150	rBV5	3927	7417	0.68%	0.077%
31	16.429	2217	2220	2222	rBV	1082	1506	0.14%	0.016%
32	16.523	2233	2236	2241	rVB4	1775	2679	0.24%	0.028%
33	17.498	2395	2402	2409	rBV	367286	559583	51.04%	5.808%
34	17.598	2412	2419	2431	rVB	588663	908080	82.82%	9.425%
35	18.156	2509	2514	2517	rBV2	9357	10844	0.99%	0.113%
36	18.221	2522	2525	2527	rBV2	1820	2300	0.21%	0.024%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032822\
 Data File : BG052932.D
 Acq On : 29 Mar 2022 18:22
 Operator : CG/JU
 Sample : N2097-15
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0AE4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
 Title : SVOA CALIBRATION

37	18.373	2547	2551	2559	rBV6	19235	30946	2.82%	0.321%
38	19.448	2730	2734	2738	rVB2	11166	14601	1.33%	0.152%
39	19.513	2741	2745	2749	rBV2	8523	12085	1.10%	0.125%
40	19.613	2760	2762	2764	rBV3	2265	2793	0.25%	0.029%
41	19.642	2765	2767	2772	rVB4	7130	7747	0.71%	0.080%
42	19.877	2801	2807	2814	rBV	772743	1096418	100.00%	11.380%
43	20.089	2841	2843	2846	rVB4	5329	5026	0.46%	0.052%
44	21.416	3065	3069	3079	rBV7	25546	61483	5.61%	0.638%
45	21.663	3106	3111	3120	rVB	204301	274454	25.03%	2.849%
46	21.780	3125	3131	3139	rVB2	378140	620439	56.59%	6.440%
47	24.864	3645	3656	3669	rBV	376737	1093302	99.72%	11.347%
48	25.088	3684	3694	3708	rBV2	213670	648594	59.16%	6.732%




Sum of corrected areas: 9634822

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032822\
Data File : BG052932.D
Acq On : 29 Mar 2022 18:22
Operator : CG/JU
Sample : N2097-15
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0AE4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

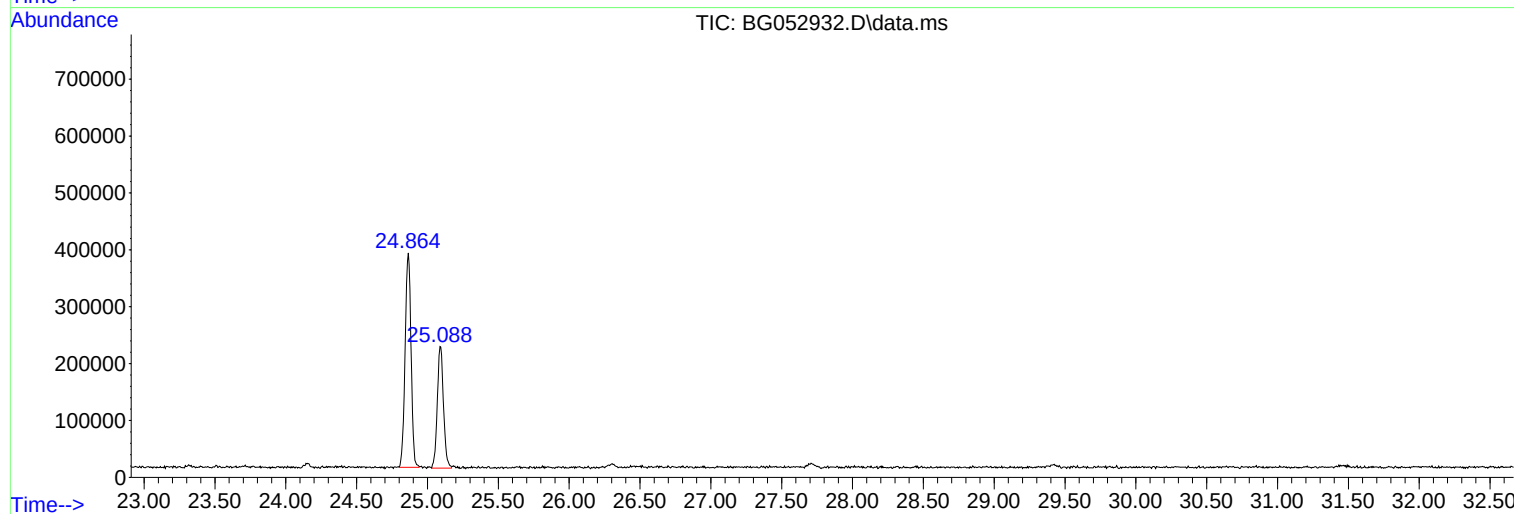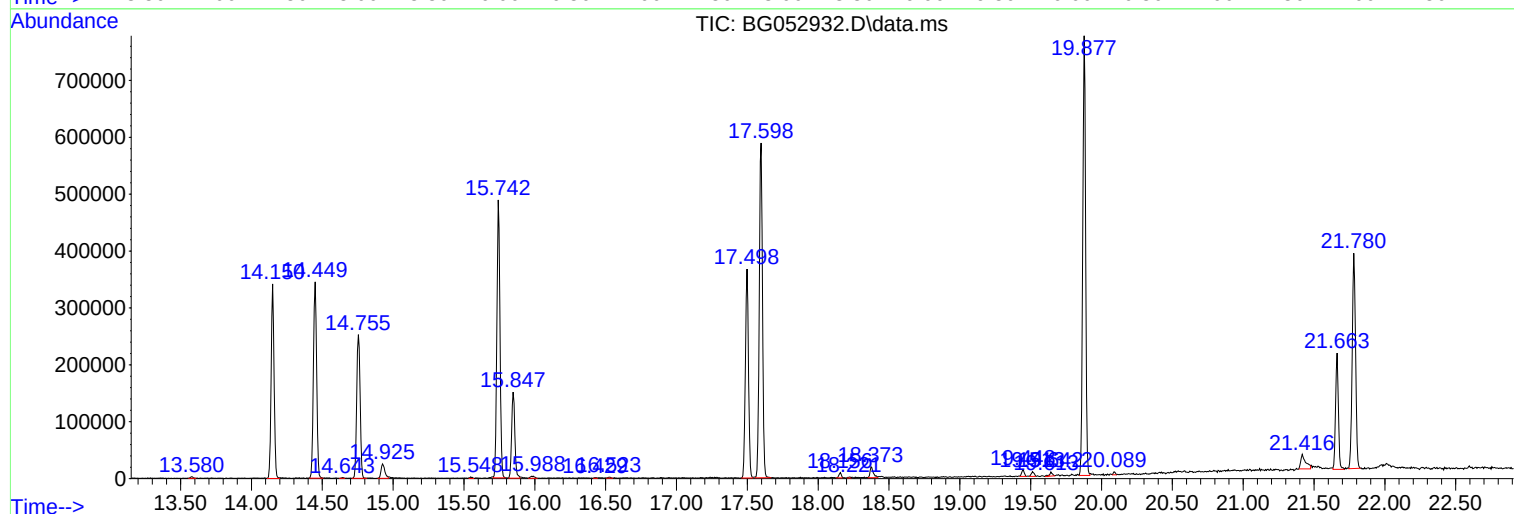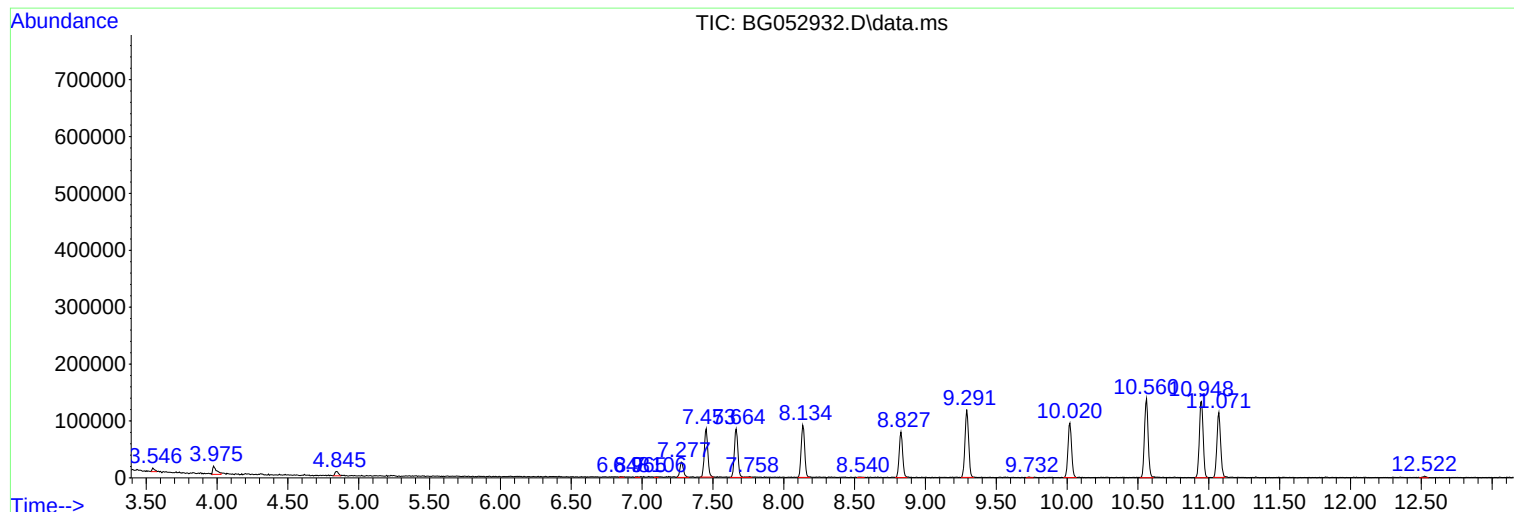

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032822\
Data File : BG052932.D
Acq On : 29 Mar 2022 18:22
Operator : CG/JU
Sample : N2097-15
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0AE4










Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Bis(2-ethylhexyl) phthalate Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
21.663	8.85 ng/ul	274454	Chrysene-d12	21.780

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Bis(2-ethylhexyl) phthalate	390	C24H38O4	000117-81-7	86
2			Phthalic acid, 2-ethylhexyl isoh...	362	C22H34O4	1000308-98-5	72
3			Phthalic acid, isohexyl 2-methyl...	334	C20H30O4	1000356-91-0	52
4			Phthalic acid, cyclohexyl 2-pent...	318	C19H26O4	1000315-55-3	52
5			Phthalic acid, di(hex-3-yl) ester	334	C20H30O4	1000356-96-7	50

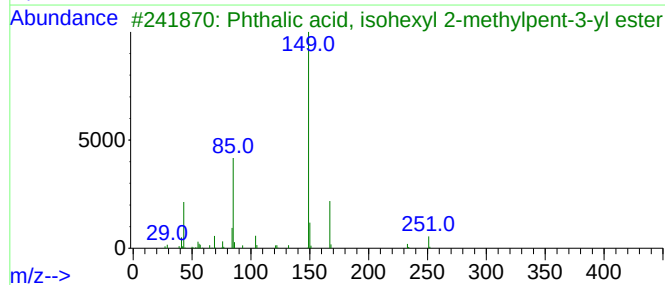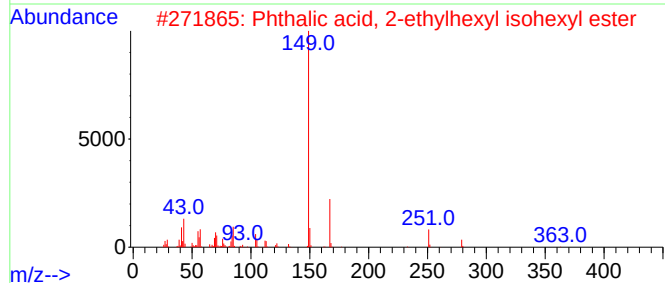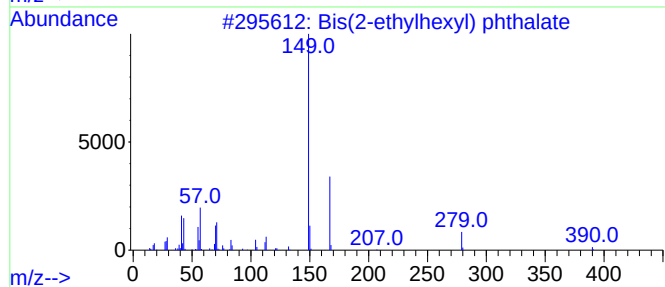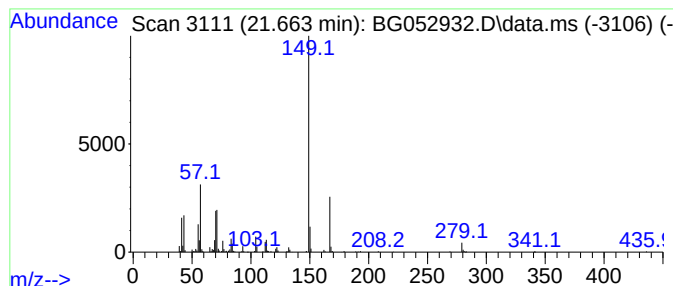

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032822\
Data File : BG052932.D
Acq On : 29 Mar 2022 18:22
Operator : CG/JU
Sample : N2097-15
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0AE4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Bis(2-ethylhexy...	21.663	8.8	ng/ul	274454	5	21.780	620439	20.0