

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032822\
 Data File : BG052937.D
 Acq On : 29 Mar 2022 21:35
 Operator : CG/JU
 Sample : N2097-19
 Misc :
 ALS Vial : 56 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0AE9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
 Title : SVOA CALIBRATION

Signal : TIC: BG052937.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.552	24	28	31	rBV4	5181	6865	0.57%	0.069%
2	3.969	97	99	106	rBV	22052	36865	3.04%	0.370%
3	7.277	656	662	669	rBV	30062	52257	4.30%	0.524%
4	7.447	684	691	704	rBV	90859	160175	13.19%	1.607%
5	7.664	721	728	738	rVB	93494	162143	13.35%	1.627%
6	8.134	801	808	815	rBV	94006	158598	13.06%	1.591%
7	8.399	852	853	858	rVB2	1801	1737	0.14%	0.017%
8	8.821	918	925	938	rBV	83467	152575	12.56%	1.531%
9	9.291	998	1005	1013	rBV	133204	233268	19.21%	2.341%
10	10.014	1122	1128	1136	rVB	101257	186328	15.34%	1.870%
11	10.560	1212	1221	1229	rBV	146264	266792	21.97%	2.677%
12	10.948	1279	1287	1297	rVB	136282	256128	21.09%	2.570%
13	11.071	1300	1308	1316	rVV	144093	264008	21.74%	2.649%
14	11.594	1395	1397	1400	rBV3	1333	1645	0.14%	0.017%
15	12.364	1523	1528	1529	rVB2	1607	2344	0.19%	0.024%
16	12.522	1550	1555	1561	rVB3	3334	5053	0.42%	0.051%
17	13.580	1730	1735	1738	rVB2	2773	3172	0.26%	0.032%
18	13.768	1765	1767	1772	rVB2	1594	2260	0.19%	0.023%
19	14.150	1825	1832	1839	rBV	363306	528361	43.50%	5.302%
20	14.449	1876	1883	1892	rVV	376583	590204	48.60%	5.923%
21	14.520	1892	1895	1899	rVB3	1692	2306	0.19%	0.023%
22	14.755	1926	1935	1943	rVB	260938	418519	34.46%	4.200%
23	14.925	1959	1964	1970	rBV2	27276	52381	4.31%	0.526%
24	15.742	2096	2103	2115	rBV	513143	815261	67.13%	8.181%
25	15.847	2115	2121	2129	rBV2	161335	244031	20.09%	2.449%
26	15.982	2140	2144	2149	rVB6	5293	9579	0.79%	0.096%
27	16.423	2218	2219	2222	rVB3	1821	1786	0.15%	0.018%
28	16.476	2226	2228	2233	rVV4	2106	3011	0.25%	0.030%
29	16.535	2233	2238	2240	rVV3	1305	1975	0.16%	0.020%
30	16.958	2307	2310	2313	rBV2	1275	1696	0.14%	0.017%
31	17.122	2336	2338	2343	rVB4	1409	1835	0.15%	0.018%
32	17.181	2346	2348	2351	rVB3	2164	1931	0.16%	0.019%
33	17.240	2354	2358	2360	rBV3	1620	2181	0.18%	0.022%
34	17.292	2364	2367	2375	rVV5	3081	6324	0.52%	0.063%
35	17.357	2375	2378	2382	rVB3	1284	1954	0.16%	0.020%
36	17.498	2394	2402	2409	rBV	356225	559528	46.07%	5.615%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032822\
 Data File : BG052937.D
 Acq On : 29 Mar 2022 21:35
 Operator : CG/JU
 Sample : N2097-19
 Misc :
 ALS Vial : 56 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0AE9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
 Title : SVOA CALIBRATION

37	17.598	2412	2419	2426	rVV	619286	976041	80.36%	9.794%
38	17.674	2429	2432	2437	rVB4	4474	7016	0.58%	0.070%
39	17.939	2476	2477	2480	rBV3	2361	2401	0.20%	0.024%
40	18.174	2516	2517	2520	rBV2	1951	1736	0.14%	0.017%
41	18.268	2531	2533	2535	rBV3	1500	1682	0.14%	0.017%
42	18.379	2549	2552	2554	rBV3	2424	2635	0.22%	0.026%
43	18.567	2582	2584	2589	rVB4	1959	2207	0.18%	0.022%
44	18.685	2602	2604	2605	rBV2	2231	1845	0.15%	0.019%
45	18.849	2627	2632	2633	rBV3	1900	2965	0.24%	0.030%
46	18.937	2646	2647	2650	rBV2	1699	1595	0.13%	0.016%
47	19.260	2700	2702	2705	rBV2	1795	1940	0.16%	0.019%
48	19.290	2705	2707	2710	rVB3	2206	1989	0.16%	0.020%
49	19.366	2716	2720	2722	rBV2	1889	2212	0.18%	0.022%
50	19.442	2730	2733	2737	rVB4	9080	10950	0.90%	0.110%
51	19.513	2739	2745	2749	rBV3	9925	15962	1.31%	0.160%
52	19.666	2769	2771	2774	rBV5	3395	1881	0.15%	0.019%
53	19.877	2801	2807	2814	rBV	819190	1176917	96.90%	11.810%
54	21.410	3064	3068	3076	rBV9	14554	30910	2.55%	0.310%
55	21.780	3125	3131	3139	rVB	380565	643412	52.98%	6.456%
56	22.808	3305	3306	3309	rBV3	5454	4444	0.37%	0.045%
57	24.859	3645	3655	3671	rVB3	412631	1214535	100.00%	12.188%
58	25.088	3684	3694	3710	rVB3	213191	664987	54.75%	6.673%




Sum of corrected areas: 9965338

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032822\
Data File : BG052937.D
Acq On : 29 Mar 2022 21:35
Operator : CG/JU
Sample : N2097-19
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0AE9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

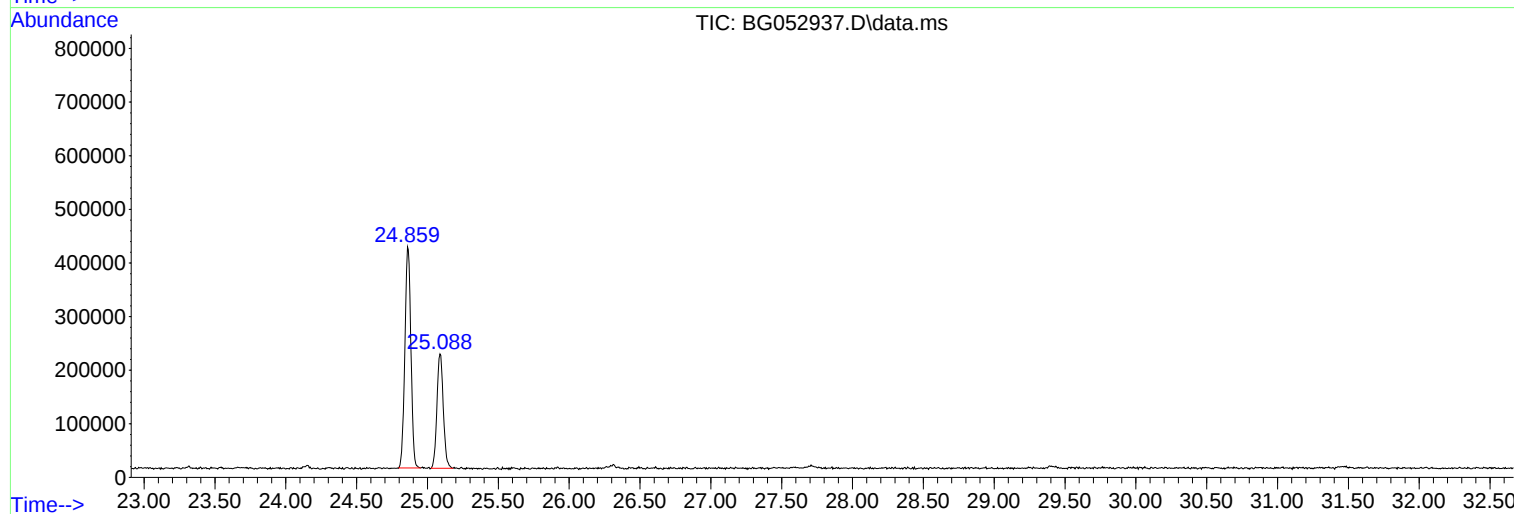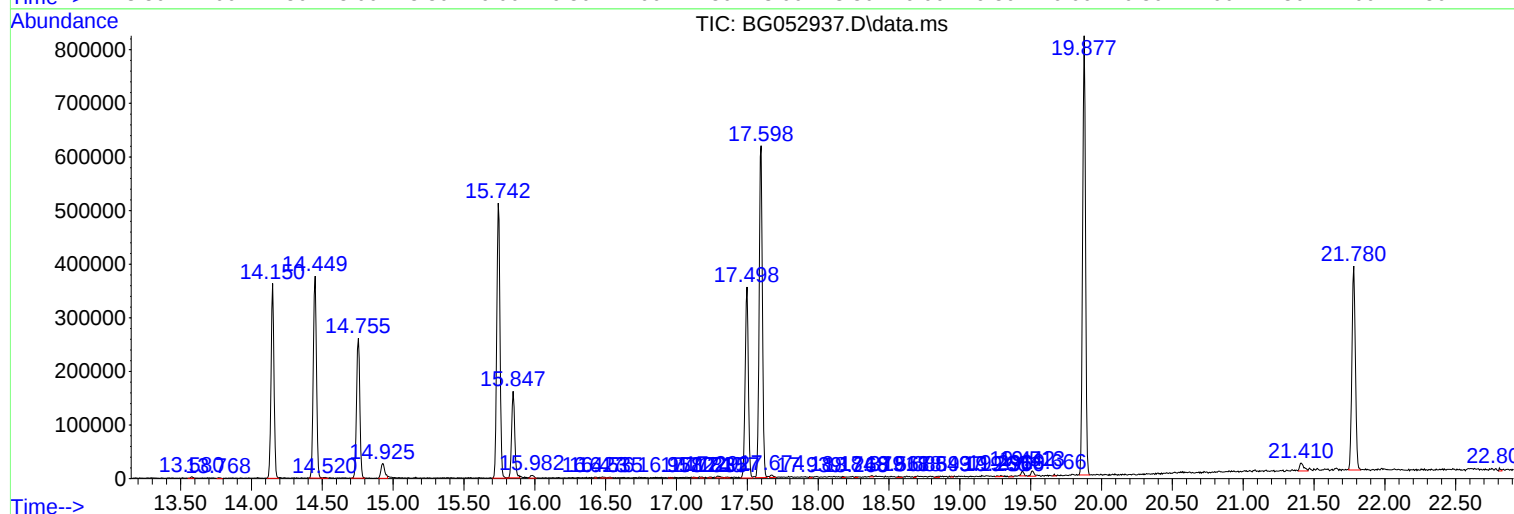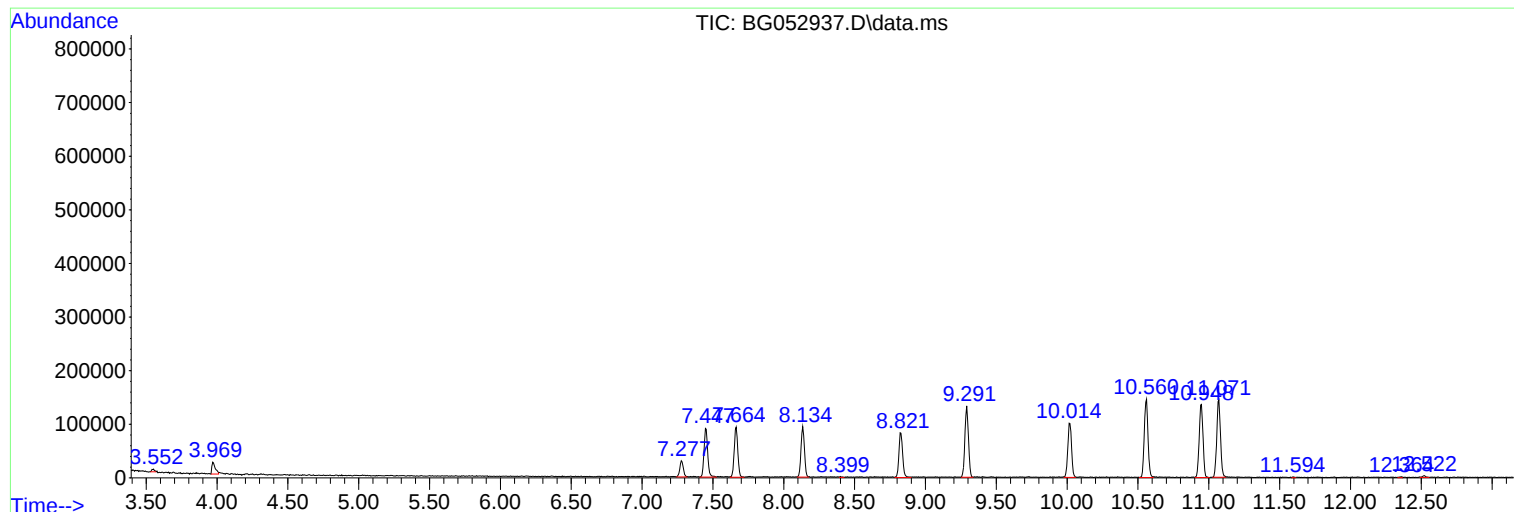

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032822\
Data File : BG052937.D
Acq On : 29 Mar 2022 21:35
Operator : CG/JU
Sample : N2097-19
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0AE9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032822\
Data File : BG052937.D
Acq On : 29 Mar 2022 21:35
Operator : CG/JU
Sample : N2097-19
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0AE9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
