

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032822\
 Data File : BG052939.D
 Acq On : 29 Mar 2022 22:52
 Operator : CG/JU
 Sample : N2097-17
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0AE7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
 Title : SVOA CALIBRATION

Signal : TIC: BG052939.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.969	97	99	112	rBV	21751	37244	3.33%	0.402%
2	7.277	657	662	670	rBV	25982	44410	3.97%	0.479%
3	7.447	685	691	700	rBV	80362	140811	12.58%	1.519%
4	7.564	707	711	712	rBV2	1581	1582	0.14%	0.017%
5	7.664	721	728	736	rVB	81924	144601	12.92%	1.560%
6	8.134	801	808	815	rVB	91062	154506	13.80%	1.667%
7	8.193	815	818	821	rBV2	1587	1930	0.17%	0.021%
8	8.827	919	926	933	rVB3	72220	127990	11.43%	1.381%
9	9.292	997	1005	1014	rVB	119298	212233	18.96%	2.290%
10	9.726	1074	1079	1083	rVB3	2087	3496	0.31%	0.038%
11	10.020	1121	1129	1135	rBV	93373	164525	14.70%	1.775%
12	10.372	1184	1189	1191	rBV3	1424	1918	0.17%	0.021%
13	10.419	1191	1197	1201	rVB3	1824	3470	0.31%	0.037%
14	10.555	1214	1220	1230	rVB	133594	244370	21.83%	2.636%
15	10.942	1279	1286	1295	rVB	136578	250809	22.40%	2.706%
16	11.071	1299	1308	1320	rBV	127388	237021	21.17%	2.557%
17	12.517	1548	1554	1563	rBV4	2838	6049	0.54%	0.065%
18	13.157	1661	1663	1666	rVB2	1627	1562	0.14%	0.017%
19	13.580	1730	1735	1739	rBV2	6537	8100	0.72%	0.087%
20	14.150	1825	1832	1843	rBV	331986	487179	43.52%	5.256%
21	14.279	1851	1854	1857	rVB3	2044	1986	0.18%	0.021%
22	14.449	1876	1883	1890	rBV	346412	545212	48.70%	5.882%
23	14.643	1913	1916	1920	rVB3	1761	2519	0.23%	0.027%
24	14.755	1928	1935	1942	rVB	251281	404492	36.13%	4.364%
25	14.925	1959	1964	1972	rBV2	23133	44428	3.97%	0.479%
26	15.054	1980	1986	1988	rVB2	991	1688	0.15%	0.018%
27	15.477	2053	2058	2061	rBV3	1989	2394	0.21%	0.026%
28	15.554	2067	2071	2075	rVB2	2382	2813	0.25%	0.030%
29	15.742	2094	2103	2110	rBV	489417	737630	65.89%	7.958%
30	15.847	2115	2121	2130	rBV	149221	224100	20.02%	2.418%
31	15.982	2140	2144	2148	rVB3	4304	5960	0.53%	0.064%
32	16.423	2216	2219	2221	rBV2	1870	1785	0.16%	0.019%
33	16.676	2258	2262	2266	rBV2	1092	1561	0.14%	0.017%
34	17.281	2362	2365	2368	rBV3	1496	1894	0.17%	0.020%
35	17.498	2395	2402	2409	rBV	357031	545541	48.73%	5.885%
36	17.598	2412	2419	2427	rVV	578103	906888	81.01%	9.784%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032822\
 Data File : BG052939.D
 Acq On : 29 Mar 2022 22:52
 Operator : CG/JU
 Sample : N2097-17
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0AE7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
 Title : SVOA CALIBRATION

37	17.657	2427	2429	2434	rVB4	989	1482	0.13%	0.016%
38	18.150	2510	2513	2516	rBV2	1375	1524	0.14%	0.016%
39	18.373	2549	2551	2555	rBV5	5231	6555	0.59%	0.071%
40	18.955	2648	2650	2652	rBV3	1813	2057	0.18%	0.022%
41	19.102	2671	2675	2677	rBV3	1030	1521	0.14%	0.016%
42	19.266	2701	2703	2706	rVB4	1767	1862	0.17%	0.020%
43	19.442	2729	2733	2738	rBV4	7850	11688	1.04%	0.126%
44	19.513	2742	2745	2751	rVB4	9058	12566	1.12%	0.136%
45	19.607	2760	2761	2764	rBV2	2293	1641	0.15%	0.018%
46	19.648	2764	2768	2771	rBV4	2892	4937	0.44%	0.053%
47	19.877	2801	2807	2814	rBV	758545	1099213	98.19%	11.858%
48	20.012	2828	2830	2833	rBV4	1831	1956	0.17%	0.021%
49	20.042	2833	2835	2837	rBV3	2529	2084	0.19%	0.022%
50	20.247	2868	2870	2873	rBV4	1894	1755	0.16%	0.019%
51	20.488	2910	2911	2914	rBV3	3092	2834	0.25%	0.031%
52	21.410	3065	3068	3072	rBV4	11760	17083	1.53%	0.184%
53	21.781	3124	3131	3141	rVB	389188	637423	56.94%	6.877%
54	23.308	3389	3391	3397	rBV5	6608	10612	0.95%	0.114%
55	24.865	3644	3656	3666	rBV2	385647	1119482	100.00%	12.077%
56	25.088	3685	3694	3706	rVB2	213553	626502	55.96%	6.759%




Sum of corrected areas: 9269474

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032822\
Data File : BG052939.D
Acq On : 29 Mar 2022 22:52
Operator : CG/JU
Sample : N2097-17
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0AE7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

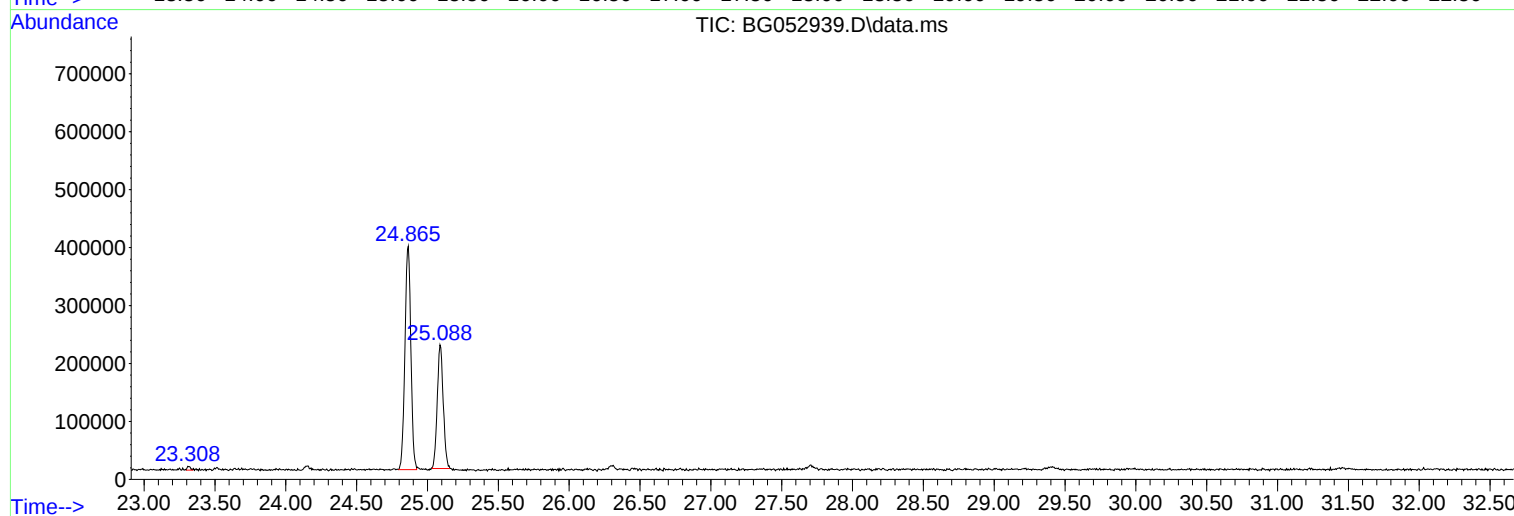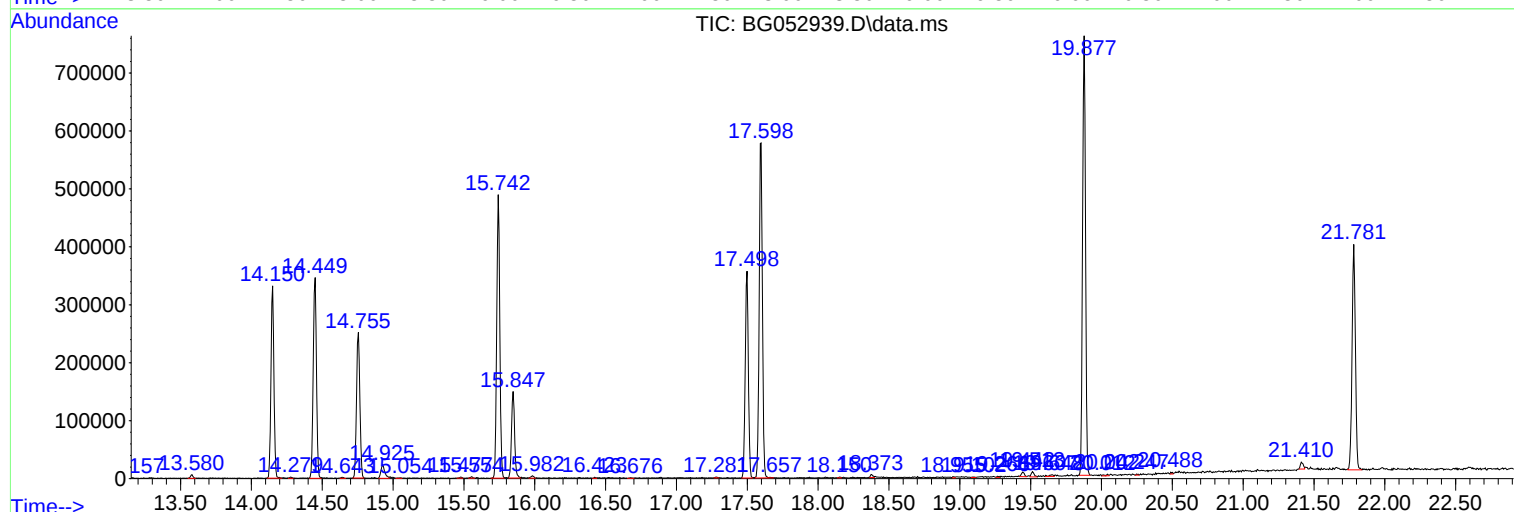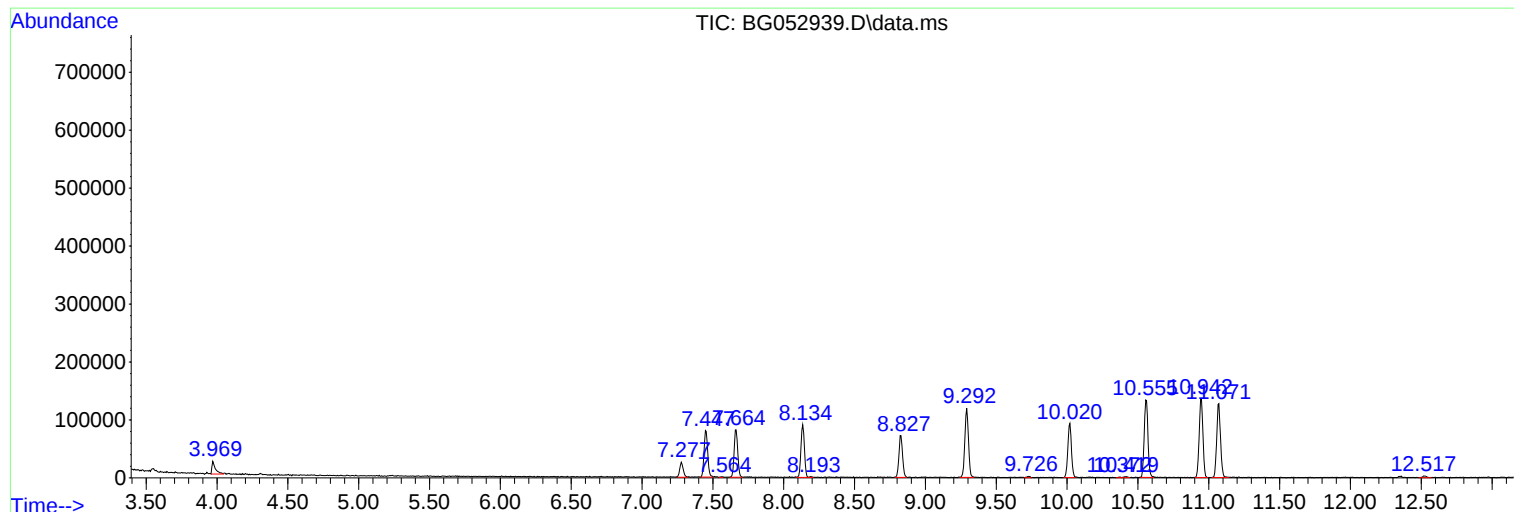

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032822\
Data File : BG052939.D
Acq On : 29 Mar 2022 22:52
Operator : CG/JU
Sample : N2097-17
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0AE7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032822\
Data File : BG052939.D
Acq On : 29 Mar 2022 22:52
Operator : CG/JU
Sample : N2097-17
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0AE7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc