

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG032916\
 Data File : BG021549.D
 Acq On : 29 Mar 2016 11:54
 Operator : UM/SJ
 Sample : H1910-20
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0AG7

Quant Time: Mar 30 01:13:05 2016
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG031616.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Mar 30 01:11:49 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.05	152	7880	20.00	ng/ul	0.00
18) Naphthalene-d8	10.86	136	39769	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.67	164	25507	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.41	188	67403	20.00	ng/ul	0.00
78) Chrysene-d12	21.66	240	78210	20.00	ng/ul	0.00
86) Perylene-d12	24.87	264	72003	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	0.00	96	0	0.00	ng/uL	
5) Phenol-d5	7.34	99	3535	4.75	ng/ul	0.02
7) Bis-(2-Chloroethyl)ether-d	7.37	67	14432	32.70	ng/ul	0.00
9) 2-Chlorophenol-d4	7.63	132	15138	26.76	ng/ul	0.00
13) 4-Methylphenol-d8	8.84	113	9411	14.75	ng/ul	0.00
19) Nitrobenzene-d5	9.22	128	9892	33.15	ng/ul	0.00
22) 2-Nitrophenol-d4	9.94	143	11184	32.79	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.56	165	18550	30.43	ng/ul	0.00
29) 4-Chloroaniline-d4	0.00	131	0	0.00	ng/ul	
44) Dimethylphthalate-d6	14.07	166	78724	37.07	ng/ul	0.00
47) Acenaphthylene-d8	14.36	160	92925	35.50	ng/ul	0.00
52) 4-Nitrophenol-d4	15.11	143	1492	4.39	ng/ul	0.02
58) Fluorene-d10	15.66	176	71065	37.11	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.79	200	13861	31.13	ng/ul	0.00
71) Anthracene-d10	17.51	188	116846	35.38	ng/ul	0.00
79) Pyrene-d10	19.79	212	141017	38.67	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.65	264	135267	40.70	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
45) Dimethylphthalate	14.12	163	2972	1.35	ng/ul#	90




(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG032916\
Data File : BG021549.D
Acq On : 29 Mar 2016 11:54
Operator : UM/SJ
Sample : H1910-20
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0AG7

Quant Time: Mar 30 01:13:05 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG031616.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Mar 30 01:11:49 2016
Response via : Initial Calibration

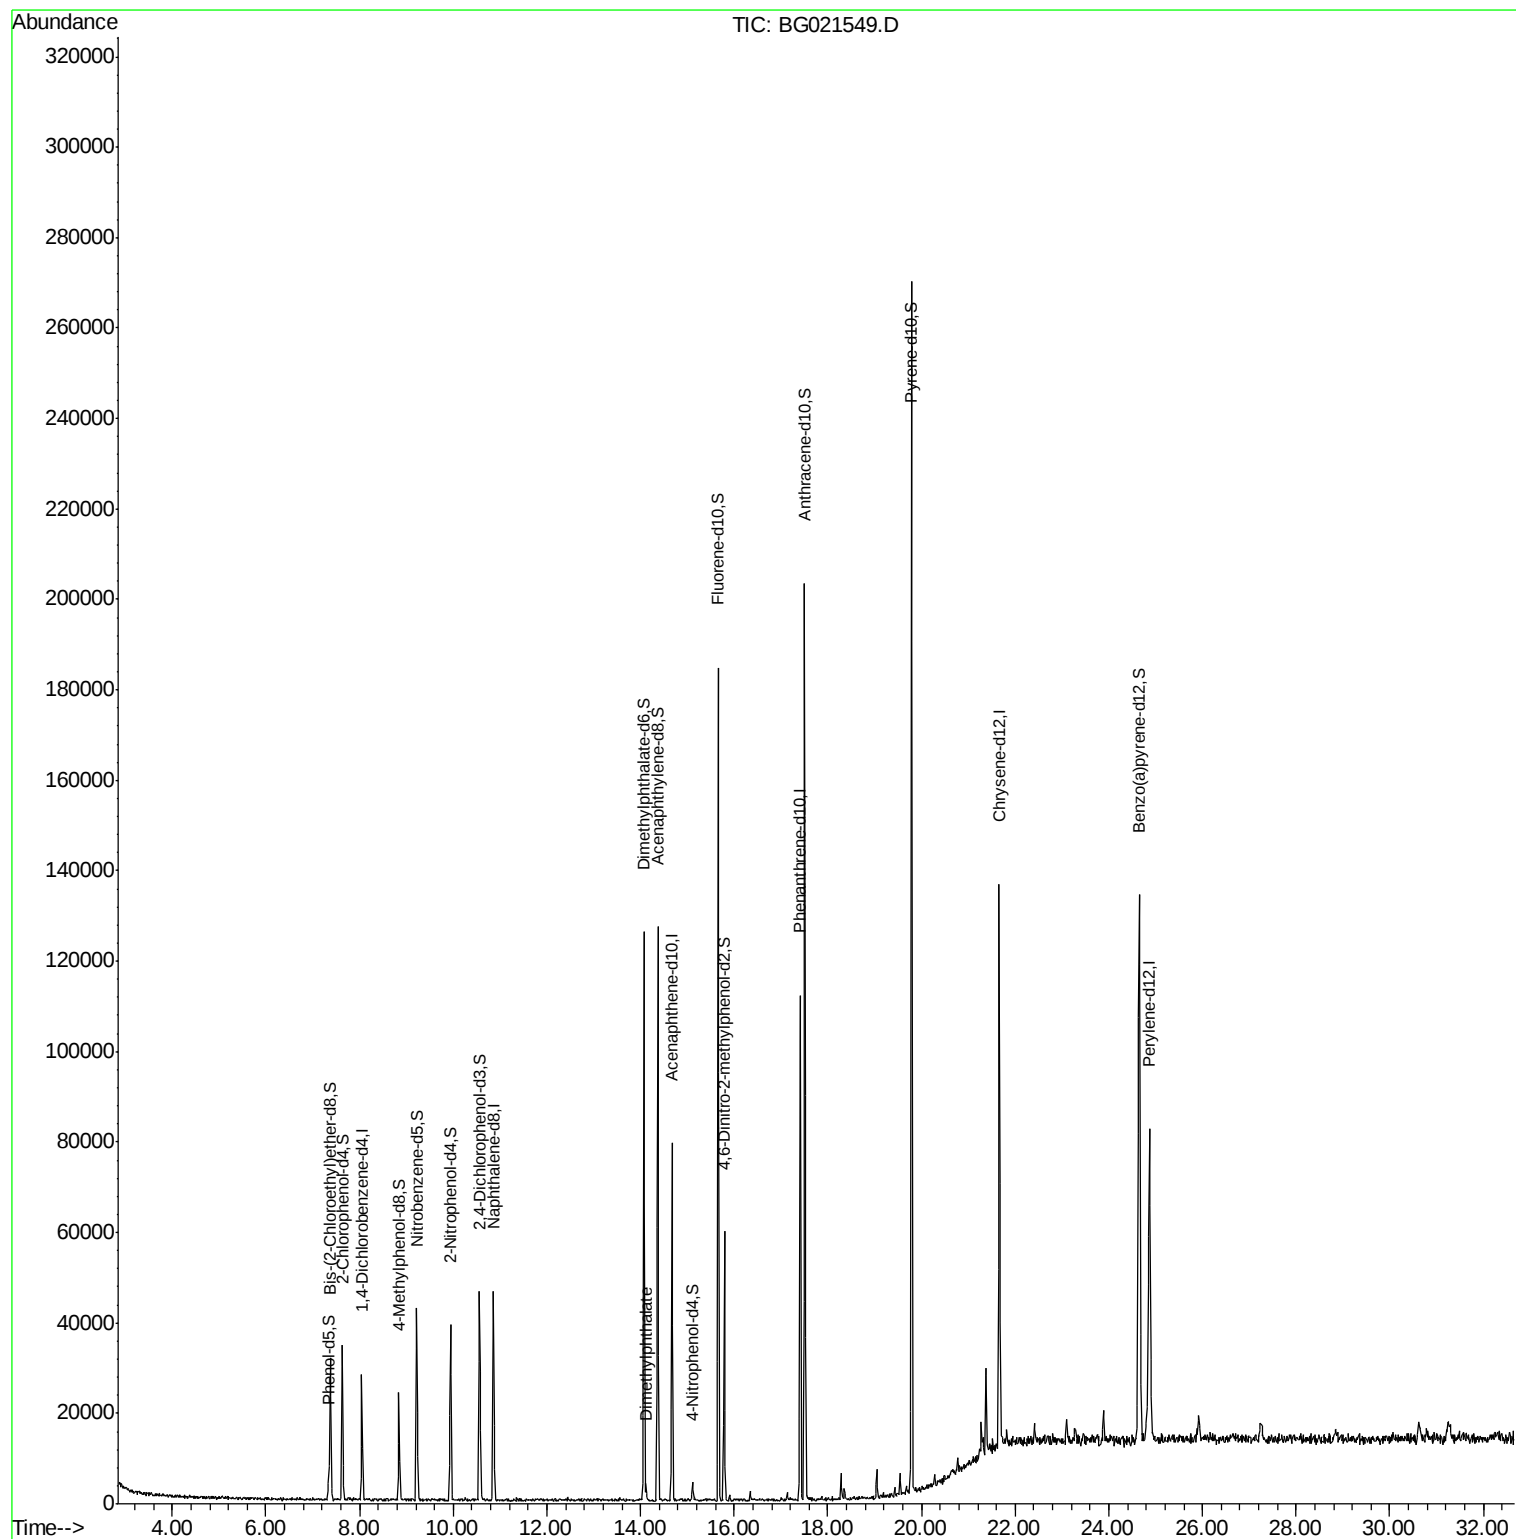

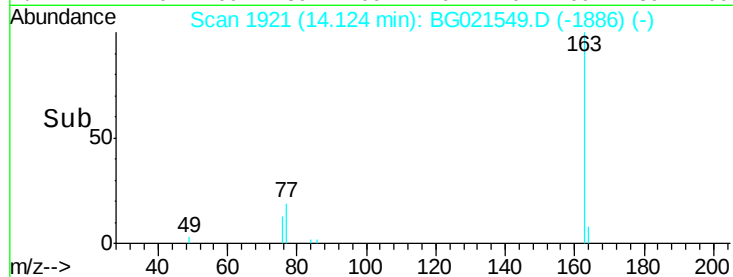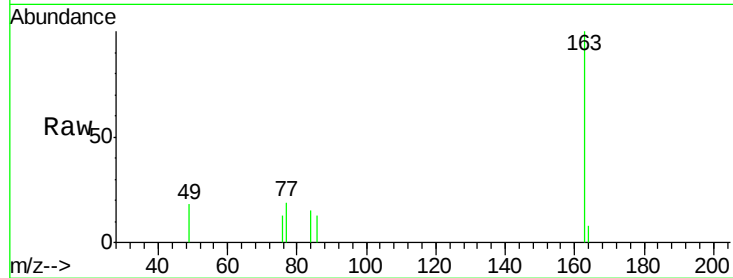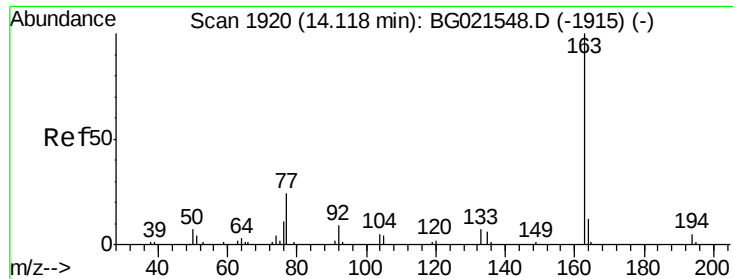

#45

Dimethylphthalate

Concen: 1.35 ng/ul

RT: 14.12 min Scan# 1921

Delta R.T. 0.01 min

Lab File: BG021549.D

Acq: 29 Mar 2016 11:54

Instrument :

BNA_G

ClientSampleId :

C0AG7

Tgt Ion:163 Resp: 2972

Ion Ratio Lower Upper

163 100

194 0.0 3.9 5.9#

164 7.9 8.7 13.1#

