

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG032916\
 Data File : BG021560.D
 Acq On : 29 Mar 2016 20:16
 Operator : UM/SJ
 Sample : H1935-09
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0AF9

Quant Time: Mar 30 01:36:44 2016
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG031616.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Mar 30 01:34:35 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.05	152	11531	20.00	ng/ul	0.00
18) Naphthalene-d8	10.85	136	48532	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.67	164	31411	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.41	188	81418	20.00	ng/ul	0.00
78) Chrysene-d12	21.67	240	93122	20.00	ng/ul	0.00
86) Perylene-d12	24.87	264	91449	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	0.00	96	0	0.00	ng/uL	
5) Phenol-d5	7.34	99	2124	1.95	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.38	67	13314	20.62	ng/ul	0.00
9) 2-Chlorophenol-d4	7.63	132	14241	17.20	ng/ul	0.00
13) 4-Methylphenol-d8	8.84	113	8457	9.06	ng/ul	0.00
19) Nitrobenzene-d5	9.22	128	9313	25.58	ng/ul	0.00
22) 2-Nitrophenol-d4	9.94	143	10004	24.04	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.57	165	16018	21.53	ng/ul	0.00
29) 4-Chloroaniline-d4	11.02	131	349	0.36	ng/ul	0.01
44) Dimethylphthalate-d6	14.07	166	66060	25.26	ng/ul	0.00
47) Acenaphthylene-d8	14.37	160	77887	24.16	ng/ul	0.00
52) 4-Nitrophenol-d4	15.11	143	1037	2.48	ng/ul	0.02
58) Fluorene-d10	15.66	176	60613	25.70	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.78	200	11115	20.66	ng/ul	0.00
71) Anthracene-d10	17.51	188	105414	26.42	ng/ul	0.00
79) Pyrene-d10	19.78	212	123549	28.45	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.65	264	123409	29.24	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
84) Bis(2-ethylhexyl)phthalate	21.52	149	3569	1.04	ng/ul#	74


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG032916\
Data File : BG021560.D
Acq On : 29 Mar 2016 20:16
Operator : UM/SJ
Sample : H1935-09
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0AF9

Quant Time: Mar 30 01:36:44 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG031616.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Mar 30 01:34:35 2016
Response via : Initial Calibration

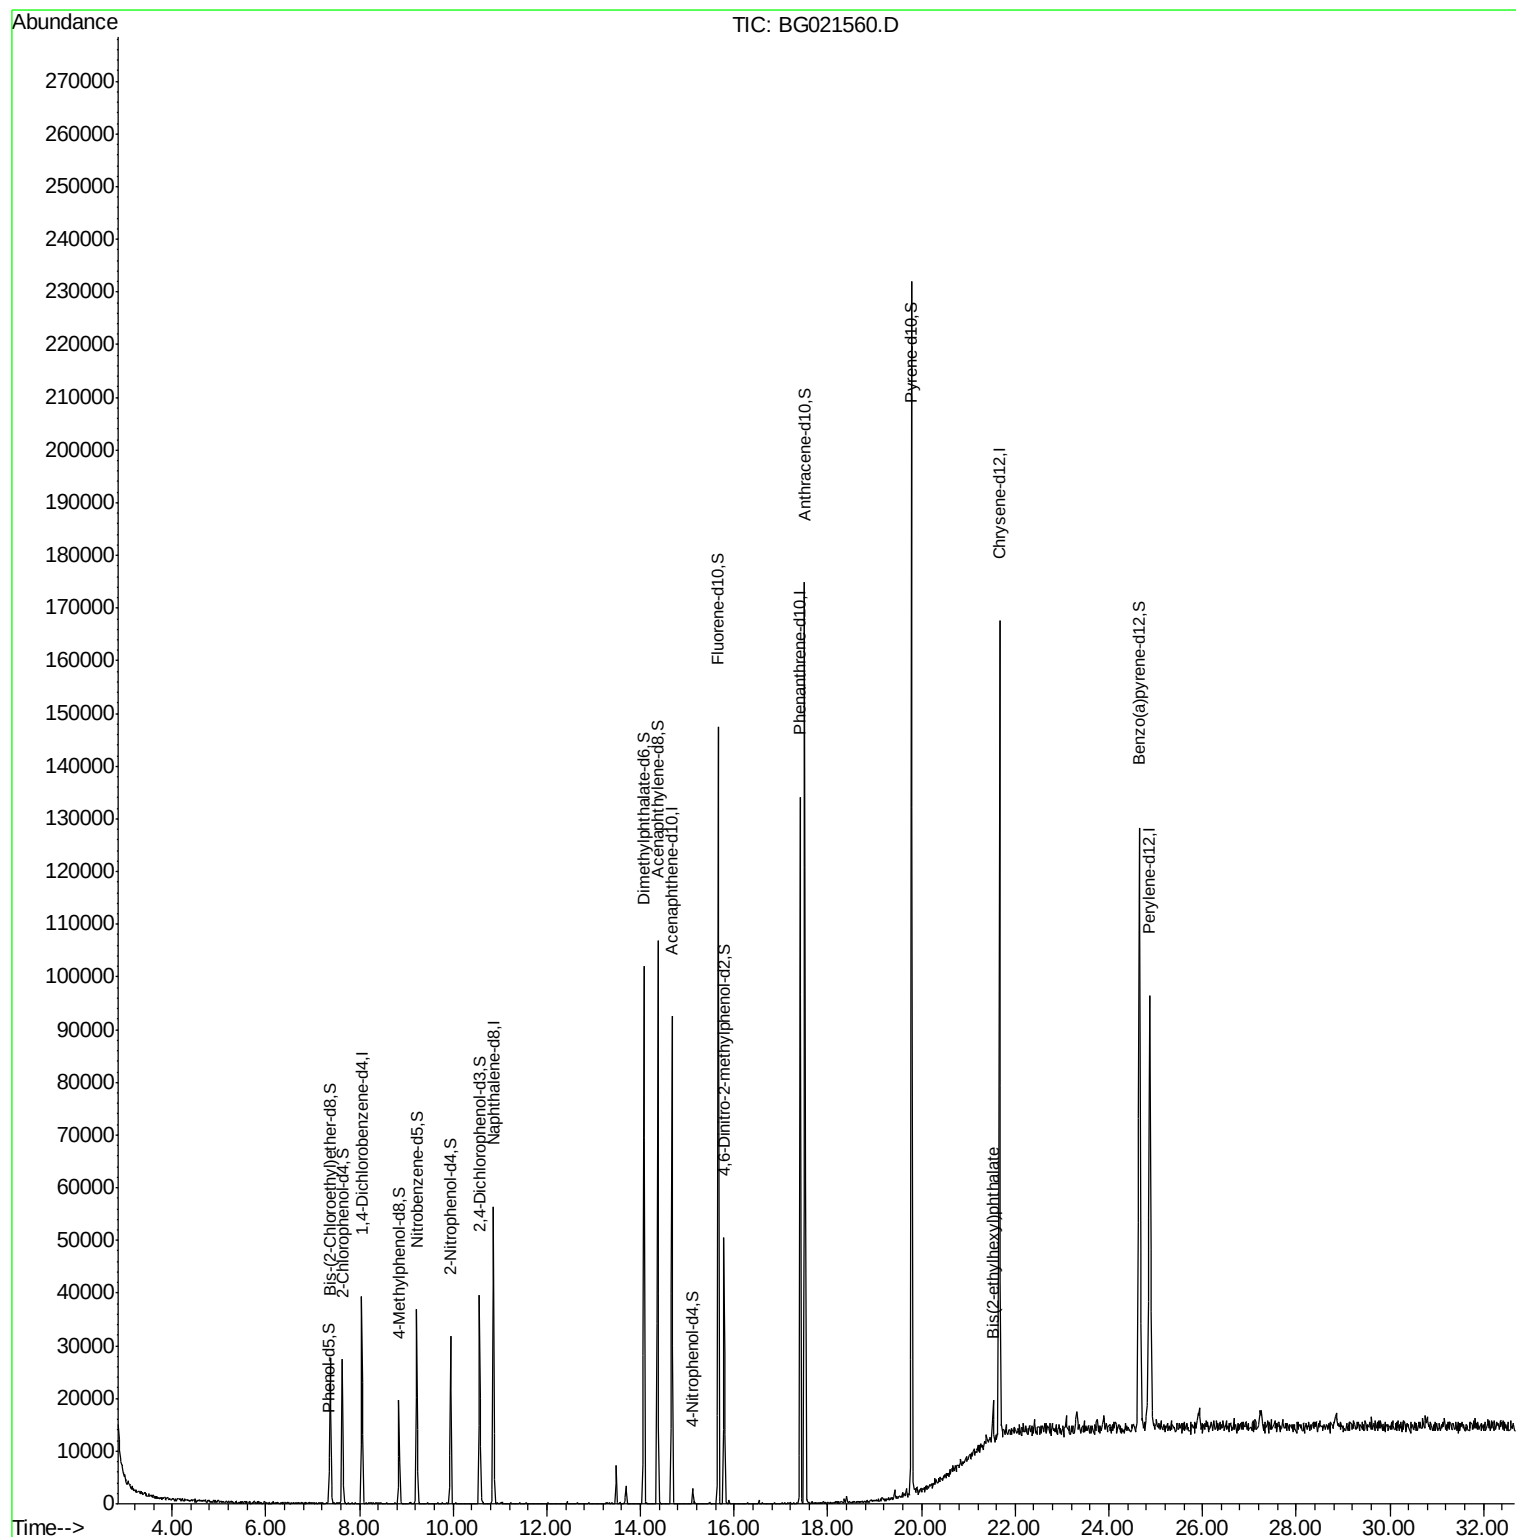

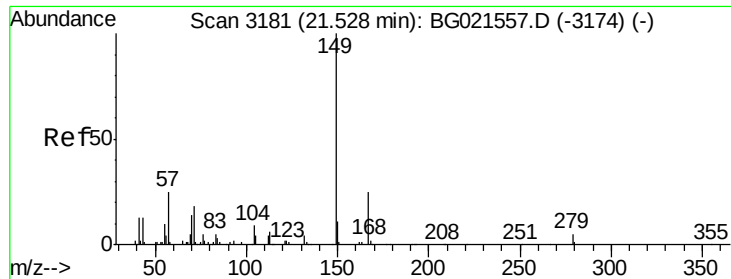

#84
 Bis(2-ethylhexyl)phthalate
 Concen: 1.04 ng/ul
 RT: 21.52 min Scan# 3180
 Delta R.T. -0.00 min
 Lab File: BG021560.D
 Acq: 29 Mar 2016 20:16

Instrument :
 BNA_G
 ClientSampleId :
 C0AF9

Tgt Ion:149 Resp: 3569
 Ion Ratio Lower Upper
 149 100
 167 39.7 20.5 30.7#
 279 0.0 3.7 5.5#

